




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040522\
Data File : VV025349.D
Acq On : 05 Apr 2022 11:58
Operator : SY/MD
Sample : VV0405WBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK334

Manual IntegrationsAPPROVED

Quant Time: Apr 06 01:29:05 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Apr 06 01:28:15 2022
Response via : Initial Calibration

Reviewed By :John Carlone 04/06/2022
Supervised By :Mahesh Dadoda 04/06/2022

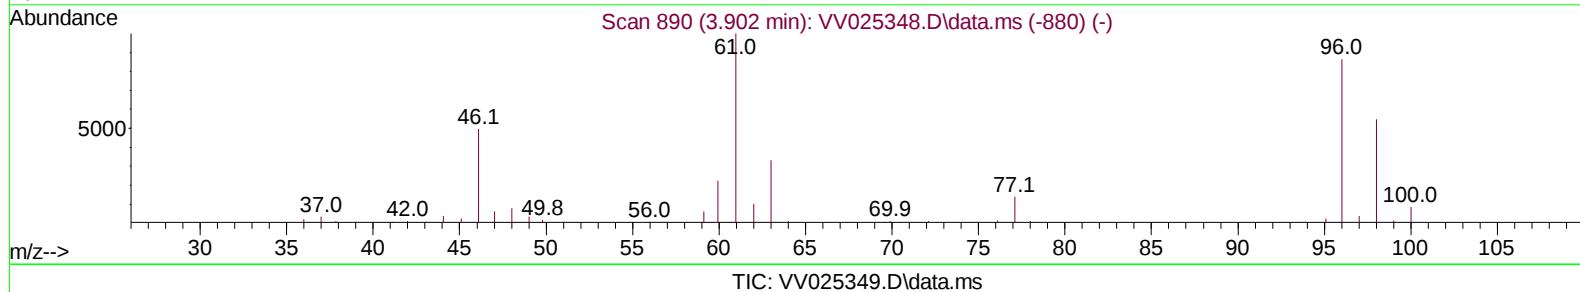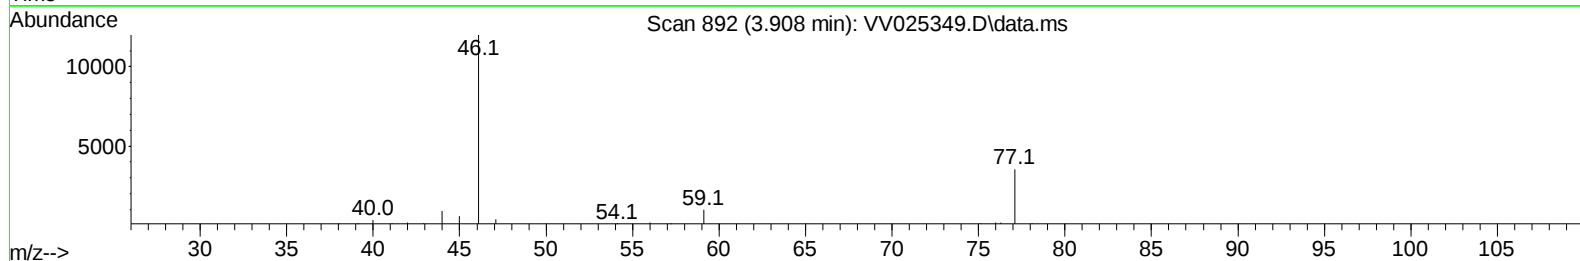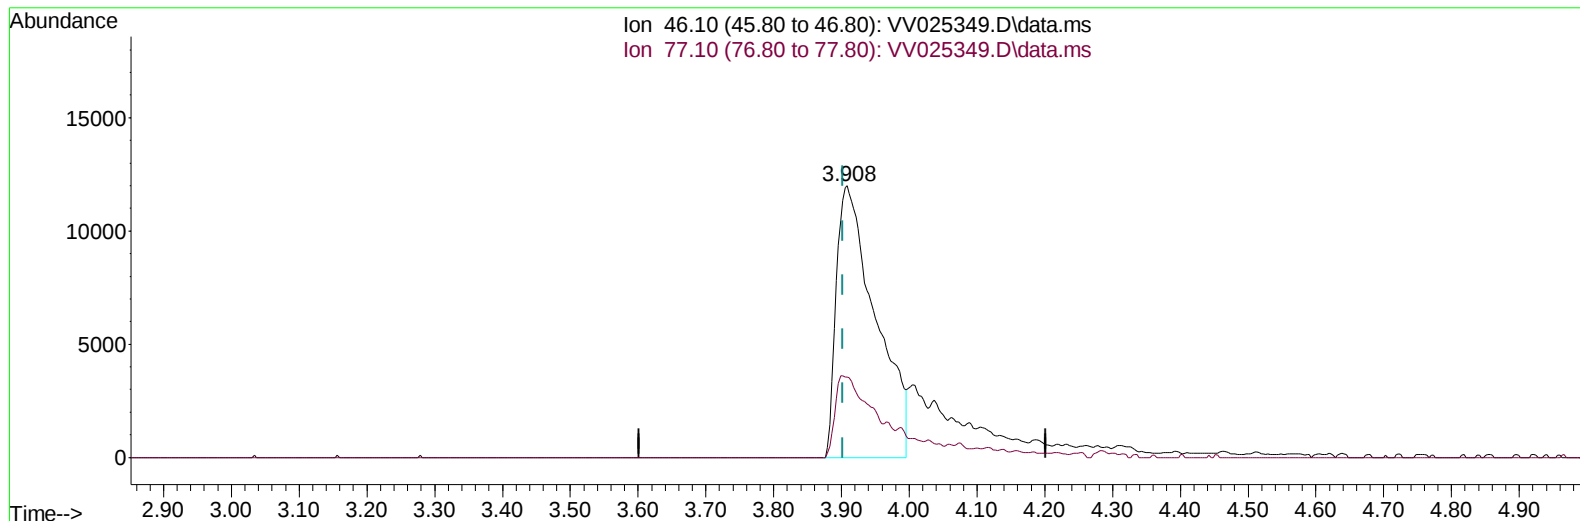

(20) 2-Butanone-d5 (S)

3.908min (+ 0.006) 41.65 ug/L

response 48120

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	24.90	25.85
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040522\
 Data File : VV025349.D
 Acq On : 05 Apr 2022 11:58
 Operator : SY/MD
 Sample : VV0405WBL01
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK334

Manual IntegrationsAPPROVED

Quant Time: Apr 06 01:29:05 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Apr 06 01:28:15 2022
 Response via : Initial Calibration

Reviewed By :John Carlone 04/06/2022
 Supervised By :Mahesh Dadoda 04/06/2022

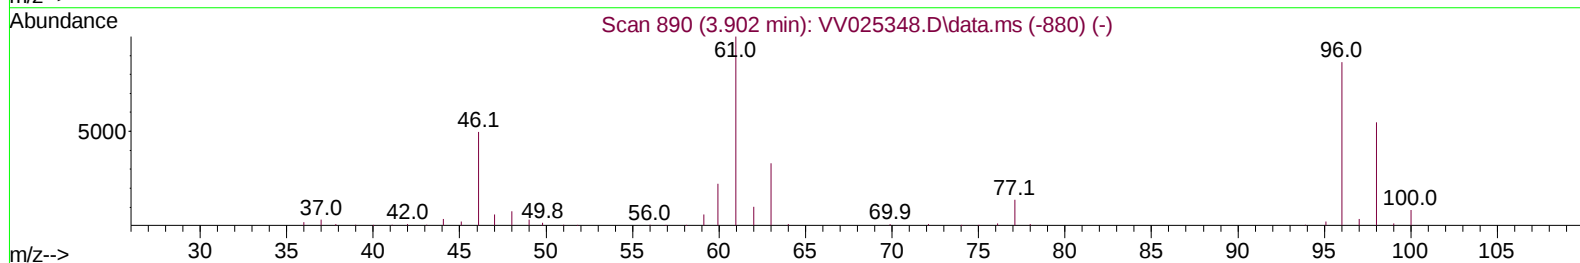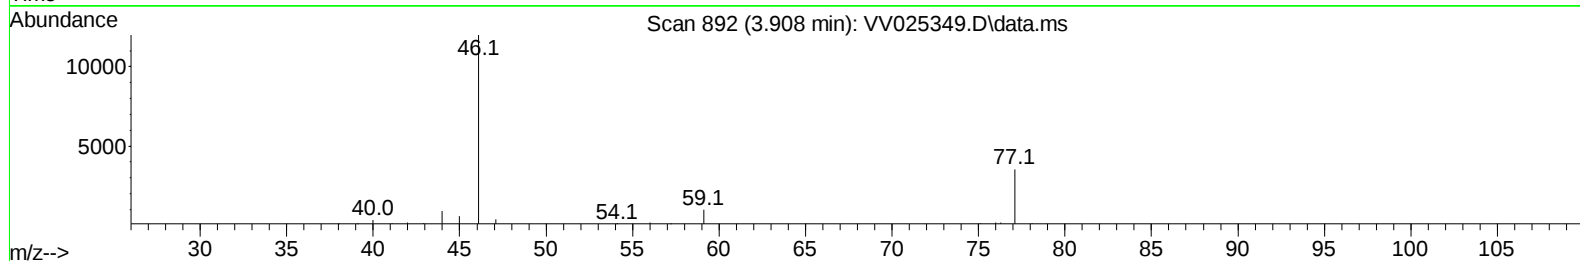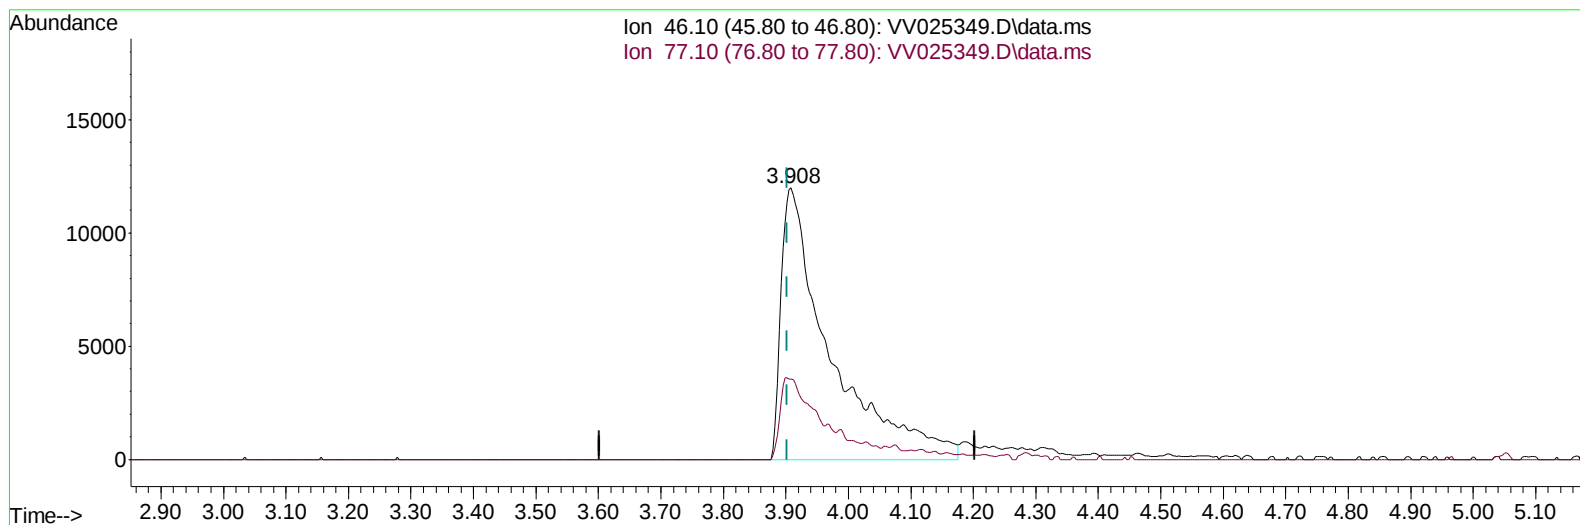

TIC: VV025349.D\data.ms

(20) 2-Butanone-d5 (S)

3.908min (+ 0.006) 56.59 ug/L m

response 65378

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	24.90	19.02
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040522\
 Data File : VV025349.D
 Acq On : 05 Apr 2022 11:58
 Operator : SY/MD
 Sample : VV0405WBL01
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK334

Manual IntegrationsAPPROVED

Reviewed By : John Carlone 04/06/2022
 Supervised By : Mahesh Dadoda 04/06/2022

Quant Time: Apr 06 01:29:05 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Apr 06 01:28:15 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.613	114	124168	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	124252	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	53025	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	59956	5.169	ug/L	0.00
Spiked Amount 5.000	Range 40 - 130		Recovery = 103.400%			
7) Chloroethane-d5	1.568	69	54974	5.647	ug/L	0.00
Spiked Amount 5.000	Range 65 - 130		Recovery = 113.000%			
11) 1,1-Dichloroethene-d2	2.105	63	91267	3.633	ug/L	0.00
Spiked Amount 5.000	Range 60 - 125		Recovery = 72.600%			
20) 2-Butanone-d5	3.908	46	65378m	56.588	ug/L	0.00
Spiked Amount 50.000	Range 40 - 130		Recovery = 113.180%			
24) Chloroform-d	4.346	84	82692	5.463	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery = 109.200%			
26) 1,2-Dichloroethane-d4	5.031	65	38596	5.769	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery = 115.400%			
32) Benzene-d6	5.047	84	159032	5.059	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery = 101.200%			
36) 1,2-Dichloropropane-d6	6.066	67	47197	5.357	ug/L	0.00
Spiked Amount 5.000	Range 60 - 140		Recovery = 107.200%			
41) Toluene-d8	7.313	98	131717	4.568	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery = 91.400%			
43) trans-1,3-Dichloroprop...	7.622	79	14264	4.963	ug/L	0.00
Spiked Amount 5.000	Range 55 - 130		Recovery = 99.200%			
46) 2-Hexanone-d5	8.088	63	49964	48.136	ug/L	0.00
Spiked Amount 50.000	Range 45 - 130		Recovery = 96.280%			
56) 1,1,2,2-Tetrachloroeth...	10.214	84	32162	5.475	ug/L	0.00
Spiked Amount 5.000	Range 65 - 120		Recovery = 109.600%			
66) 1,2-Dichlorobenzene-d4	11.622	152	46025	5.404	ug/L	0.00
Spiked Amount 5.000	Range 80 - 120		Recovery = 108.000%			
Target Compounds						Qvalue
16) Methylene chloride	2.507	84	5343	0.544	ug/L	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040522\
Data File : VV025349.D
Acq On : 05 Apr 2022 11:58
Operator : SY/MD
Sample : VV0405WBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK334

Manual IntegrationsAPPROVED

Quant Time: Apr 06 01:29:05 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Apr 06 01:28:15 2022
Response via : Initial Calibration

Reviewed By : John Carlone 04/06/2022
Supervised By : Mahesh Dadoda 04/06/2022

