




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040522\
 Data File : VV025350.D
 Acq On : 05 Apr 2022 12:36
 Operator : SY/MD
 Sample : N2261-01
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFY38

Manual IntegrationsAPPROVED

Quant Time: Apr 06 01:29:18 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Apr 06 01:28:15 2022
 Response via : Initial Calibration

Reviewed By :John Carlone 04/06/2022
 Supervised By :Mahesh Dadoda 04/06/2022

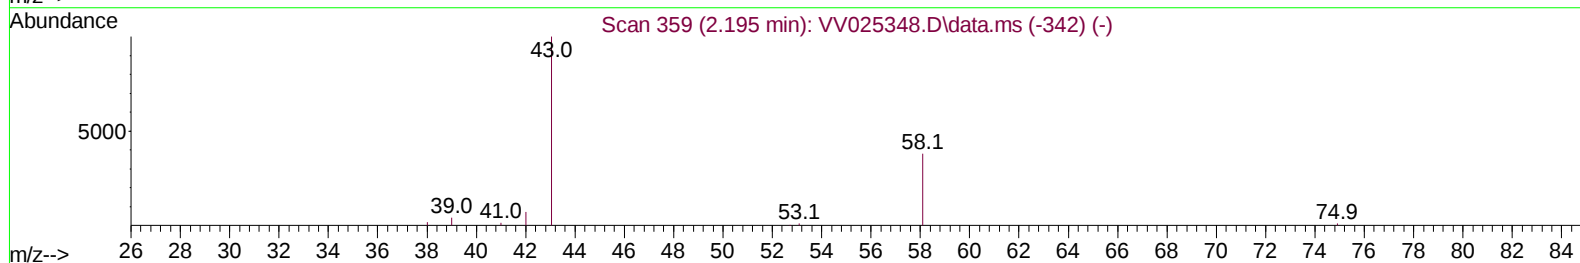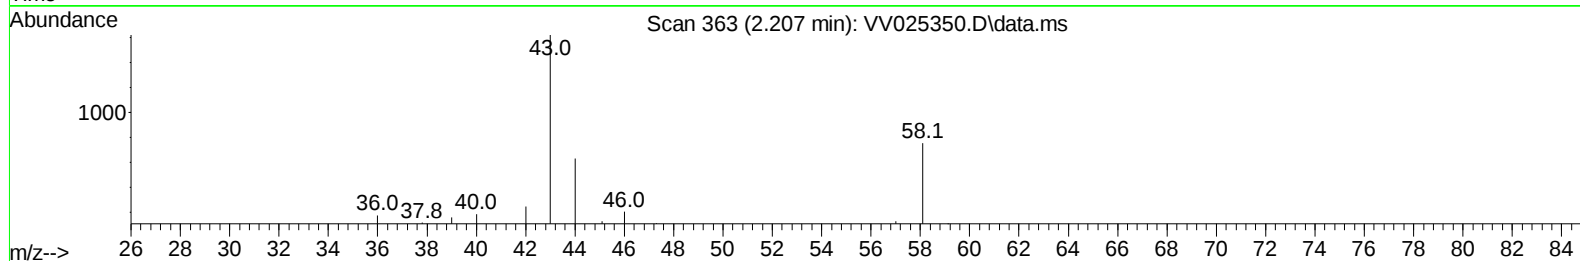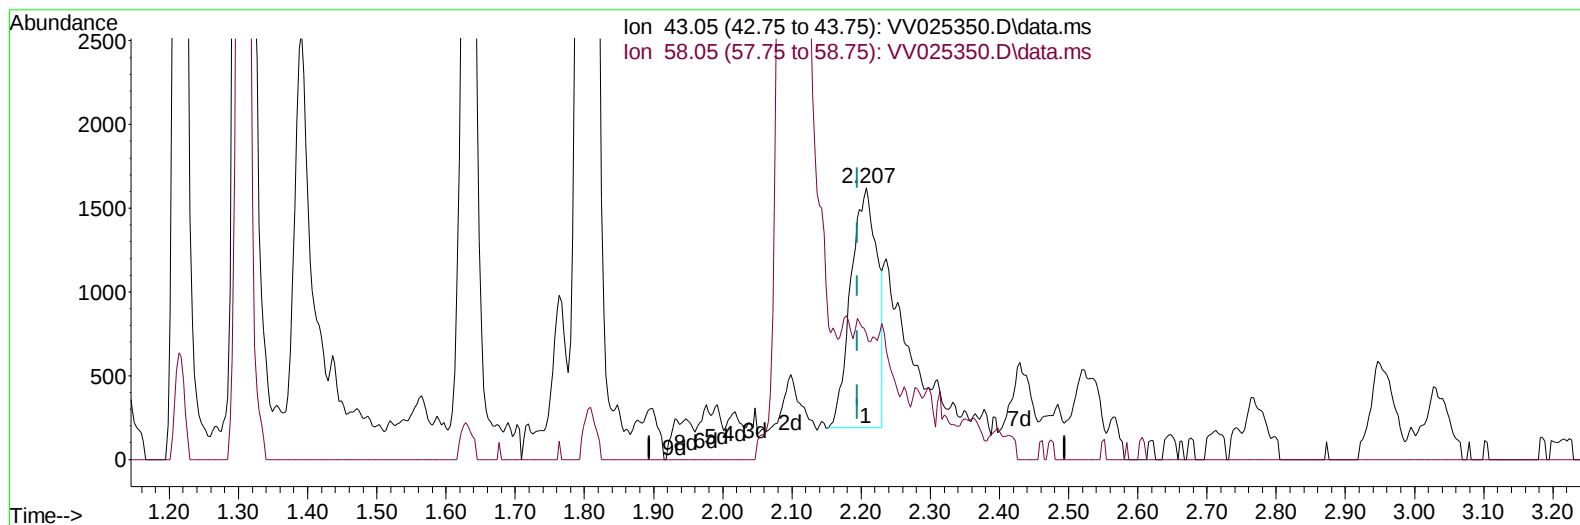

TIC: VV025350.D\data.ms

(13) Acetone (T)

2.207min (+ 0.013) 4.09 ug/L

response 3835

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	25.60	0.00
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040522\
 Data File : VV025350.D
 Acq On : 05 Apr 2022 12:36
 Operator : SY/MD
 Sample : N2261-01
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFY38

Manual IntegrationsAPPROVED

Quant Time: Apr 06 01:29:18 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Apr 06 01:28:15 2022
 Response via : Initial Calibration

Reviewed By :John Carlone 04/06/2022
 Supervised By :Mahesh Dadoda 04/06/2022

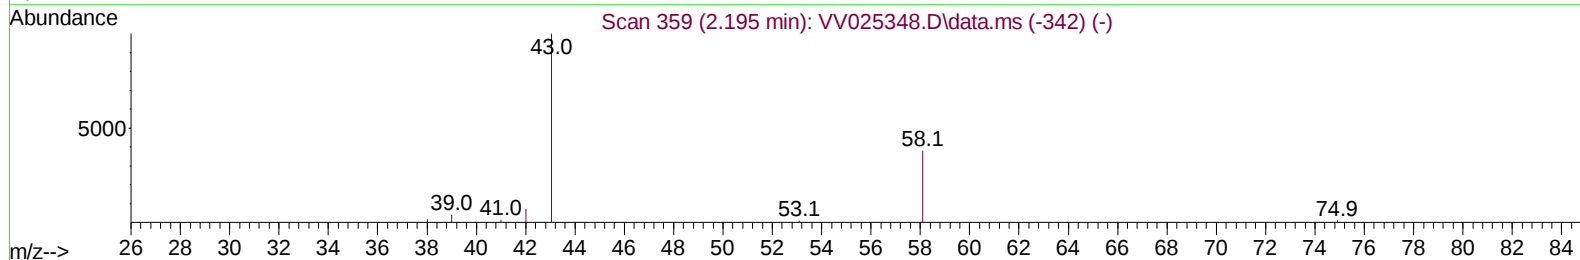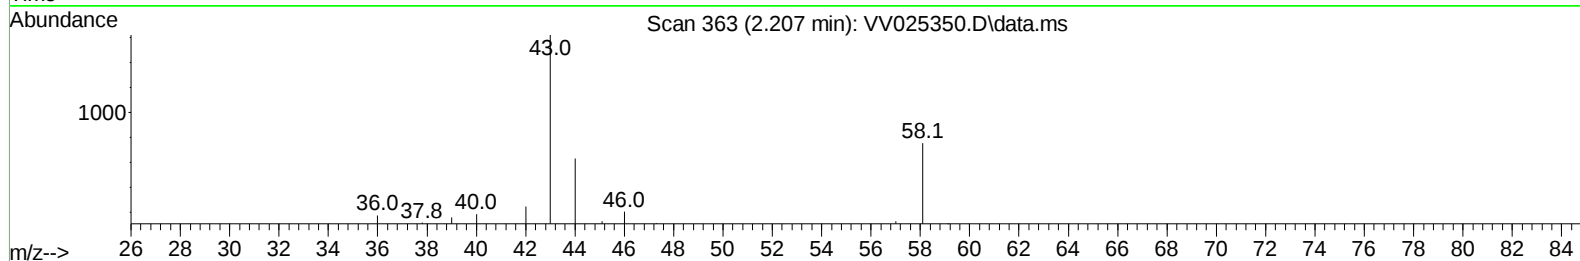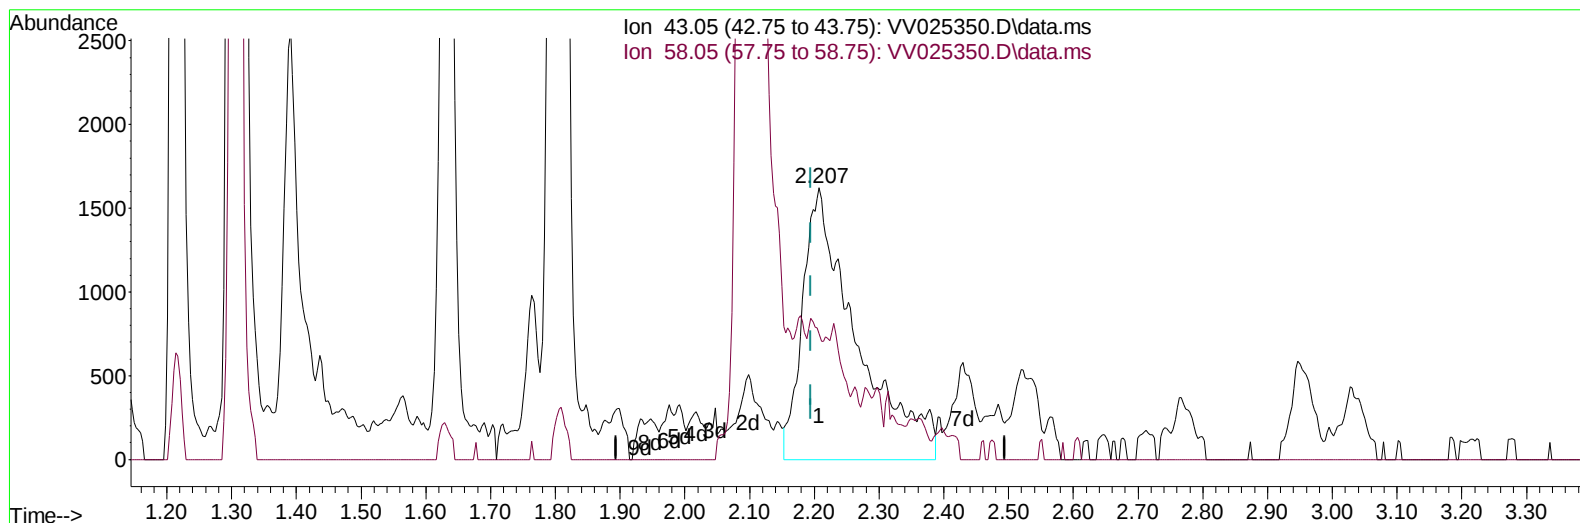

TIC: VV025350.D\data.ms

(13) Acetone (T)

2.207min (+ 0.013) 9.95 ug/L m

response 9339

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	25.60	0.00
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040522\
Data File : VV025350.D
Acq On : 05 Apr 2022 12:36
Operator : SY/MD
Sample : N2261-01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFY38

Manual IntegrationsAPPROVED

Quant Time: Apr 06 01:29:18 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Apr 06 01:28:15 2022
Response via : Initial Calibration

Reviewed By :John Carlone 04/06/2022
Supervised By :Mahesh Dadoda 04/06/2022

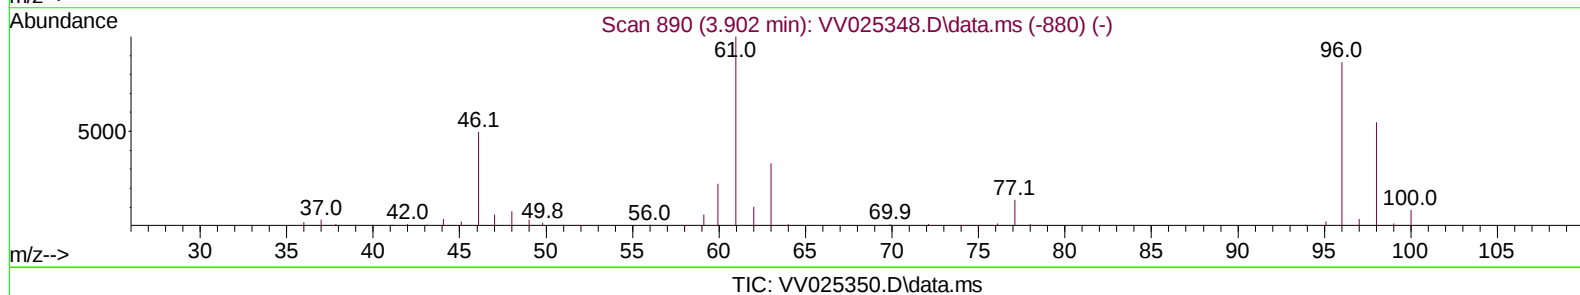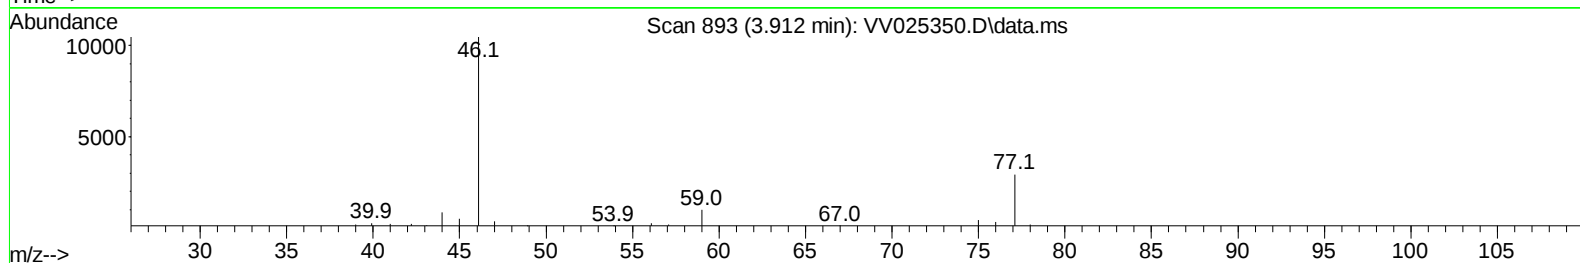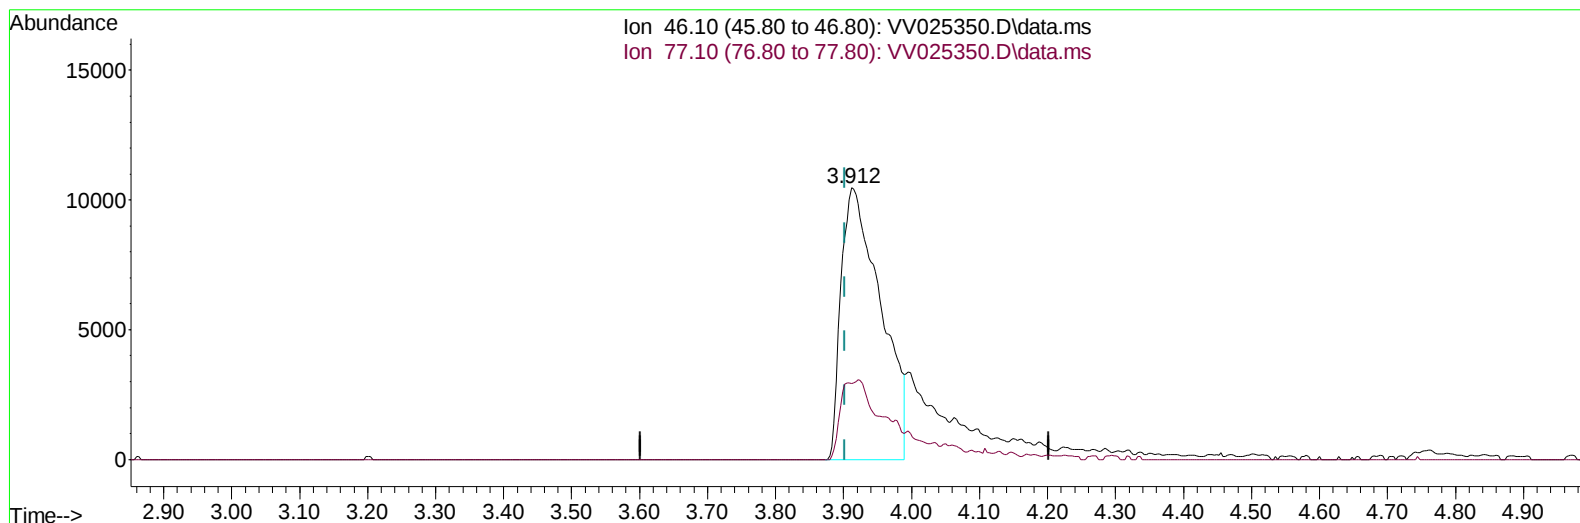

(20) 2-Butanone-d5 (S)

3.912min (+ 0.010) 34.36 ug/L

response 42266

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	24.90	8.73#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040522\
 Data File : VV025350.D
 Acq On : 05 Apr 2022 12:36
 Operator : SY/MD
 Sample : N2261-01
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFY38

Manual IntegrationsAPPROVED

Quant Time: Apr 06 01:29:18 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Apr 06 01:28:15 2022
 Response via : Initial Calibration

Reviewed By :John Carlone 04/06/2022
 Supervised By :Mahesh Dadoda 04/06/2022

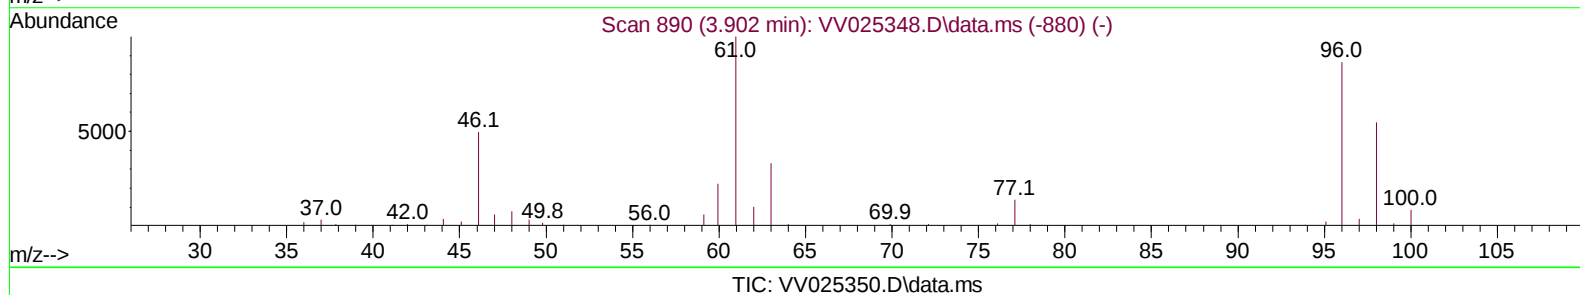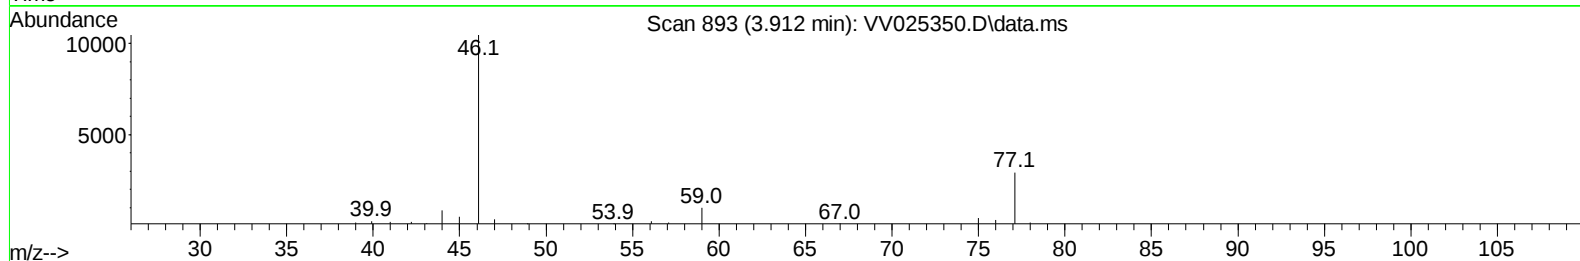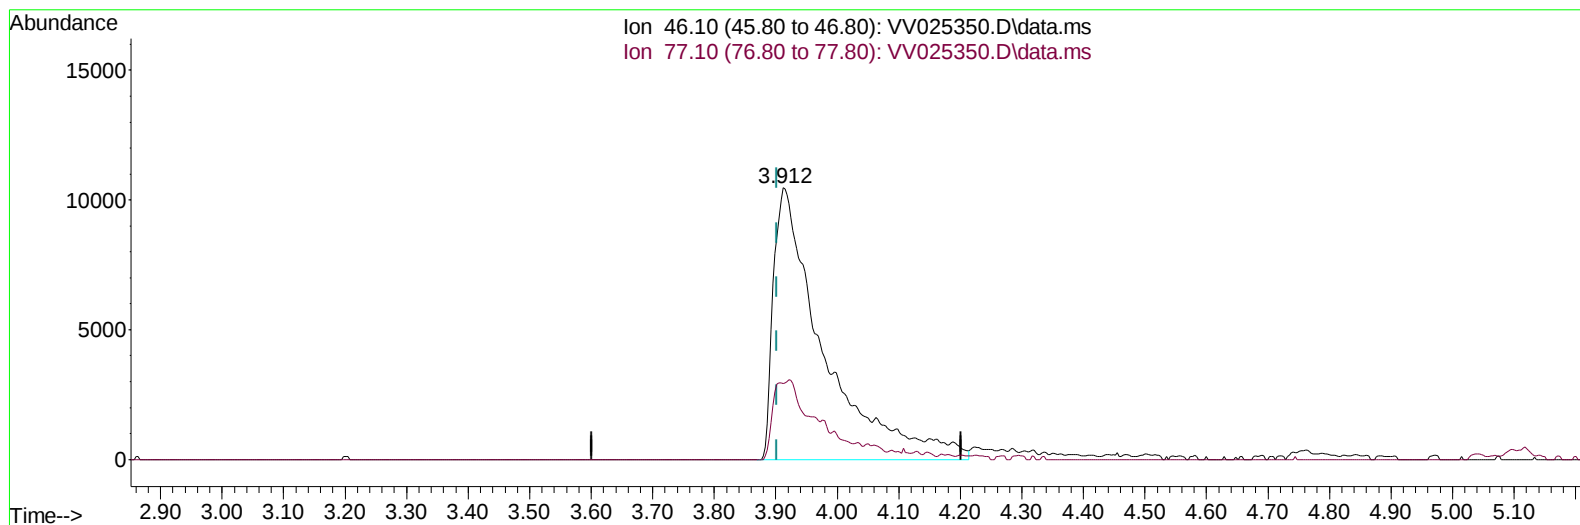

(20) 2-Butanone-d5 (S)

3.912min (+ 0.010) 48.32 ug/L m

response 59434

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	24.90	6.21#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040522\
 Data File : VV025350.D
 Acq On : 05 Apr 2022 12:36
 Operator : SY/MD
 Sample : N2261-01
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFY38

Manual IntegrationsAPPROVED

Quant Time: Apr 06 01:29:18 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Apr 06 01:28:15 2022
 Response via : Initial Calibration

Reviewed By :John Carlone 04/06/2022
 Supervised By :Mahesh Dadoda 04/06/2022

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.612	114		132188	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117		128864	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152		64100	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.304	65		55695	4.511	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130		Recovery	=	90.200%	
7) Chloroethane-d5	1.568	69		50756	4.898	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130		Recovery	=	98.000%	
11) 1,1-Dichloroethene-d2	2.105	63		92798	3.470	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125		Recovery	=	69.400%	
20) 2-Butanone-d5	3.912	46		59434m	48.322	ug/L	0.00
Spiked Amount 50.000	Range 40	- 130		Recovery	=	96.640%	
24) Chloroform-d	4.342	84		78529	4.873	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery	=	97.400%	
26) 1,2-Dichloroethane-d4	5.027	65		33759	4.740	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery	=	94.800%	
32) Benzene-d6	5.043	84		146709	4.500	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery	=	90.000%	
36) 1,2-Dichloropropane-d6	6.066	67		42527	4.655	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140		Recovery	=	93.000%	
41) Toluene-d8	7.313	98		124315	4.157	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery	=	83.200%	
43) trans-1,3-Dichloroprop...	7.622	79		13739	4.609	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130		Recovery	=	92.200%	
46) 2-Hexanone-d5	8.088	63		47232	43.876	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130		Recovery	=	87.760%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84		28562	4.688	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120		Recovery	=	93.800%	
66) 1,2-Dichlorobenzene-d4	11.622	152		47539	4.618	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120		Recovery	=	92.400%	
Target Compounds							
						Qvalue	
12) 1,1-Dichloroethene	2.114	96		13473	1.012	ug/L #	1
13) Acetone	2.207	43		9339m	9.951	ug/L	
16) Methylene chloride	2.507	84		2031	0.194	ug/L	91
19) 1,1-Dichloroethane	3.188	63		26432	1.658	ug/L	99
29) 1,1,1-Trichloroethane	4.606	97		2008	0.129	ug/L #	88
33) Benzene	5.101	78		4617	0.122	ug/L	100
34) Trichloroethene	5.915	95		2565	0.247	ug/L	82
42) Toluene	7.391	91		14287	0.354	ug/L	93
47) Tetrachloroethene	7.976	164		1228	0.160	ug/L	88
52) Ethylbenzene	9.018	91		6117	0.143	ug/L	99
53) m,p-Xylene	9.143	106		3419	0.205	ug/L	85
54) o-Xylene	9.548	106		1765	0.111	ug/L	88
63) 1,2,4-Trimethylbenzene	10.915	105		3881	0.114	ug/L	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040522\
Data File : VV025350.D
Acq On : 05 Apr 2022 12:36
Operator : SY/MD
Sample : N2261-01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFY38

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 04/06/2022
Supervised By :Mahesh Dadoda 04/06/2022

Quant Time: Apr 06 01:29:18 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Apr 06 01:28:15 2022
Response via : Initial Calibration

