




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040522\
 Data File : VV025352.D
 Acq On : 05 Apr 2022 13:23
 Operator : SY/MD
 Sample : N2261-03
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFY40

Manual IntegrationsAPPROVED

Quant Time: Apr 06 01:29:50 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Apr 06 01:28:15 2022
 Response via : Initial Calibration

Reviewed By :John Carlone 04/06/2022
 Supervised By :Mahesh Dadoda 04/06/2022

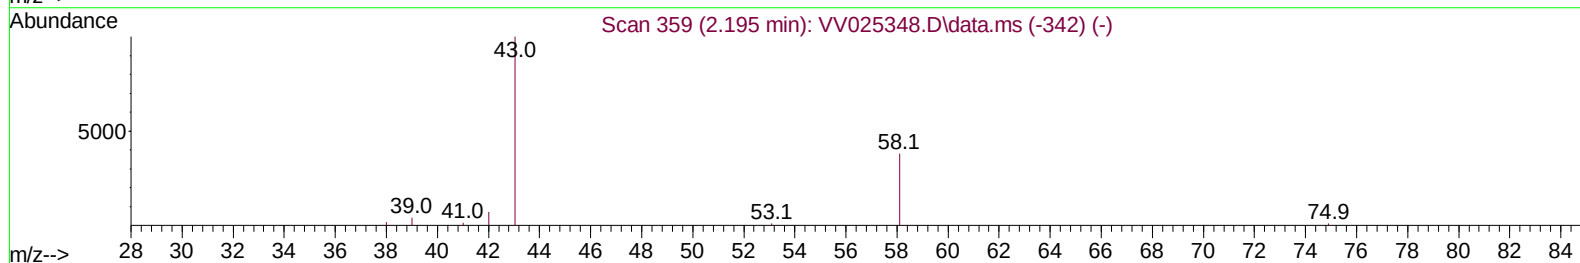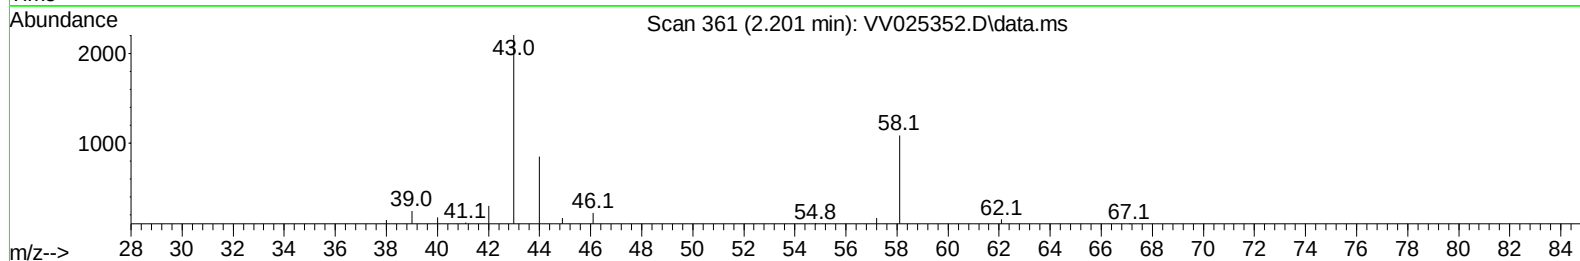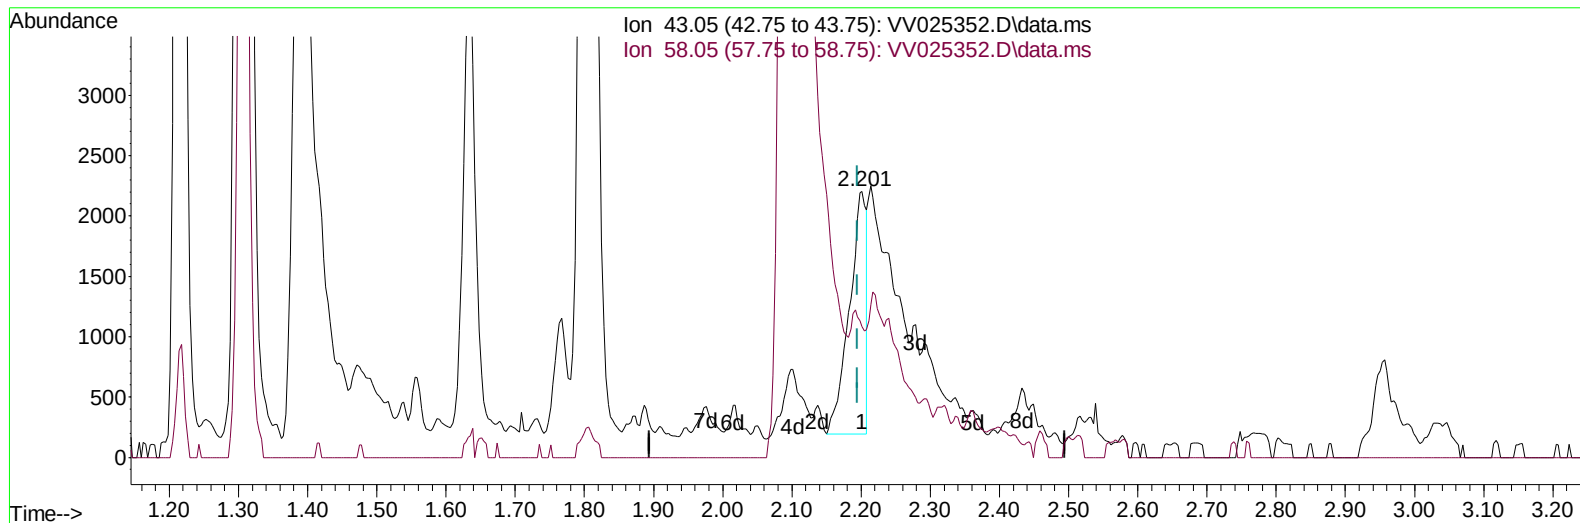

TIC: VV025352.D\data.ms

(13) Acetone (T)

2.201min (+ 0.007) 3.09 ug/L

response 3426

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	25.60	0.00
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040522\
 Data File : VV025352.D
 Acq On : 05 Apr 2022 13:23
 Operator : SY/MD
 Sample : N2261-03
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFY40

Manual IntegrationsAPPROVED

Quant Time: Apr 06 01:29:50 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Apr 06 01:28:15 2022
 Response via : Initial Calibration

Reviewed By :John Carlone 04/06/2022
 Supervised By :Mahesh Dadoda 04/06/2022

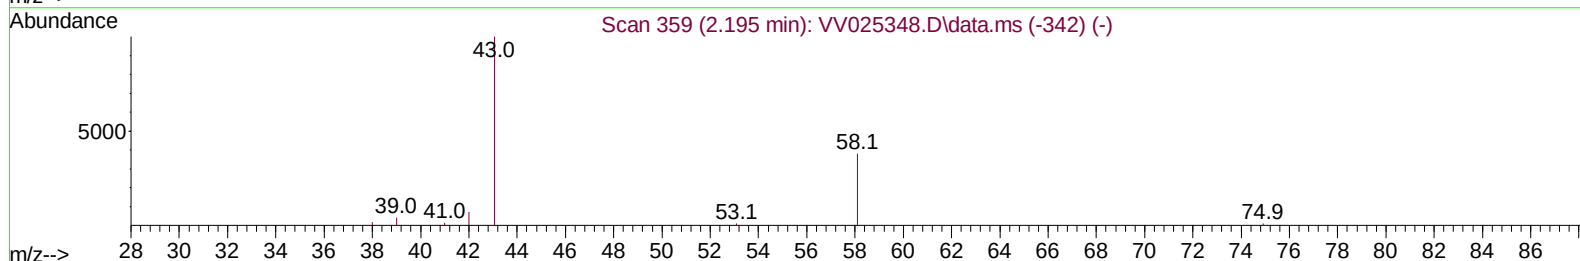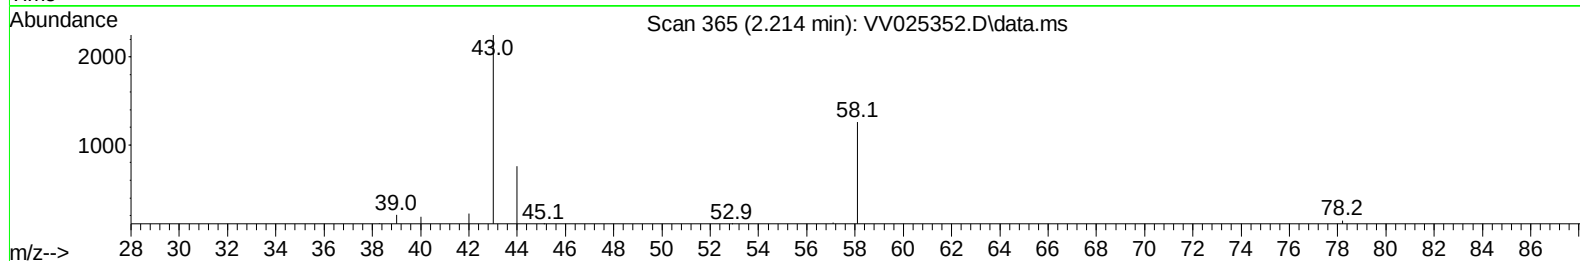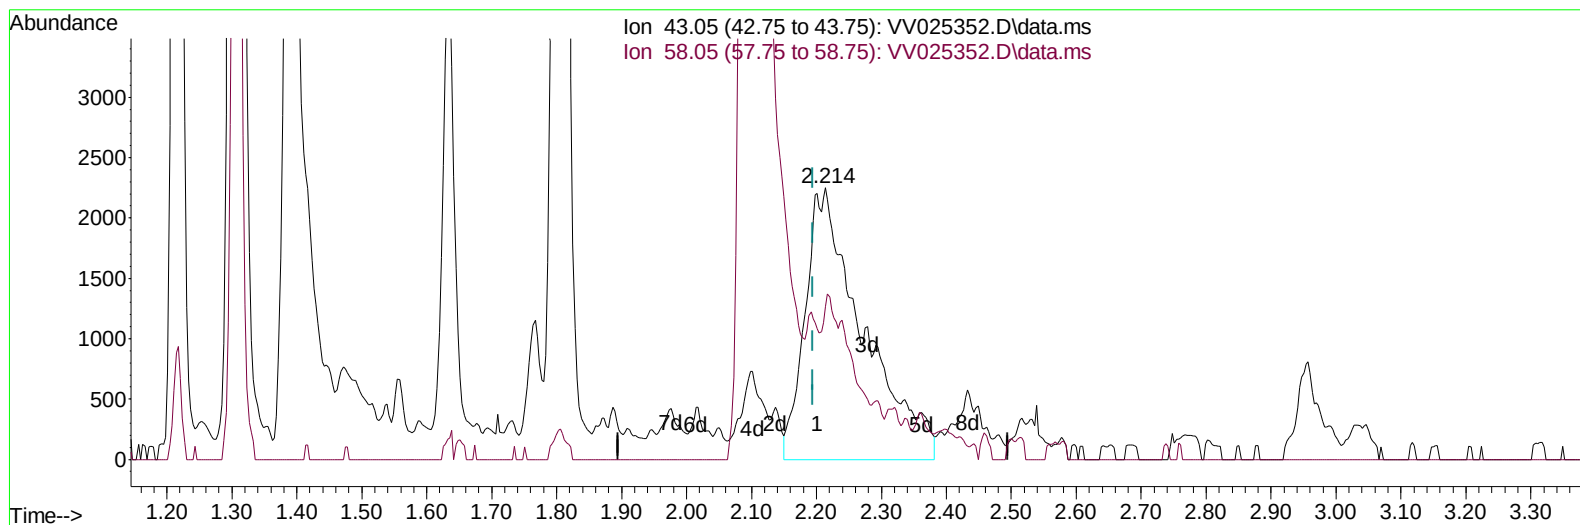

TIC: VV025352.D\data.ms

(13) Acetone (T)

2.214min (+ 0.019) 12.52 ug/L m

response 13872

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	25.60	0.00
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040522\
 Data File : VV025352.D
 Acq On : 05 Apr 2022 13:23
 Operator : SY/MD
 Sample : N2261-03
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFY40

Manual IntegrationsAPPROVED

Quant Time: Apr 06 01:29:50 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Apr 06 01:28:15 2022
 Response via : Initial Calibration

Reviewed By :John Carlone 04/06/2022
 Supervised By :Mahesh Dadoda 04/06/2022

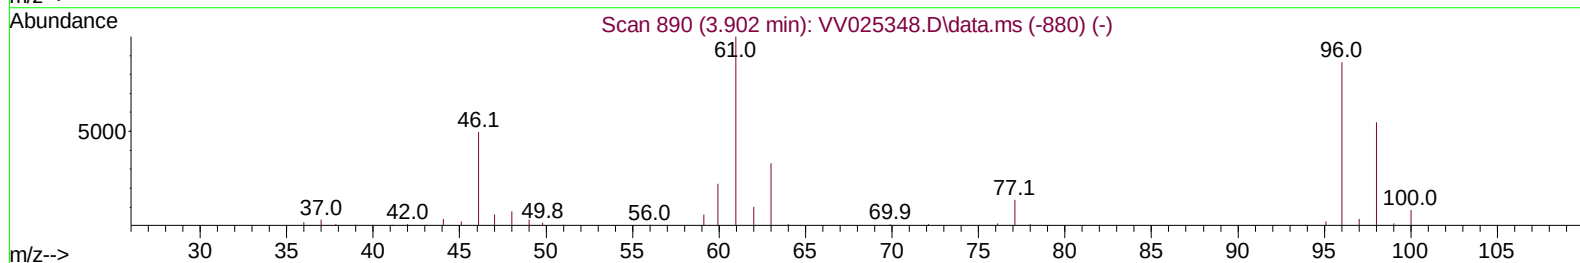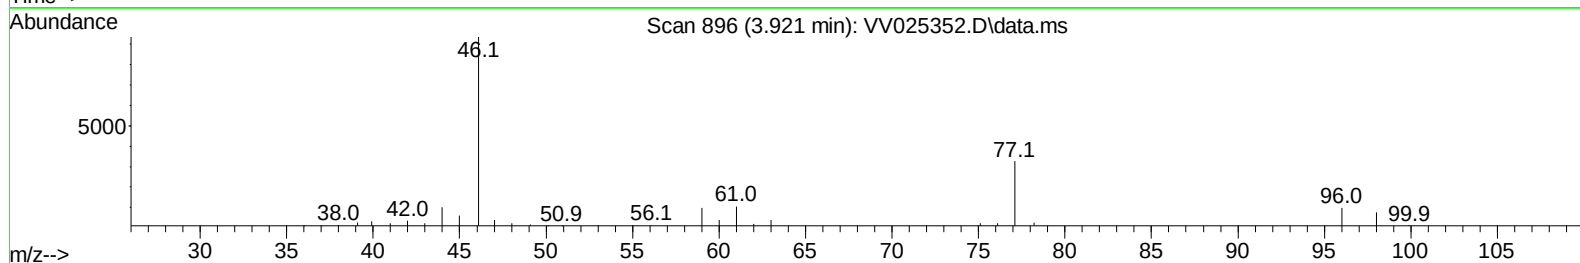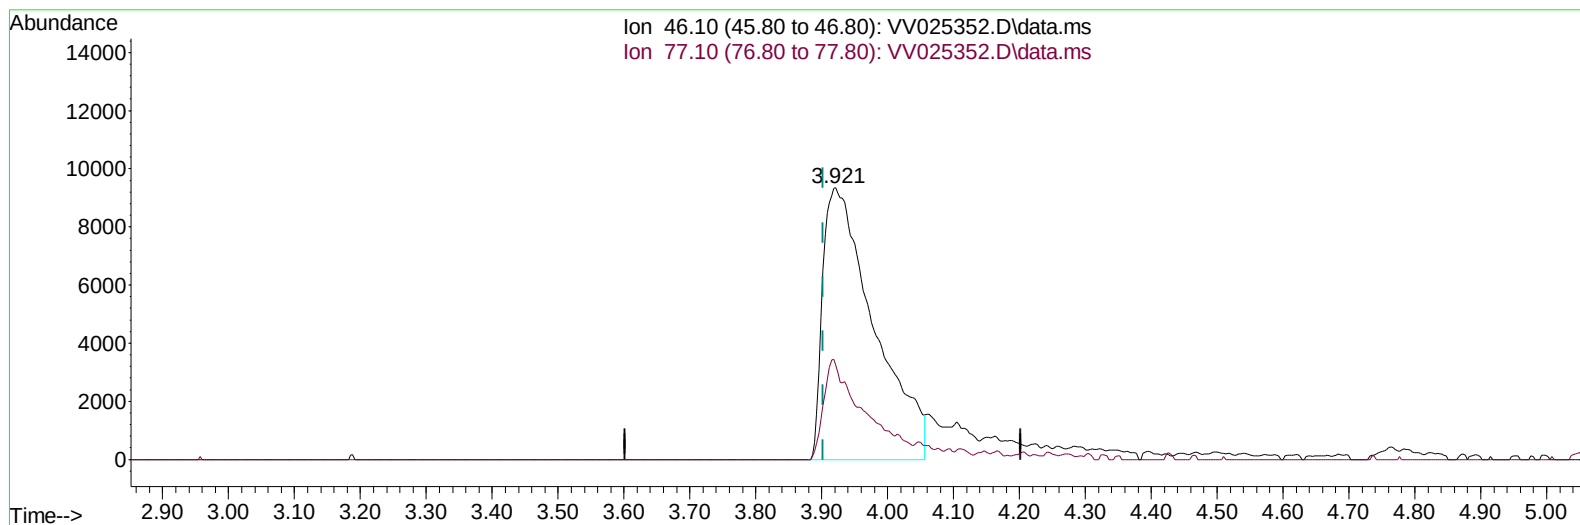

TIC: VV025352.D\data.ms

(20) 2-Butanone-d5 (S)

3.921min (+ 0.019) 34.63 ug/L

response 50303

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	24.90	26.90
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040522\
 Data File : VV025352.D
 Acq On : 05 Apr 2022 13:23
 Operator : SY/MD
 Sample : N2261-03
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFY40

Manual IntegrationsAPPROVED

Quant Time: Apr 06 01:29:50 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Apr 06 01:28:15 2022
 Response via : Initial Calibration

Reviewed By :John Carlone 04/06/2022
 Supervised By :Mahesh Dadoda 04/06/2022

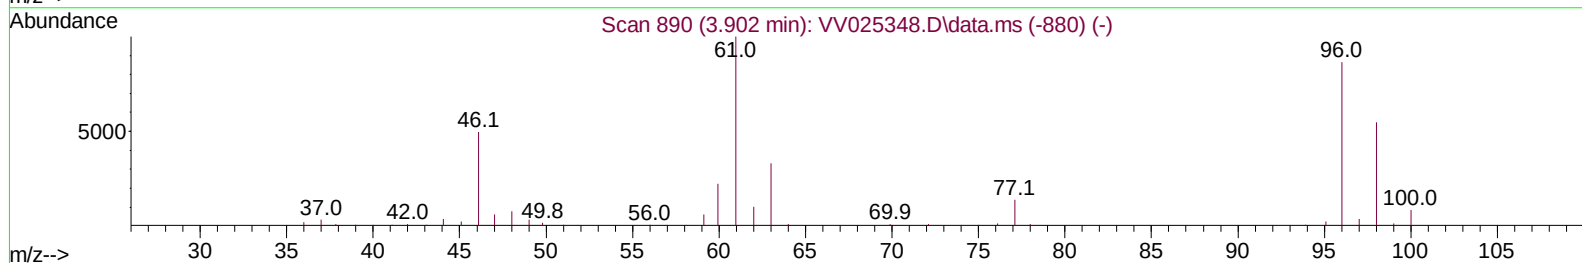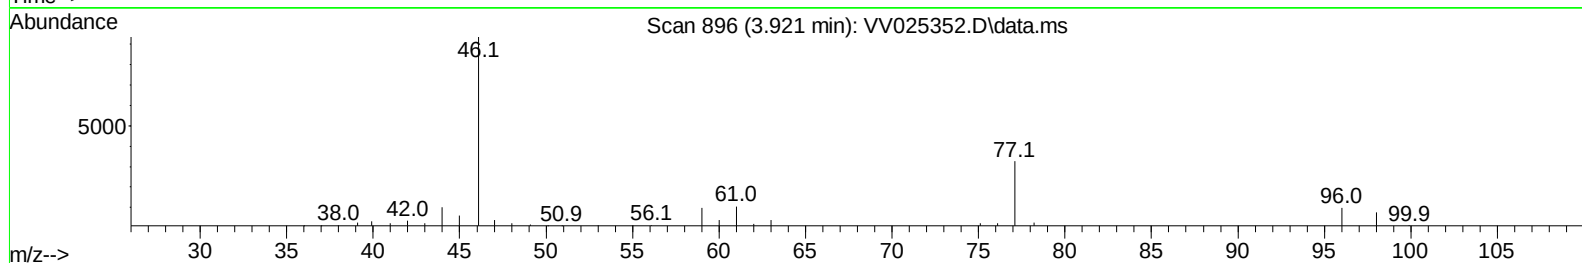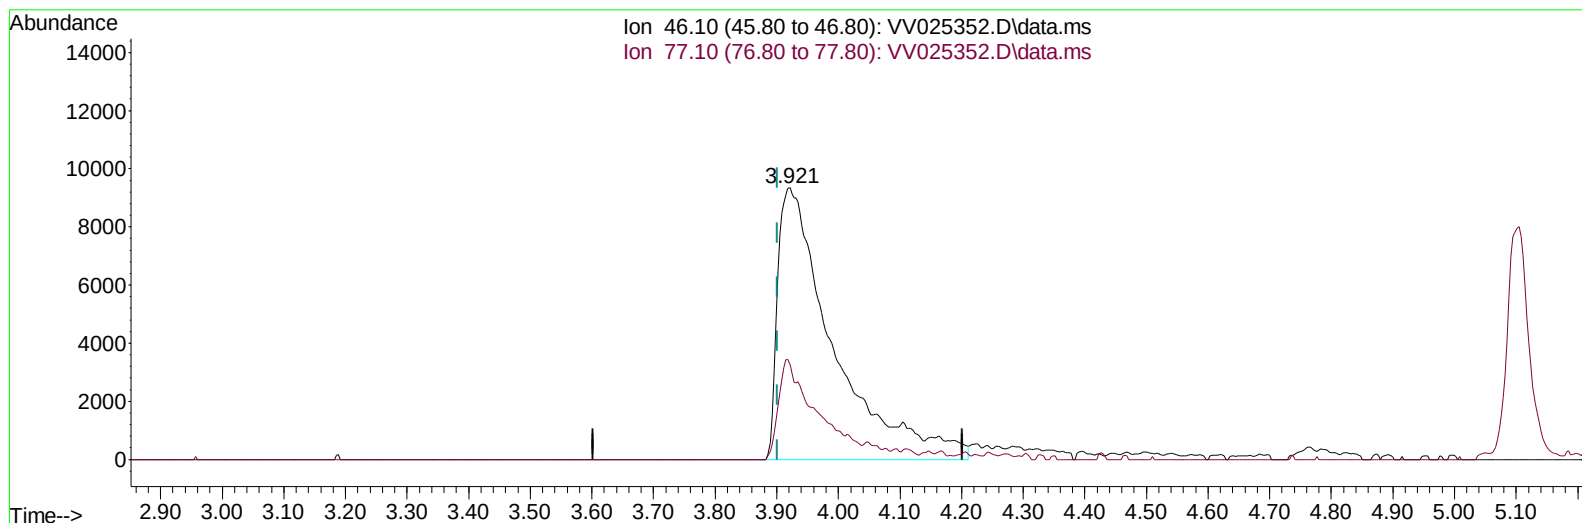

TIC: VV025352.D\data.ms

(20) 2-Butanone-d5 (S)

3.921min (+ 0.019) 40.37 ug/L m

response 58641

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	24.90	23.07
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040522\
 Data File : VV025352.D
 Acq On : 05 Apr 2022 13:23
 Operator : SY/MD
 Sample : N2261-03
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFY40

Manual IntegrationsAPPROVED

Quant Time: Apr 06 01:29:50 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Apr 06 01:28:15 2022
 Response via : Initial Calibration

Reviewed By : John Carlone 04/06/2022
 Supervised By : Mahesh Dadoda 04/06/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	156114	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	150873	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	75029	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	55784	3.825	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130	Recovery	=	76.600%	
7) Chloroethane-d5	1.568	69	52236	4.268	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130	Recovery	=	85.400%	
11) 1,1-Dichloroethene-d2	2.105	63	84545	2.677	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125	Recovery	=	53.600%#	
20) 2-Butanone-d5	3.921	46	58641m	40.370	ug/L	0.02
Spiked Amount 50.000	Range 40	- 130	Recovery	=	80.740%	
24) Chloroform-d	4.349	84	78002	4.099	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	82.000%	
26) 1,2-Dichloroethane-d4	5.034	65	34318	4.080	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	81.600%	
32) Benzene-d6	5.050	84	146768	3.845	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	77.000%	
36) 1,2-Dichloropropane-d6	6.069	67	43322	4.050	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140	Recovery	=	81.000%	
41) Toluene-d8	7.317	98	129197	3.690	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	73.800%	
43) trans-1,3-Dichloroprop...	7.625	79	13426	3.847	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130	Recovery	=	77.000%	
46) 2-Hexanone-d5	8.092	63	50100	39.751	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130	Recovery	=	79.500%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	28840	4.043	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120	Recovery	=	80.800%	
66) 1,2-Dichlorobenzene-d4	11.622	152	47837	3.970	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120	Recovery	=	79.400%#	
Target Compounds						
					Qvalue	
12) 1,1-Dichloroethene	2.114	96	1948	0.124	ug/L #	1
13) Acetone	2.214	43	13872m	12.515	ug/L	
19) 1,1-Dichloroethane	3.192	63	16955	0.900	ug/L	93
22) cis-1,2-Dichloroethene	3.928	96	2530	0.221	ug/L	80
25) Chloroform	4.378	83	12285	0.588	ug/L	95
33) Benzene	5.101	78	82829	1.872	ug/L	100
42) Toluene	7.391	91	49707	1.052	ug/L	96
47) Tetrachloroethene	7.979	164	553	0.062	ug/L	85
52) Ethylbenzene	9.018	91	5441	0.109	ug/L	96
53) m,p-Xylene	9.146	106	2621	0.134	ug/L	97
54) o-Xylene	9.548	106	2011	0.108	ug/L	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040522\
Data File : VV025352.D
Acq On : 05 Apr 2022 13:23
Operator : SY/MD
Sample : N2261-03
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFY40

Manual IntegrationsAPPROVED

Quant Time: Apr 06 01:29:50 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Apr 06 01:28:15 2022
Response via : Initial Calibration

Reviewed By :John Carlone 04/06/2022
Supervised By :Mahesh Dadoda 04/06/2022

