

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040522\
 Data File : VV025349.D
 Acq On : 05 Apr 2022 11:58
 Operator : SY/MD
 Sample : VV0405WBL01
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK334

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV025349.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	75	83	94	rVB	96466	98585	23.37%	2.817%
2	1.568	156	164	174	rBV	86078	97646	23.15%	2.790%
3	2.105	321	331	344	rBV	171513	249867	59.24%	7.139%
4	2.507	443	456	468	rBV2	12081	20831	4.94%	0.595%
5	3.908	881	892	919	rBV2	20201	84609	20.06%	2.417%
6	4.343	1011	1027	1057	rVB2	77866	197980	46.94%	5.657%
7	5.043	1230	1245	1273	rBV2	168364	421811	100.00%	12.052%
8	5.613	1411	1422	1448	rBV	138328	285197	67.61%	8.149%
9	5.912	1504	1515	1525	rBV7	3287	7330	1.74%	0.209%
10	6.066	1550	1563	1591	rBV2	95608	201293	47.72%	5.751%
11	6.985	1838	1849	1873	rBV2	41085	78071	18.51%	2.231%
12	7.313	1940	1951	1970	rBV	193574	342562	81.21%	9.788%
13	7.397	1974	1977	1987	rVB5	3109	4235	1.00%	0.121%
14	7.622	2038	2047	2063	rBV2	22119	40654	9.64%	1.162%
15	8.088	2182	2192	2224	rBV	129918	288206	68.33%	8.235%
16	8.850	2418	2429	2460	rBV	220551	362863	86.03%	10.368%
17	10.214	2842	2853	2867	rBV2	65174	105314	24.97%	3.009%
18	11.246	3164	3174	3193	rBV	202156	313971	74.43%	8.971%
19	11.622	3279	3291	3314	rBV	184417	288923	68.50%	8.255%
20	12.246	3475	3485	3495	rVB2	2885	4719	1.12%	0.135%
21	14.040	4034	4043	4053	rBV3	3235	5217	1.24%	0.149%




Sum of corrected areas: 3499884

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040522\
Data File : VV025349.D
Acq On : 05 Apr 2022 11:58
Operator : SY/MD
Sample : VV0405WBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK334

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

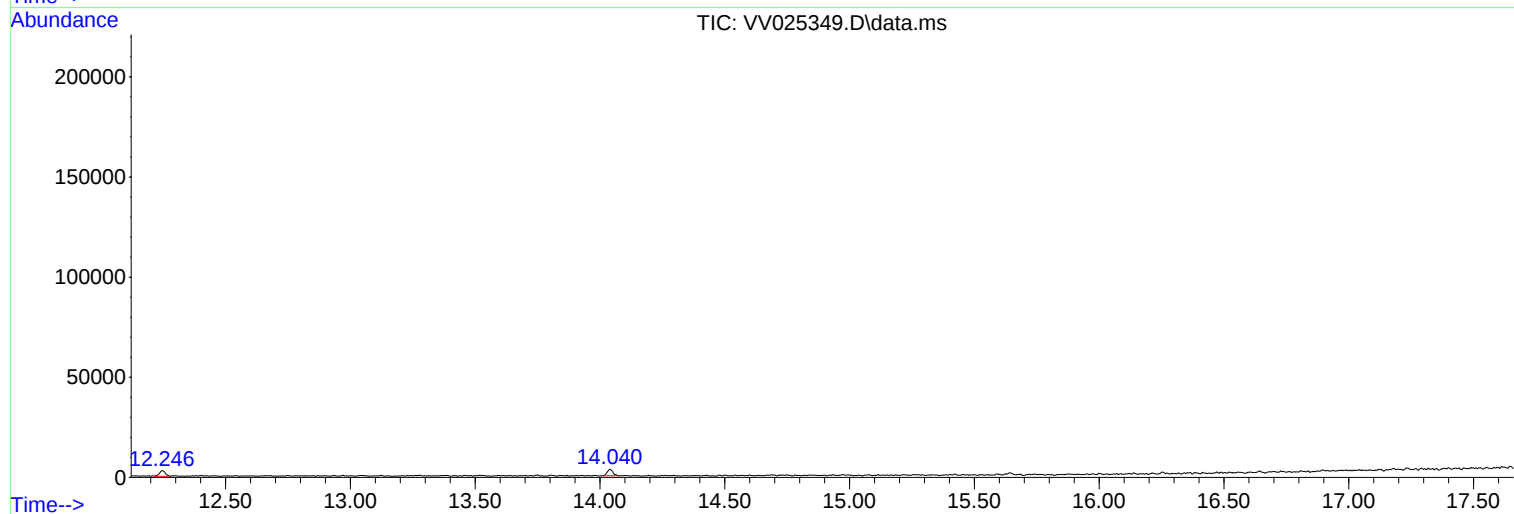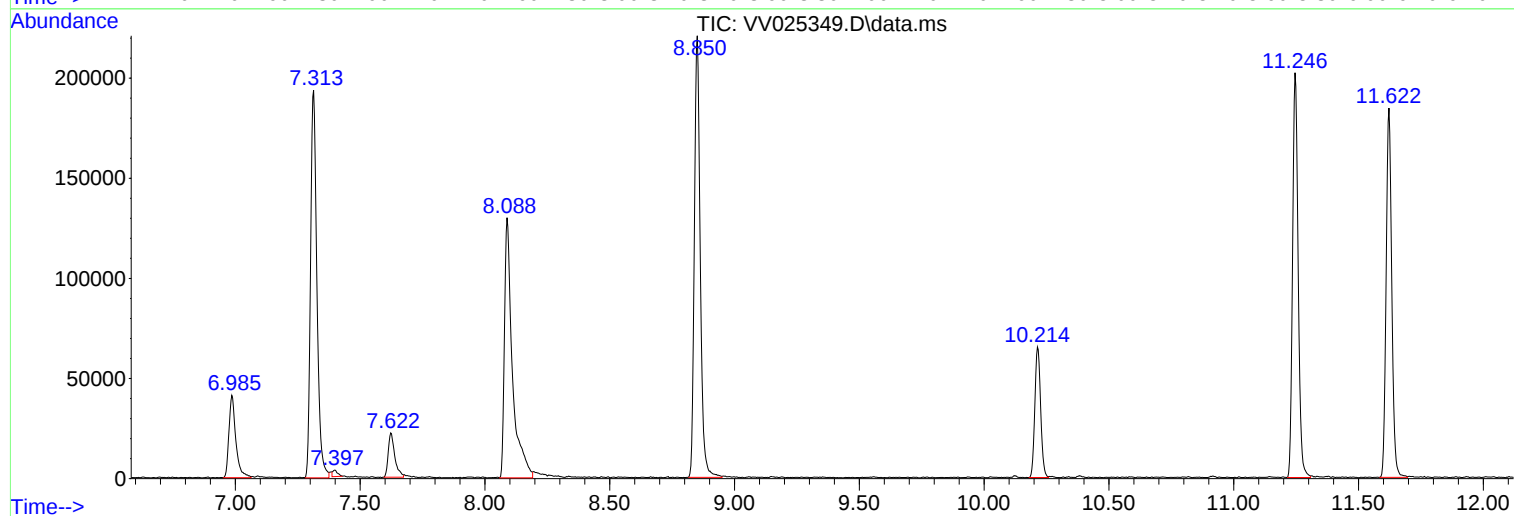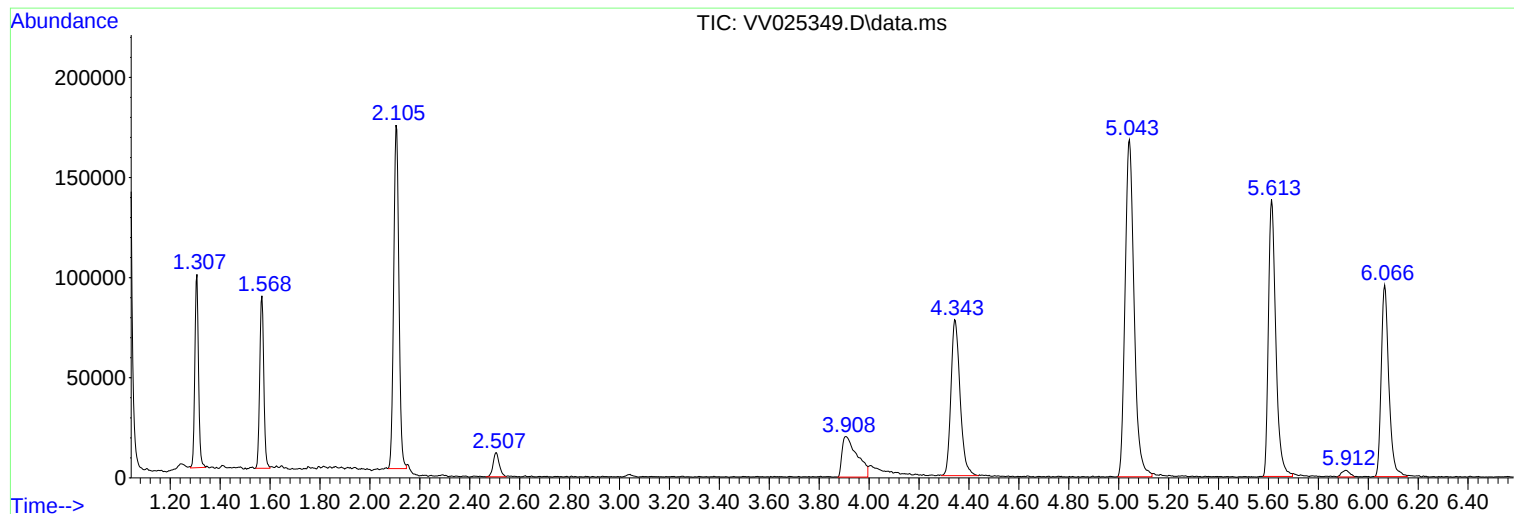

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040522\
Data File : VV025349.D
Acq On : 05 Apr 2022 11:58
Operator : SY/MD
Sample : VV0405WBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK334

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040522\
Data File : VV025349.D
Acq On : 05 Apr 2022 11:58
Operator : SY/MD
Sample : VV0405WBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK334

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc