
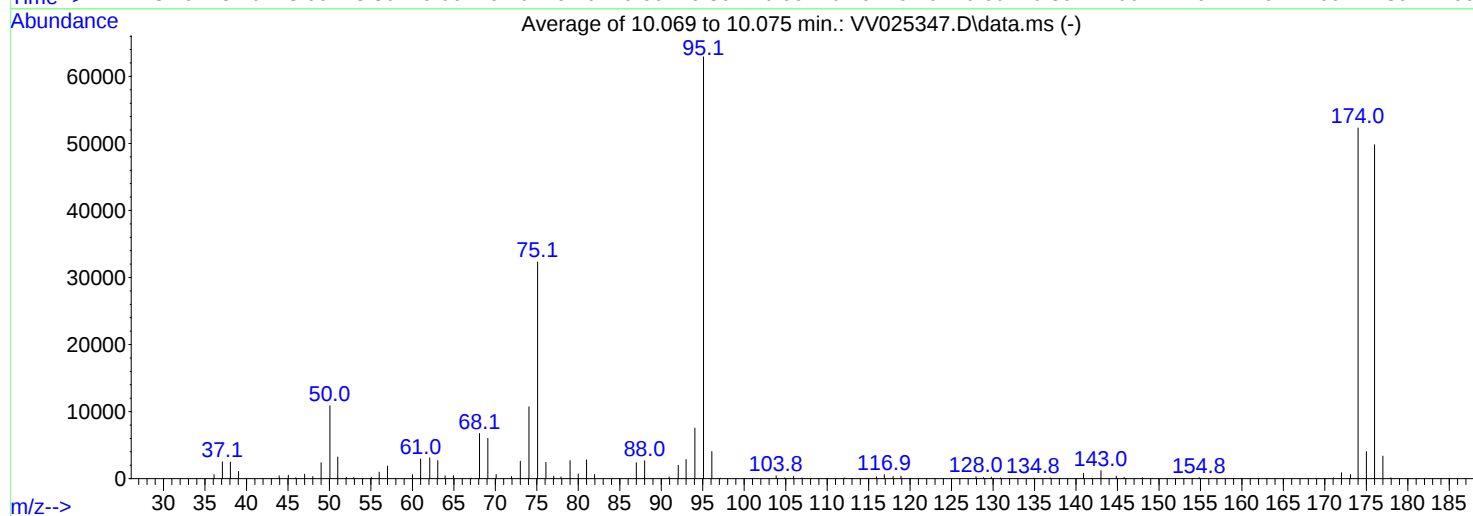


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040522\
 Data File : VV025347.D
 Acq On : 05 Apr 2022 08:58
 Operator : SY/MD
 Sample : BFB295
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB295

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Wed Apr 06 01:28:15 2022

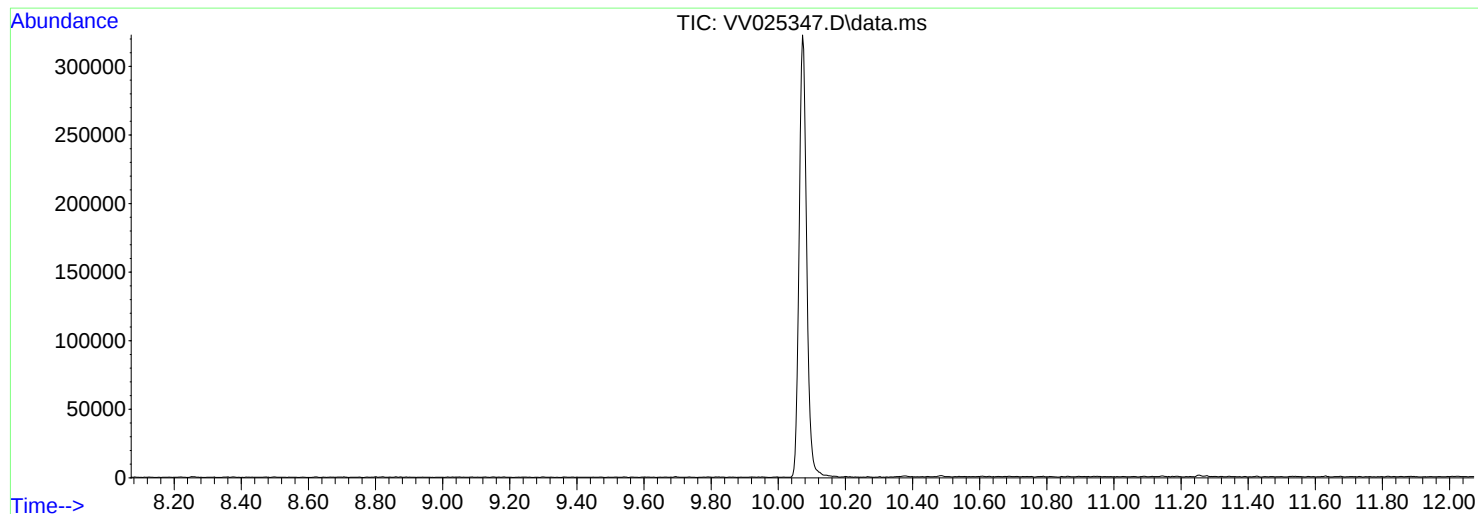

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.3	10894	PASS
75	95	30	80	51.4	32323	PASS
95	95	100	100	100.0	62917	PASS
96	95	5	9	6.4	4035	PASS
173	174	0.00	2	1.2	617	PASS
174	95	50	120	83.2	52323	PASS
175	174	5	9	7.7	4031	PASS
176	174	95	105	95.2	49813	PASS
177	176	5	10	6.7	3362	PASS

m/z	Abundance
40.10	226.0
43.90	280.0

Instrument :
MSVOA_V
ClientSampleId :
BFB295

m/z	Abundance
36.10	608.0
37.10	2545.0
38.00	2350.0
39.00	1017.0
40.00	237.0
44.00	619.0
45.00	545.0
46.00	122.0
47.00	681.0
48.00	381.0
49.00	2393.0
50.10	10730.0
51.00	3004.0
52.00	186.0
52.90	148.0
55.10	222.0
56.00	999.0
57.00	1875.0
60.00	549.0
61.00	3165.0
62.10	3032.0
63.00	2628.0
64.00	456.0
65.00	430.0
68.10	6689.0
69.10	5837.0
70.10	511.0
72.00	296.0
73.00	2557.0
74.10	10733.0
75.10	31704.0
76.10	2511.0
77.00	409.0
77.90	304.0
79.00	2656.0
80.00	696.0
81.00	2683.0
82.00	624.0
87.00	2477.0
88.00	2788.0
90.90	253.0
92.00	1992.0
93.00	2674.0
94.10	7137.0
95.10	60768.0
96.10	4089.0
103.80	424.0
104.90	122.0
105.90	336.0
107.00	159.0
111.00	105.0
112.00	114.0
115.90	263.0
116.90	559.0
117.90	299.0
118.90	443.0
127.90	271.0
129.00	172.0
129.80	227.0
130.90	134.0
134.80	118.0
136.90	108.0
140.90	824.0
141.90	117.0
143.00	1063.0
144.90	396.0
145.80	164.0
148.00	159.0
154.80	164.0
171.00	140.0
172.00	731.0
174.00	48816.0
175.00	3883.0
176.00	47096.0
177.00	3183.0
178.00	107.0

Instrument :
MSVOA_V
ClientSampleId :
BFB295

m/z	Abundance
36.10	626.0
37.10	2568.0
38.10	2558.0
39.00	1141.0
40.00	275.0
44.00	728.0
45.10	555.0
45.90	140.0
47.00	696.0
48.00	307.0
49.00	2458.0
50.10	11295.0
51.00	3346.0
52.00	202.0
52.90	160.0
55.00	221.0
56.00	992.0
57.00	1995.0
58.00	106.0
60.00	601.0
61.00	2963.0
62.10	3163.0
63.10	2788.0
64.00	465.0
64.90	443.0
68.10	7060.0
69.10	6143.0
70.10	650.0
71.90	309.0
73.00	2650.0
74.10	11116.0
75.10	33632.0
76.10	2532.0
77.10	407.0
77.80	267.0
79.00	2826.0
80.00	707.0
81.00	2912.0
81.90	634.0
87.00	2437.0
88.00	2766.0
91.00	259.0
92.10	2064.0
93.00	2918.0
94.00	7778.0
95.10	65296.0
96.10	4145.0
97.20	113.0
103.80	472.0
104.90	125.0
105.90	375.0
106.90	129.0
112.00	134.0
114.80	100.0
115.90	290.0
116.90	630.0
117.90	322.0
118.90	393.0
127.90	297.0
128.80	173.0
129.80	262.0
130.90	144.0
134.90	121.0
136.90	135.0
140.90	851.0
143.00	1257.0
144.90	395.0
145.80	197.0
148.00	152.0
154.80	177.0
171.00	141.0
172.00	927.0
173.10	974.0
174.00	54064.0
175.00	4139.0
176.00	51528.0
177.00	3474.0
178.00	112.0

Instrument :
MSVOA_V
ClientSampleId :
BFB295

m/z	Abundance
36.10	565.0
37.10	2389.0
38.10	2517.0
39.10	1103.0
40.00	280.0
44.00	818.0
45.10	495.0
45.90	154.0
47.00	607.0
48.00	254.0
49.00	2295.0
50.00	10656.0
51.00	3356.0
52.10	208.0
52.90	140.0
55.00	192.0
56.00	970.0
57.00	1828.0
57.90	116.0
60.00	645.0
61.00	2660.0
62.10	3087.0
63.10	2702.0
63.90	395.0
64.90	457.0
67.10	232.0
68.10	6445.0
69.10	6081.0
70.10	678.0
71.90	323.0
73.00	2581.0
74.00	10345.0
75.10	31632.0
76.10	2278.0
77.00	365.0
78.00	253.0
79.00	2613.0
80.00	758.0
81.00	2773.0
81.90	639.0
87.00	2253.0
88.00	2442.0
91.00	261.0
92.10	1889.0
93.00	3034.0
94.00	7685.0
95.10	62688.0
96.10	3872.0
97.10	120.0
103.90	399.0
104.90	107.0
106.00	378.0
106.90	104.0
112.10	103.0
113.00	101.0
114.70	101.0
116.00	293.0
116.90	594.0
118.00	322.0
118.90	322.0
128.00	277.0
128.70	173.0
129.80	248.0
130.90	118.0
136.90	159.0
140.90	705.0
143.00	1274.0
144.80	379.0
145.80	185.0
148.00	147.0
154.90	163.0
157.20	114.0
159.00	109.0
171.10	115.0
172.00	979.0
173.10	876.0
174.00	54088.0
175.00	4072.0
176.00	50816.0
177.00	3429.0
177.90	120.0

Instrument :
MSVOA_V
ClientSampleId :
BFB295