




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040622\
 Data File : VV025369.D
 Acq On : 06 Apr 2022 17:22
 Operator : SY/MD
 Sample : N2291-03
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B30

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 04/07/2022
 Supervised By :Mahesh Dadoda 04/07/2022

Quant Time: Apr 07 01:28:19 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Apr 07 01:24:47 2022
 Response via : Initial Calibration

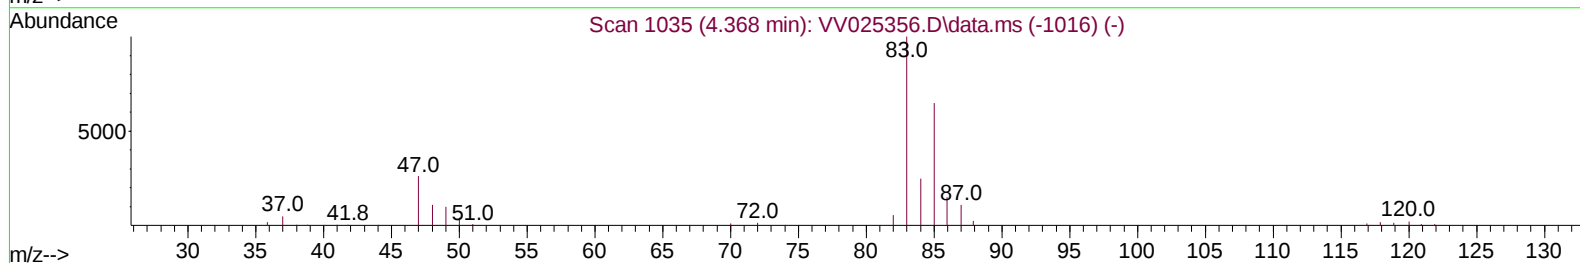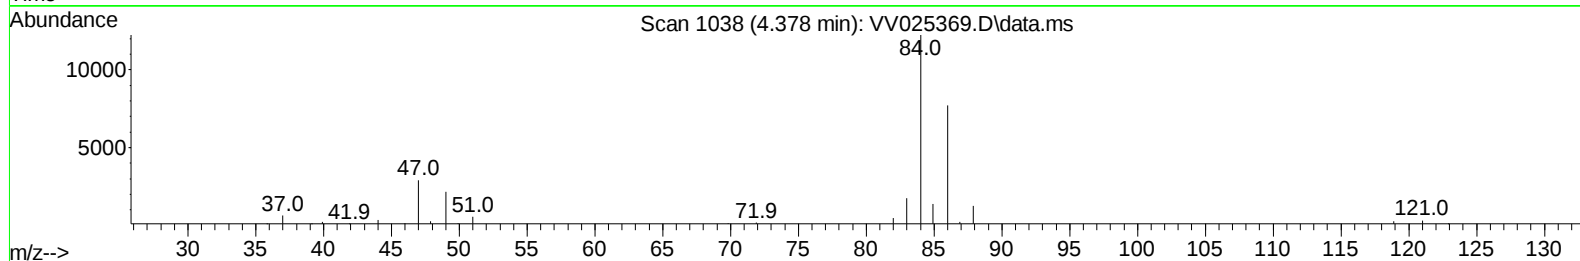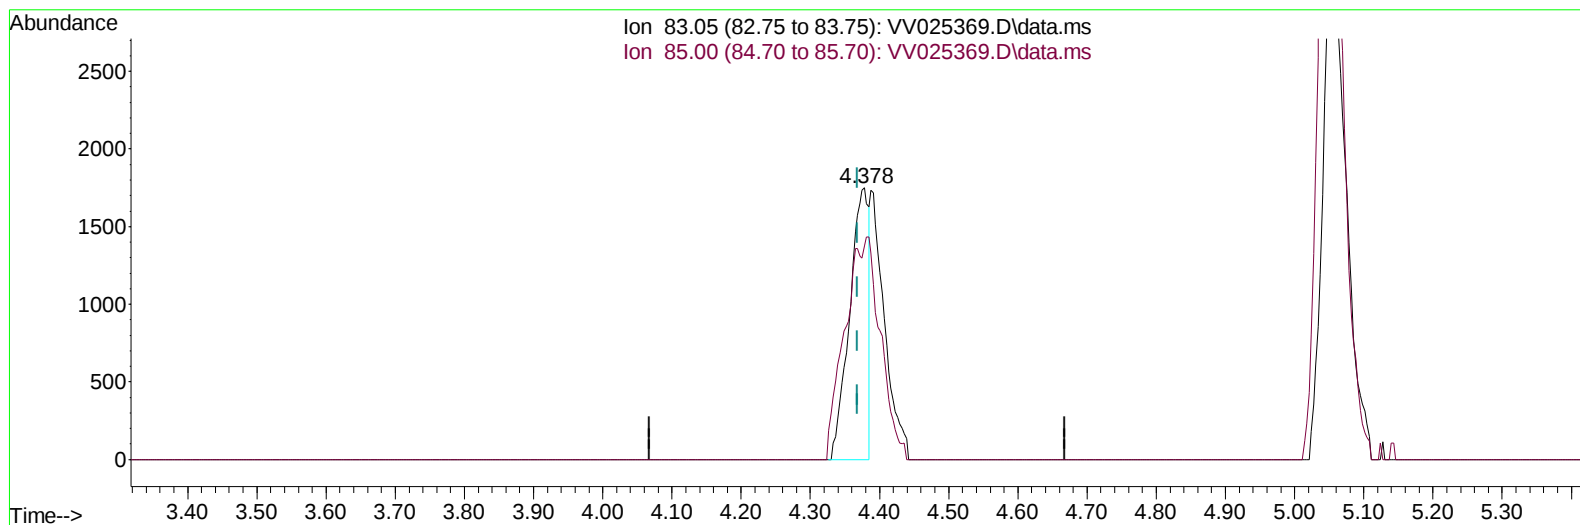

TIC: VV025369.D\data.ms

(25) Chloroform (T)

4.378min (+ 0.010) 0.16 ug/L

response 3321

Ion	Exp%	Act%
83.05	100.00	100.00
85.00	63.80	78.73
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040622\
 Data File : VV025369.D
 Acq On : 06 Apr 2022 17:22
 Operator : SY/MD
 Sample : N2291-03
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B30

Manual IntegrationsAPPROVED

Quant Time: Apr 07 01:28:19 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Apr 07 01:24:47 2022
 Response via : Initial Calibration

Reviewed By :John Carlone 04/07/2022
 Supervised By :Mahesh Dadoda 04/07/2022

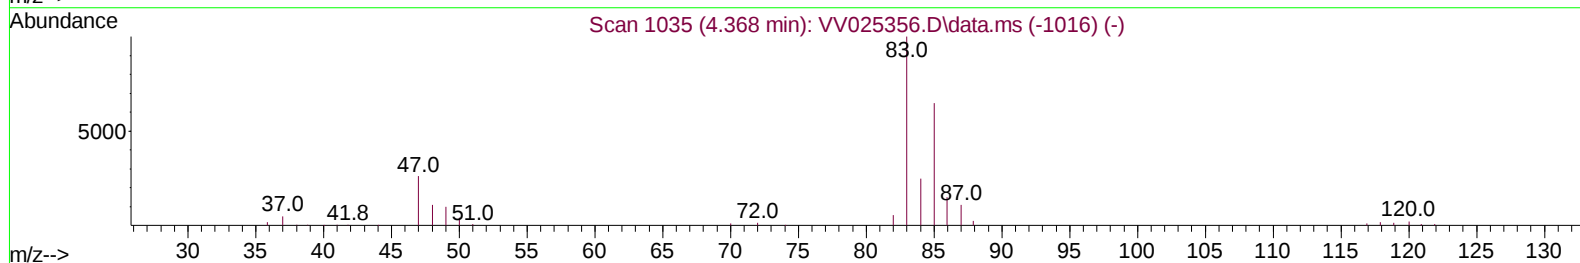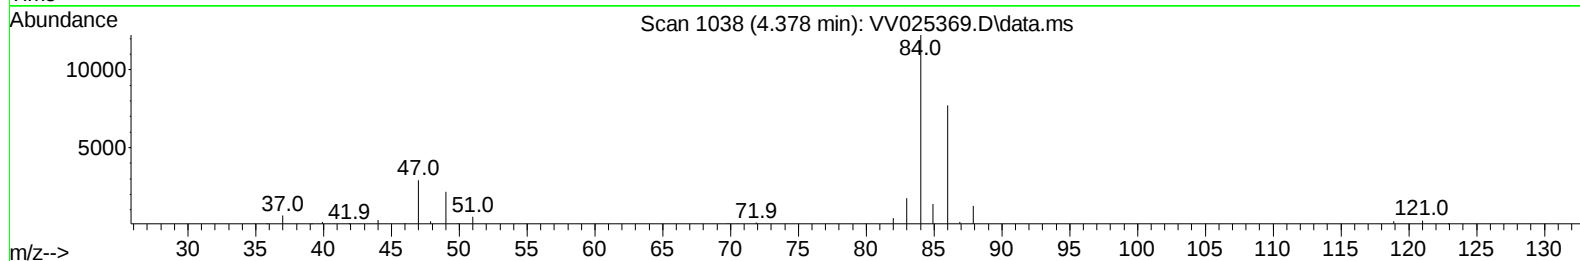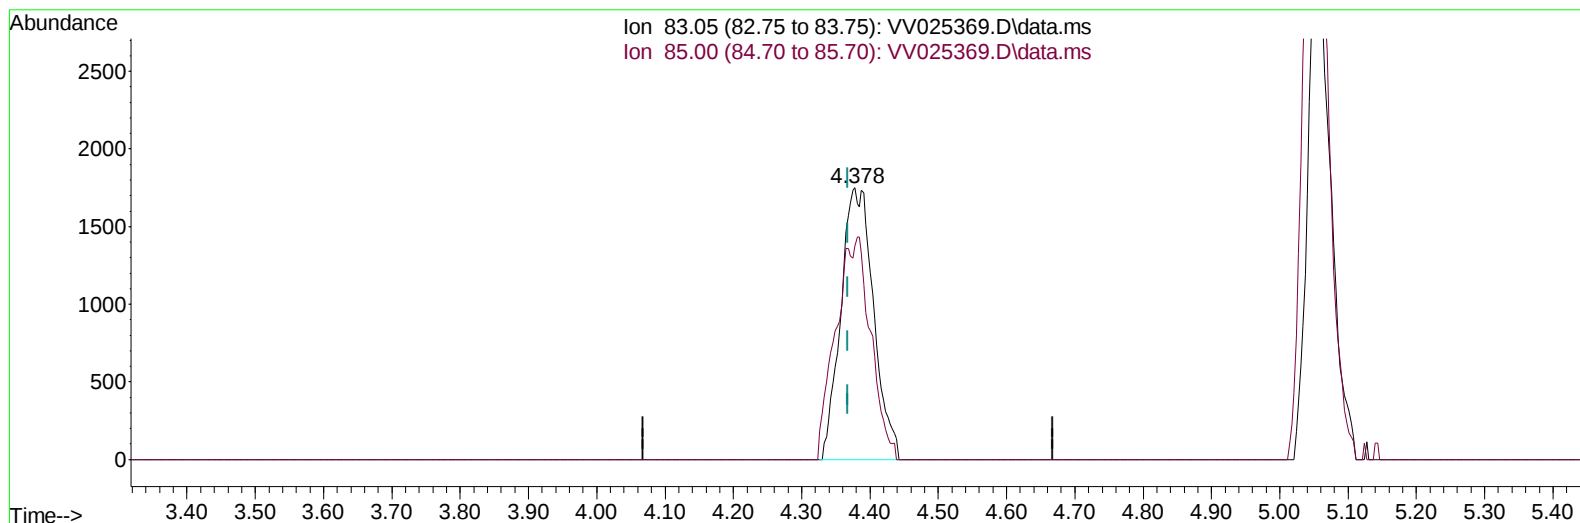

TIC: VV025369.D\data.ms

(25) Chloroform (T)

4.378min (+ 0.010) 0.28 ug/L m

response 5814

Ion	Exp%	Act%
83.05	100.00	100.00
85.00	63.80	78.73
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040622\
 Data File : VV025369.D
 Acq On : 06 Apr 2022 17:22
 Operator : SY/MD
 Sample : N2291-03
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B30

Manual IntegrationsAPPROVED

Quant Time: Apr 07 01:28:19 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Apr 07 01:24:47 2022
 Response via : Initial Calibration

Reviewed By :John Carlone 04/07/2022
 Supervised By :Mahesh Dadoda 04/07/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	157354	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	150750	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	68880	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	56186	3.823	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130	Recovery	=	76.400%	
7) Chloroethane-d5	1.568	69	58034	4.704	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130	Recovery	=	94.000%	
11) 1,1-Dichloroethene-d2	2.108	63	89938	2.825	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125	Recovery	=	56.400%#	
20) 2-Butanone-d5	3.883	46	92462	63.152	ug/L	0.00
Spiked Amount 50.000	Range 40	- 130	Recovery	=	126.300%	
24) Chloroform-d	4.352	84	99568	5.191	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	103.800%	
26) 1,2-Dichloroethane-d4	5.034	65	45048	5.313	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	106.200%	
32) Benzene-d6	5.050	84	194780	5.107	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	102.200%	
36) 1,2-Dichloropropane-d6	6.069	67	59824	5.597	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140	Recovery	=	112.000%	
41) Toluene-d8	7.317	98	168523	4.818	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	96.400%	
43) trans-1,3-Dichloroprop...	7.625	79	16515	4.736	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130	Recovery	=	94.800%	
46) 2-Hexanone-d5	8.088	63	77308	61.388	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130	Recovery	=	122.780%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	38770	5.440	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120	Recovery	=	108.800%	
66) 1,2-Dichlorobenzene-d4	11.622	152	62242	5.626	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120	Recovery	=	112.600%	
Target Compounds						
						Qvalue
9) Trichlorofluoromethane	1.754	101	361701	12.923	ug/L	99
22) cis-1,2-Dichloroethene	3.915	96	24506	2.121	ug/L	96
25) Chloroform	4.378	83	5814m	0.276	ug/L	
31) Carbon tetrachloride	4.831	117	5115	0.324	ug/L	93
34) Trichloroethene	5.915	95	81543	6.716	ug/L	96
45) 1,1,2-Trichloroethane	7.851	97	1145	0.163	ug/L	86
47) Tetrachloroethene	7.973	164	349864	39.076	ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040622\
Data File : VV025369.D
Acq On : 06 Apr 2022 17:22
Operator : SY/MD
Sample : N2291-03
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B30

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 04/07/2022
Supervised By :Mahesh Dadoda 04/07/2022

Quant Time: Apr 07 01:28:19 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Apr 07 01:24:47 2022
Response via : Initial Calibration

