

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW040622\
 Data File : VW025360.D
 Acq On : 06 Apr 2022 13:51
 Operator : SY/MD
 Sample : N2289-01
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFFC6

Quant Time: Apr 07 01:26:23 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Apr 07 01:24:47 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	167954	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	160014	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	71055	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	56496	3.601	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	72.000%	
7) Chloroethane-d5	1.568	69	59774	4.540	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	90.800%	
11) 1,1-Dichloroethene-d2	2.108	63	90840	2.673	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	53.400%#	
20) 2-Butanone-d5	3.883	46	83287	53.296	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	106.600%	
24) Chloroform-d	4.352	84	99829	4.876	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	97.600%	
26) 1,2-Dichloroethane-d4	5.034	65	44014	4.864	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	97.200%	
32) Benzene-d6	5.050	84	184709	4.563	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	91.200%	
36) 1,2-Dichloropropane-d6	6.069	67	55757	4.915	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	98.200%	
41) Toluene-d8	7.317	98	157706	4.247	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	85.000%	
43) trans-1,3-Dichloroprop...	7.625	79	17062	4.610	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	92.200%	
46) 2-Hexanone-d5	8.088	63	65787	49.215	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	98.440%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	37670	4.980	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	99.600%	
66) 1,2-Dichlorobenzene-d4	11.622	152	58021	5.084	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	101.600%	
Target Compounds					Qvalue	
25) Chloroform	4.381	83	31966	1.422	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040622\
Data File : VV025360.D
Acq On : 06 Apr 2022 13:51
Operator : SY/MD
Sample : N2289-01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFFC6

Quant Time: Apr 07 01:26:23 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Apr 07 01:24:47 2022
Response via : Initial Calibration

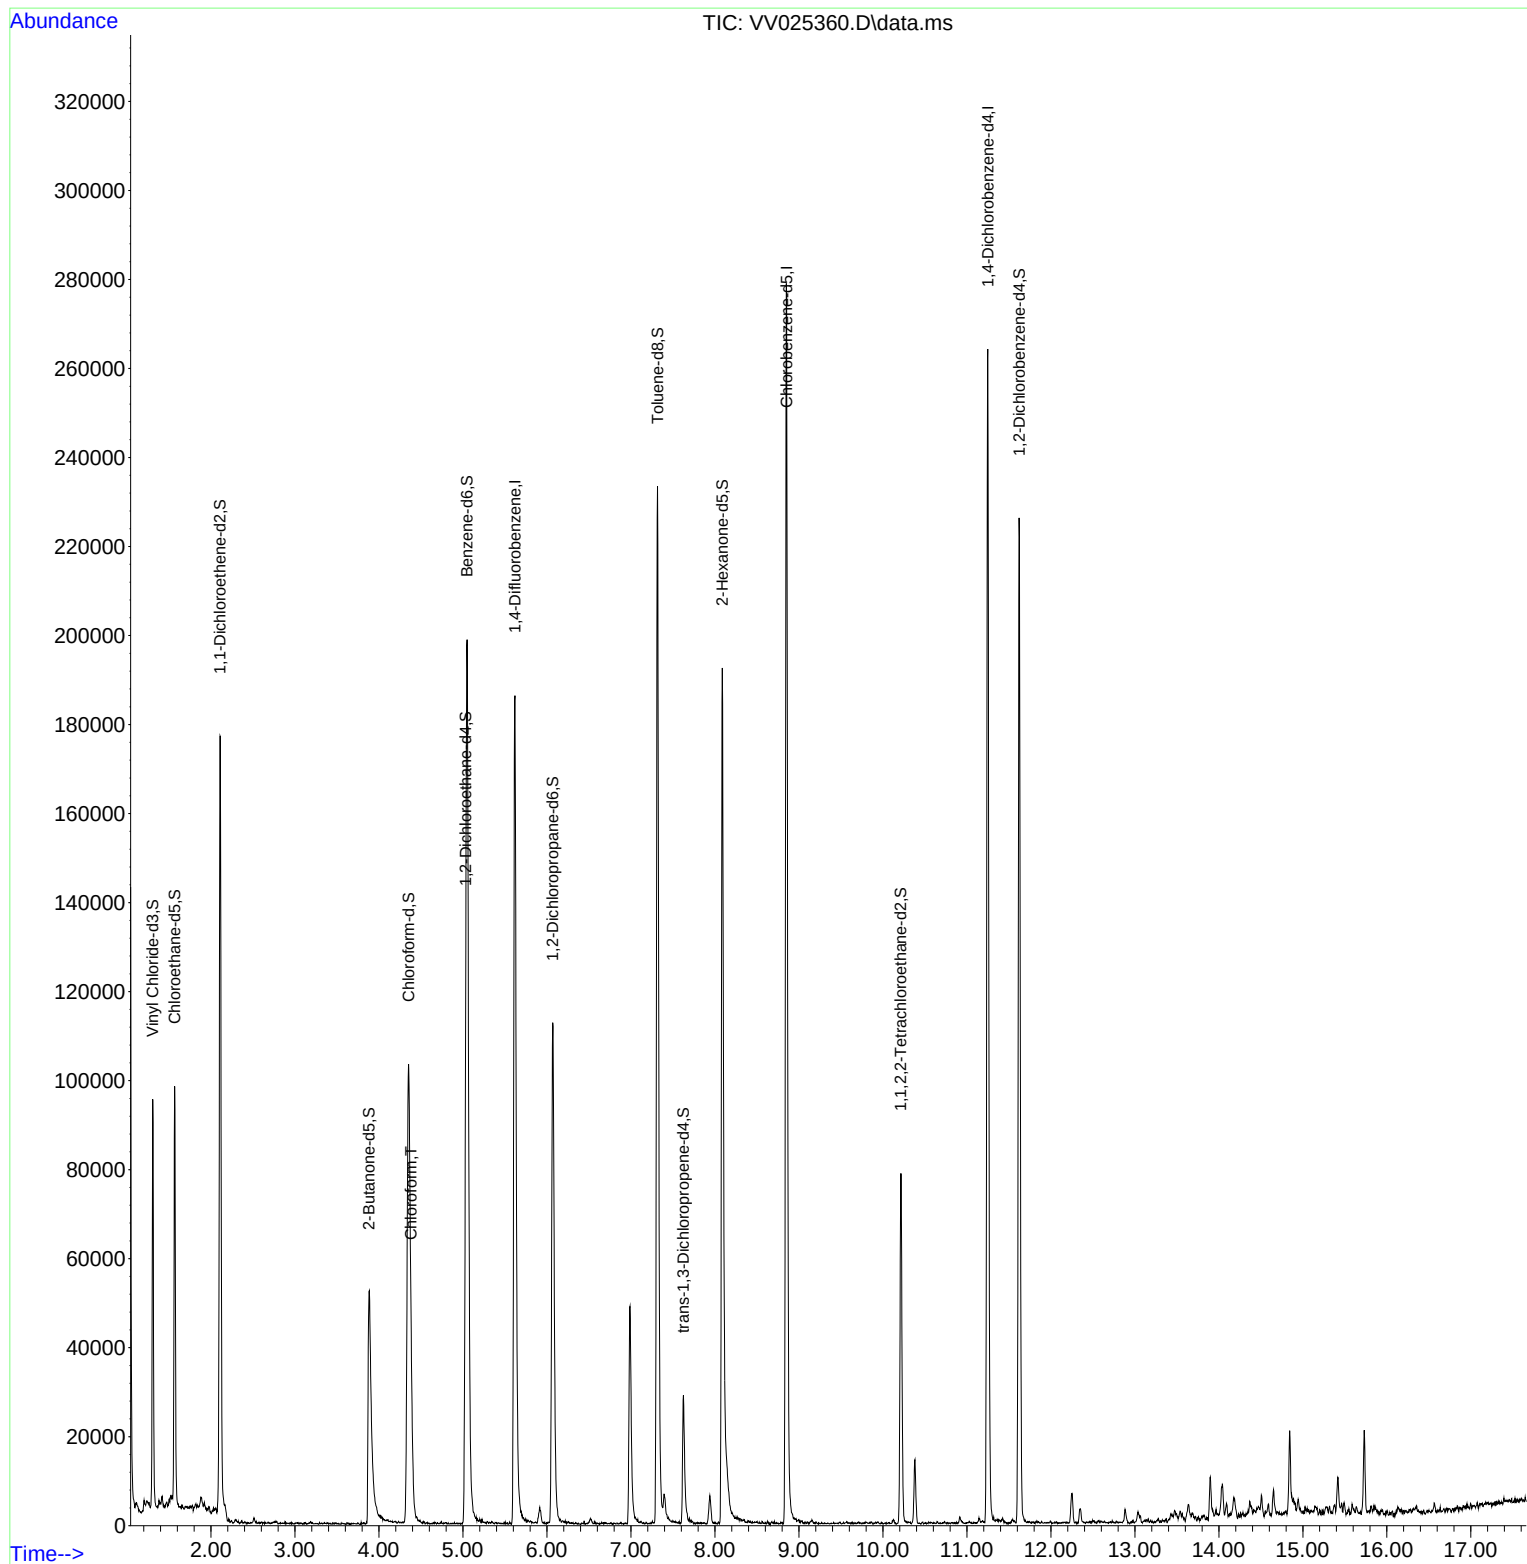

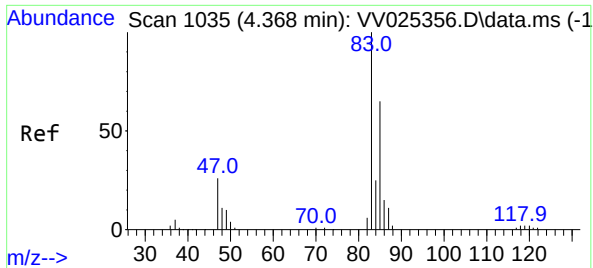

#25
 Chloroform
 Concen: 1.422 ug/L
 RT: 4.381 min Scan# 10
 Delta R.T. 0.013 min
 Lab File: VV025360.D
 Acq: 06 Apr 2022 13:51

Instrument :
 MSVOA_V
 ClientSampleId :
 BFFC6

Tgt Ion: 83 Resp: 31966

Ion	Ratio	Lower	Upper
83	100		
85	61.7	44.7	82.9

