

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW040622\
 Data File : VW025361.D
 Acq On : 06 Apr 2022 14:14
 Operator : SY/MD
 Sample : N2289-03
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFFD0

Quant Time: Apr 07 01:26:35 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Apr 07 01:24:47 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	143770	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	138092	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	60461	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	51983	3.871	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	77.400%	
7) Chloroethane-d5	1.568	69	51727	4.589	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	91.800%	
11) 1,1-Dichloroethene-d2	2.108	63	82038	2.820	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	56.400%#	
20) 2-Butanone-d5	3.883	46	74272	55.521	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	111.040%	
24) Chloroform-d	4.349	84	87286	4.980	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	99.600%	
26) 1,2-Dichloroethane-d4	5.034	65	39560	5.107	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	102.200%	
32) Benzene-d6	5.050	84	166435	4.764	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	95.200%	
36) 1,2-Dichloropropane-d6	6.069	67	50199	5.127	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	102.600%	
41) Toluene-d8	7.317	98	138215	4.313	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	86.200%	
43) trans-1,3-Dichloroprop...	7.625	79	15027	4.705	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	94.000%	
46) 2-Hexanone-d5	8.088	63	57666	49.989	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	99.980%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	33455	5.125	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	102.400%	
66) 1,2-Dichlorobenzene-d4	11.622	152	51001	5.252	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	105.000%	
Target Compounds						
					Qvalue	
13) Acetone	2.166	43	4248	4.162	ug/L	91
25) Chloroform	4.375	83	12724	0.661	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040622\
Data File : VV025361.D
Acq On : 06 Apr 2022 14:14
Operator : SY/MD
Sample : N2289-03
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFFD0

Quant Time: Apr 07 01:26:35 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Apr 07 01:24:47 2022
Response via : Initial Calibration




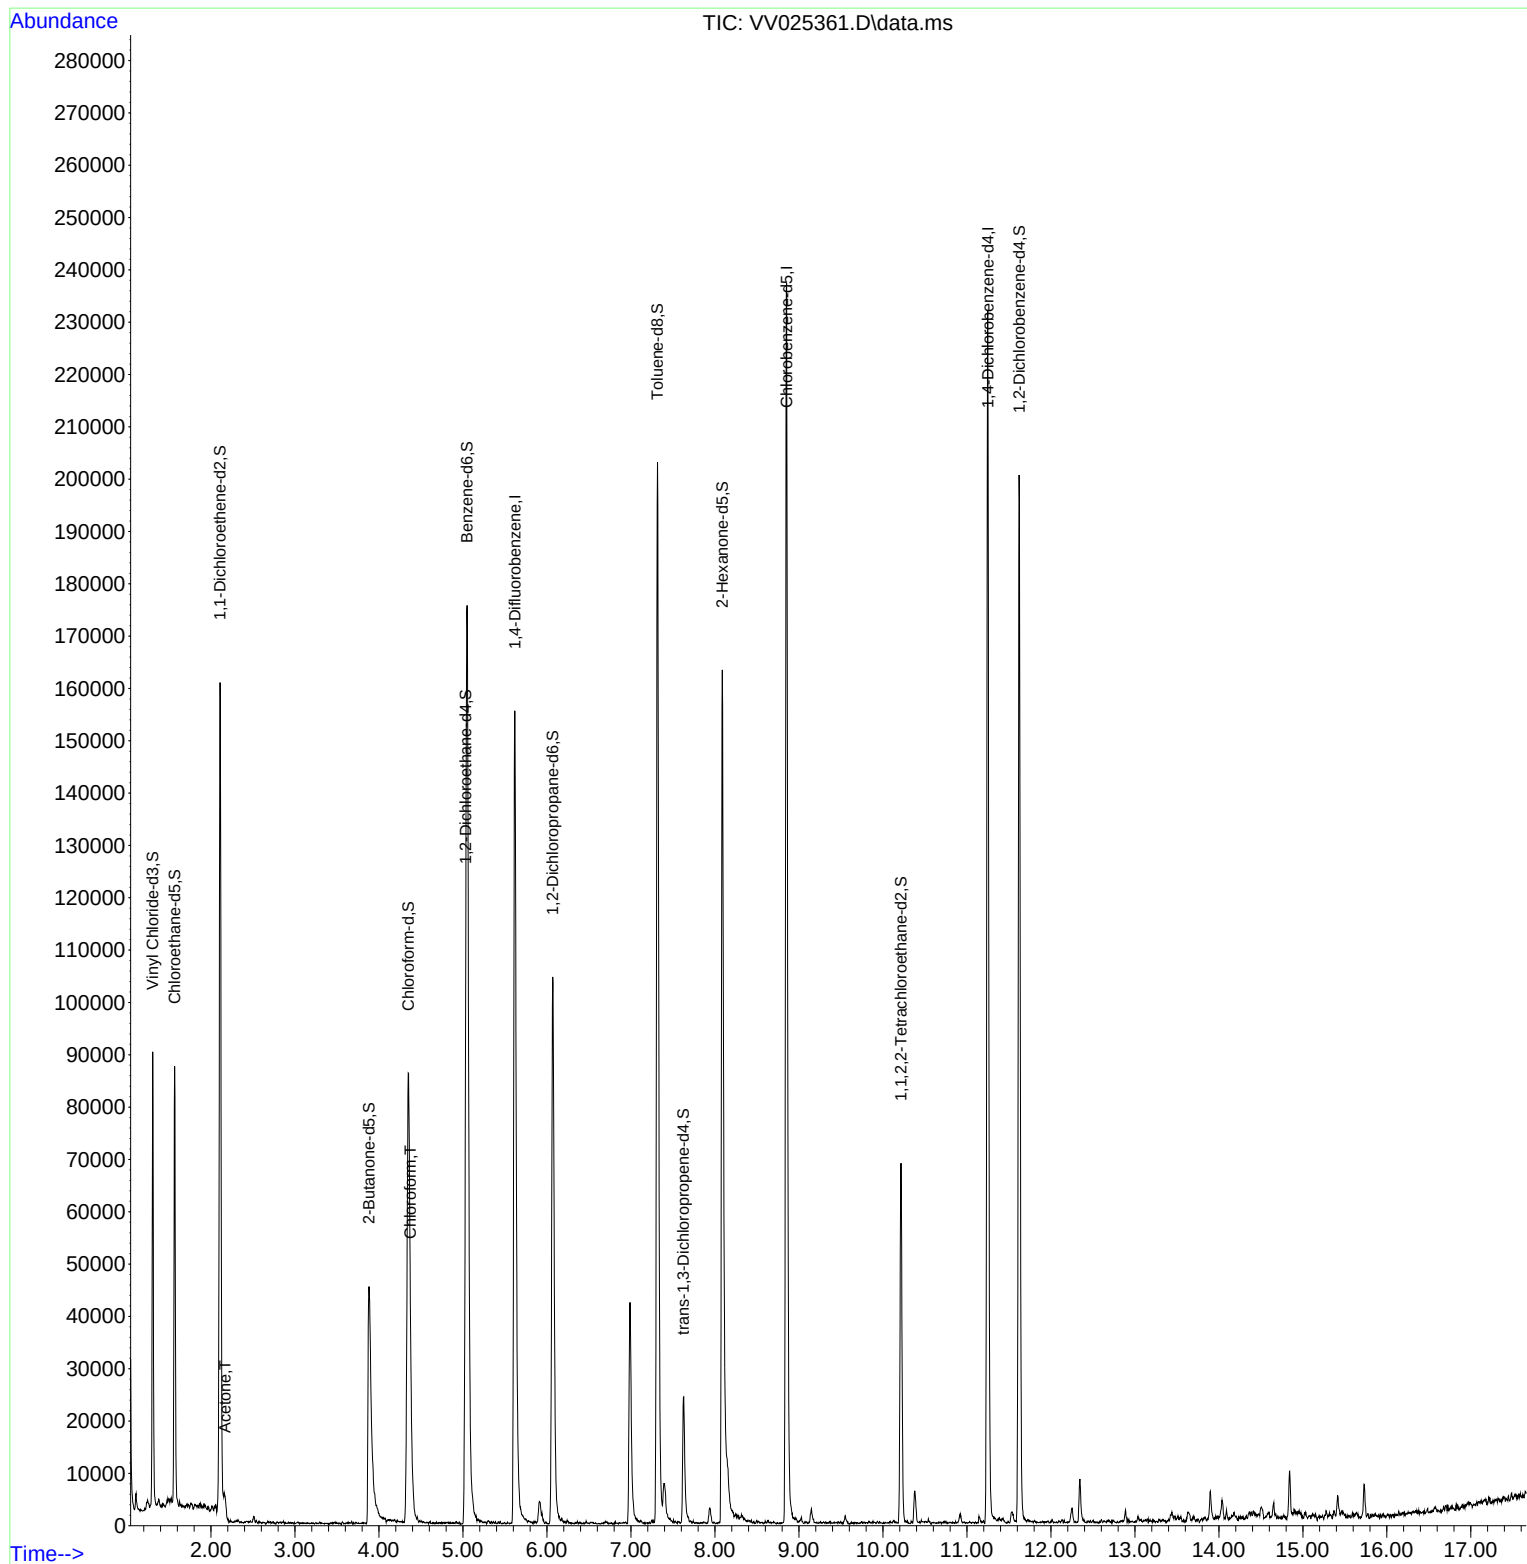


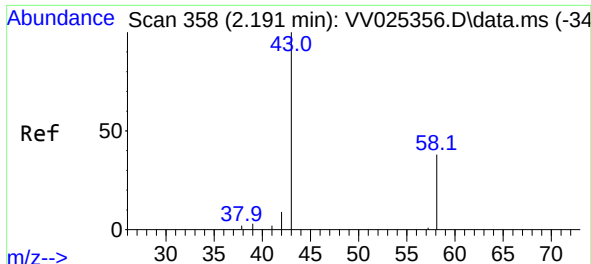

#13
Acetone
Concen: 4.162 ug/L
RT: 2.166 min Scan# 31
Delta R.T. -0.026 min
Lab File: VV025361.D
Acq: 06 Apr 2022 14:14

Instrument :
MSVOA_V
ClientSampleId :
BFFD0

Tgt Ion: 43 Resp: 4248
Ion Ratio Lower Upper
43 100
58 30.0 0.0 51.2

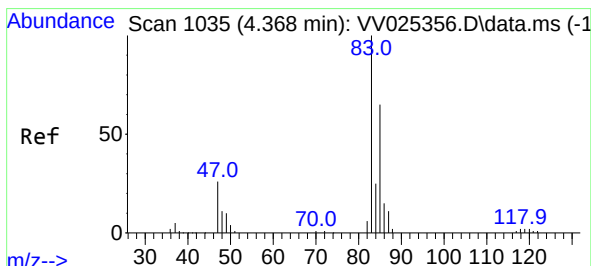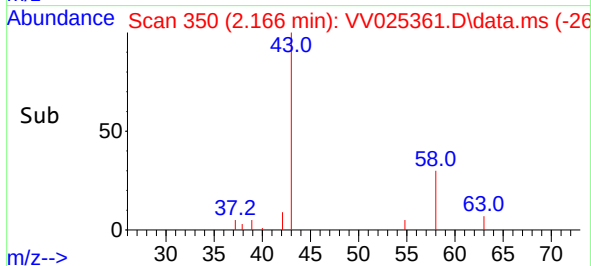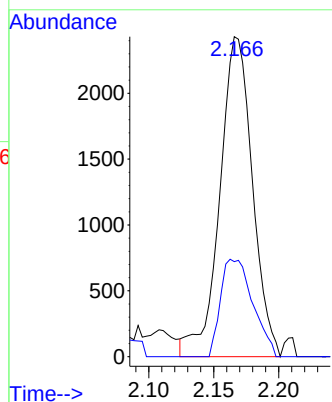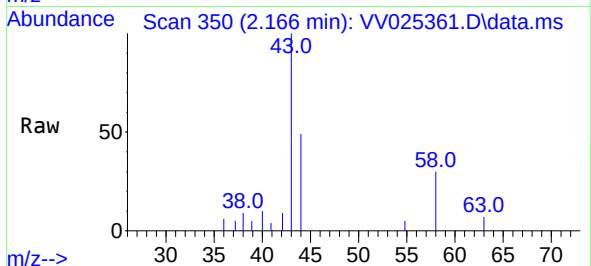

#25
Chloroform
Concen: 0.661 ug/L
RT: 4.375 min Scan# 1037
Delta R.T. 0.007 min
Lab File: VV025361.D
Acq: 06 Apr 2022 14:14

Tgt Ion: 83 Resp: 12724
Ion Ratio Lower Upper
83 100
85 65.2 44.7 82.9

