

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW040622\
 Data File : VW025373.D
 Acq On : 06 Apr 2022 18:56
 Operator : SY/MD
 Sample : N2291-07
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B34

Quant Time: Apr 07 01:29:14 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Apr 07 01:24:47 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	161755	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	156532	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	66838	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	56567	3.744	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	74.800%
7) Chloroethane-d5	1.568	69	57945	4.569	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	91.400%
11) 1,1-Dichloroethene-d2	2.108	63	89169	2.725	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	54.400%#
20) 2-Butanone-d5	3.883	46	88119	58.548	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	117.100%
24) Chloroform-d	4.352	84	98800	5.011	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.200%
26) 1,2-Dichloroethane-d4	5.034	65	45444	5.214	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	104.200%
32) Benzene-d6	5.050	84	192963	4.873	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.400%
36) 1,2-Dichloropropane-d6	6.069	67	56659	5.105	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	102.200%
41) Toluene-d8	7.317	98	164913	4.540	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	90.800%
43) trans-1,3-Dichloroprop...	7.625	79	16543	4.569	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	91.400%
46) 2-Hexanone-d5	8.088	63	68821	52.630	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	105.260%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	38309	5.177	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	103.600%
66) 1,2-Dichlorobenzene-d4	11.622	152	61326	5.713	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	114.200%
Target Compounds						Qvalue
47) Tetrachloroethene	7.982	164	1882	0.202	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040622\
Data File : VV025373.D
Acq On : 06 Apr 2022 18:56
Operator : SY/MD
Sample : N2291-07
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B34


Quant Time: Apr 07 01:29:14 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Apr 07 01:24:47 2022
Response via : Initial Calibration

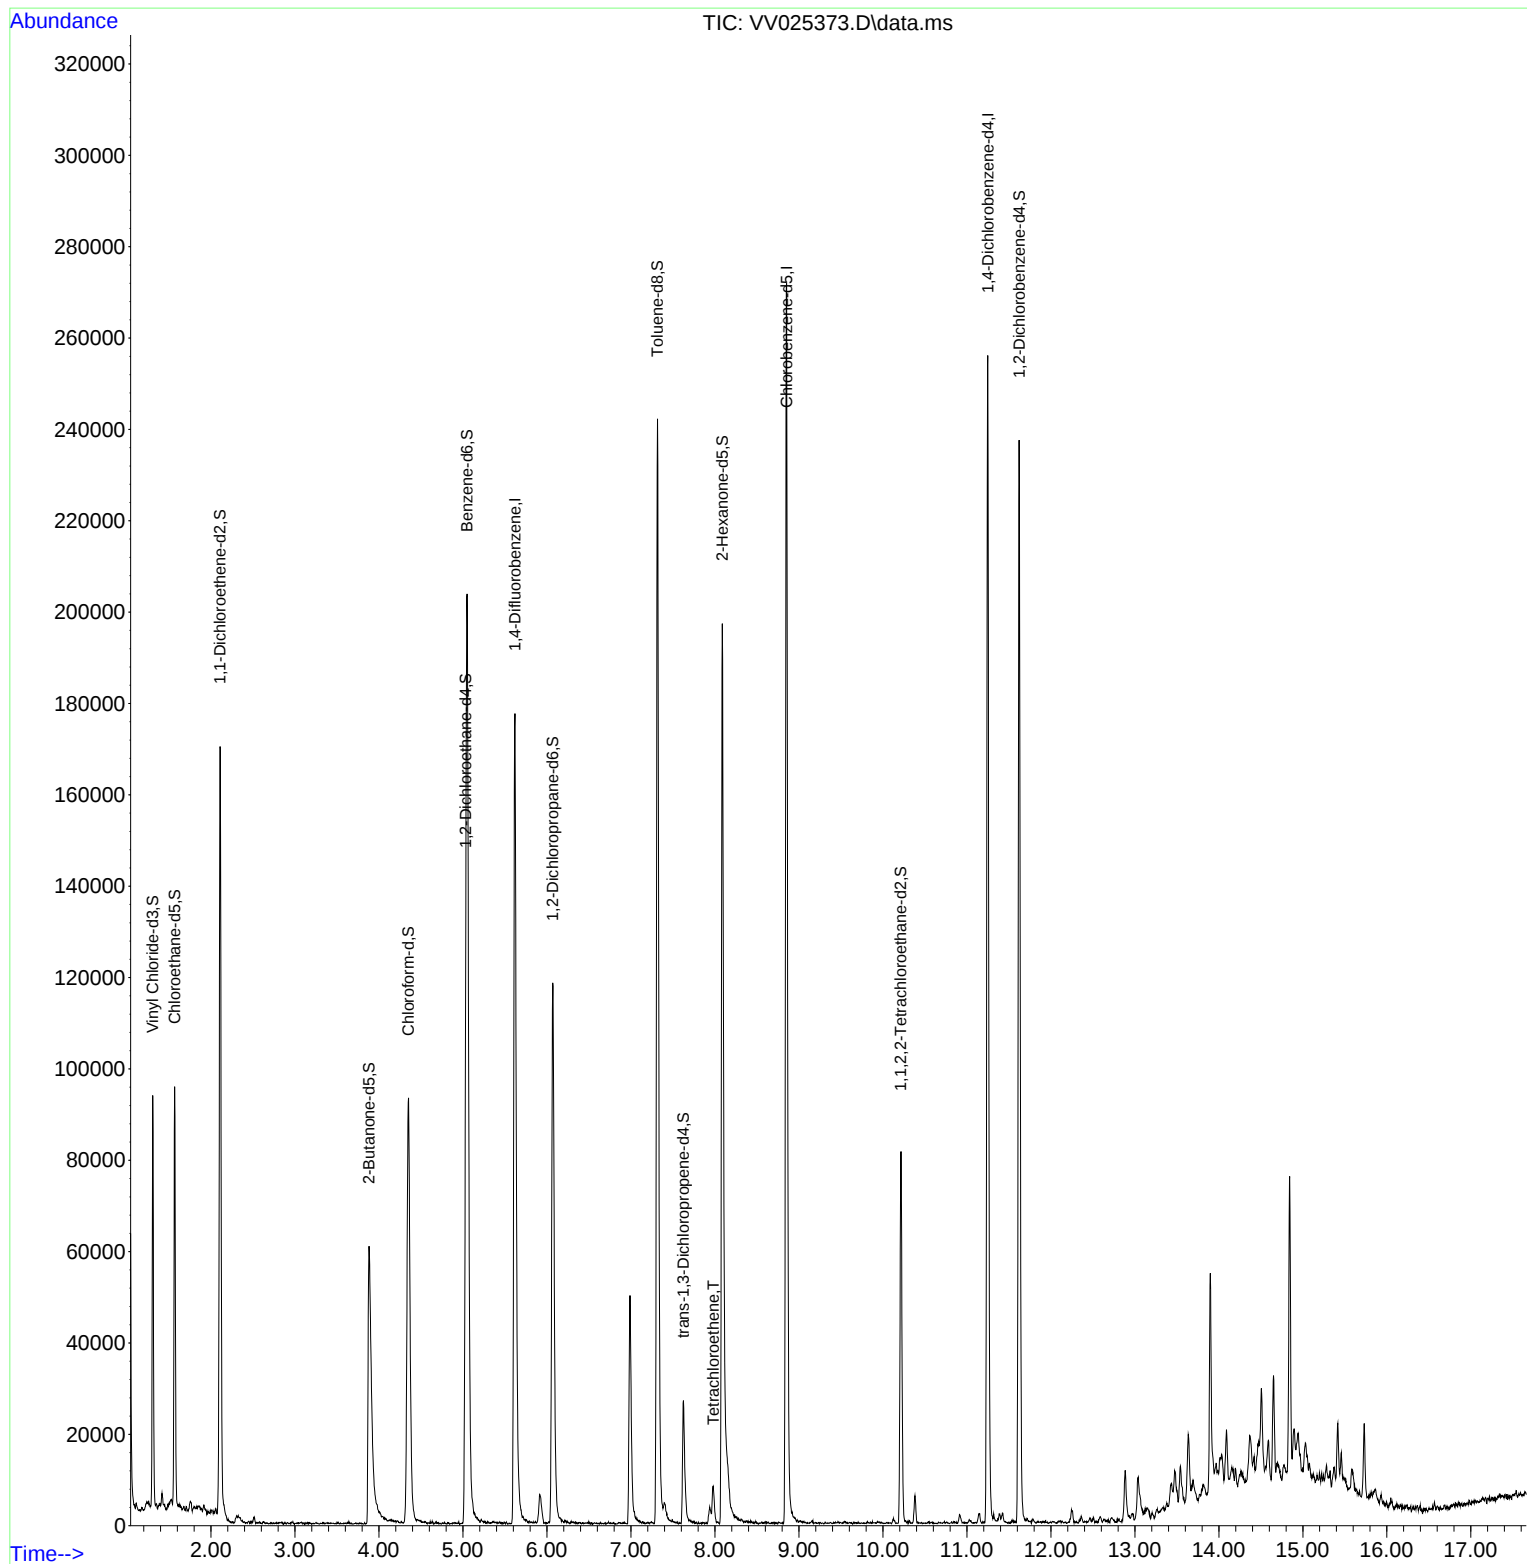

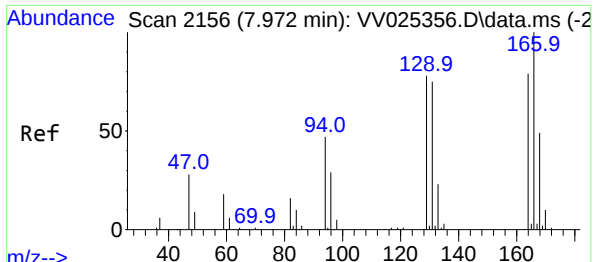

#47
Tetrachloroethene
Concen: 0.202 ug/L
RT: 7.982 min Scan# 21
Delta R.T. 0.010 min
Lab File: VV025373.D
Acq: 06 Apr 2022 18:56

Instrument :
MSVOA_V
ClientSampleId :
C0B34

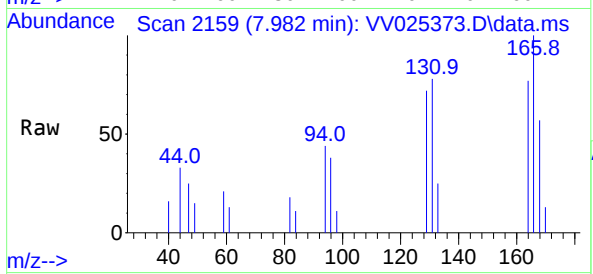

Tgt Ion:	164	Resp:	1882
Ion	Ratio	Lower	Upper
164	100		
129	93.4	67.5	125.4
131	101.1	68.0	126.4
166	130.4	86.2	160.2

