

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040622\
 Data File : VV025357.D
 Acq On : 06 Apr 2022 11:50
 Operator : SY/MD
 Sample : VV0406WBL01
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK335

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV025357.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	95	rVB	82932	84589	20.94%	2.466%
2	1.568	156	164	178	rVB	76469	89482	22.16%	2.609%
3	2.108	321	332	359	rVB	154417	232982	57.69%	6.793%
4	2.507	446	456	469	rVB	13449	23389	5.79%	0.682%
5	3.896	877	888	922	rBV2	28774	111385	27.58%	3.248%
6	4.346	1009	1028	1058	rBV2	74725	194440	48.14%	5.670%
7	5.043	1229	1245	1272	rBV2	161450	403873	100.00%	11.776%
8	5.613	1410	1422	1443	rBV	141753	292790	72.50%	8.537%
9	6.066	1546	1563	1584	rBV2	93348	194653	48.20%	5.676%
10	6.986	1839	1849	1872	rBV	37526	73619	18.23%	2.147%
11	7.313	1940	1951	1970	rBV	181368	320385	79.33%	9.342%
12	7.625	2039	2048	2071	rBV2	22376	41488	10.27%	1.210%
13	8.088	2180	2192	2229	rBV	137064	292799	72.50%	8.538%
14	8.850	2418	2429	2449	rBV	222014	366038	90.63%	10.673%
15	10.214	2841	2853	2865	rBV	63724	101007	25.01%	2.945%
16	11.246	3163	3174	3193	rBV	201776	316471	78.36%	9.228%
17	11.622	3279	3291	3309	rBV	172307	276719	68.52%	8.069%
18	12.249	3476	3486	3496	rBV2	3391	5545	1.37%	0.162%
19	14.040	4032	4043	4053	rBV2	4750	7885	1.95%	0.230%




Sum of corrected areas: 3429539

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040622\
Data File : VV025357.D
Acq On : 06 Apr 2022 11:50
Operator : SY/MD
Sample : VV0406WBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK335

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

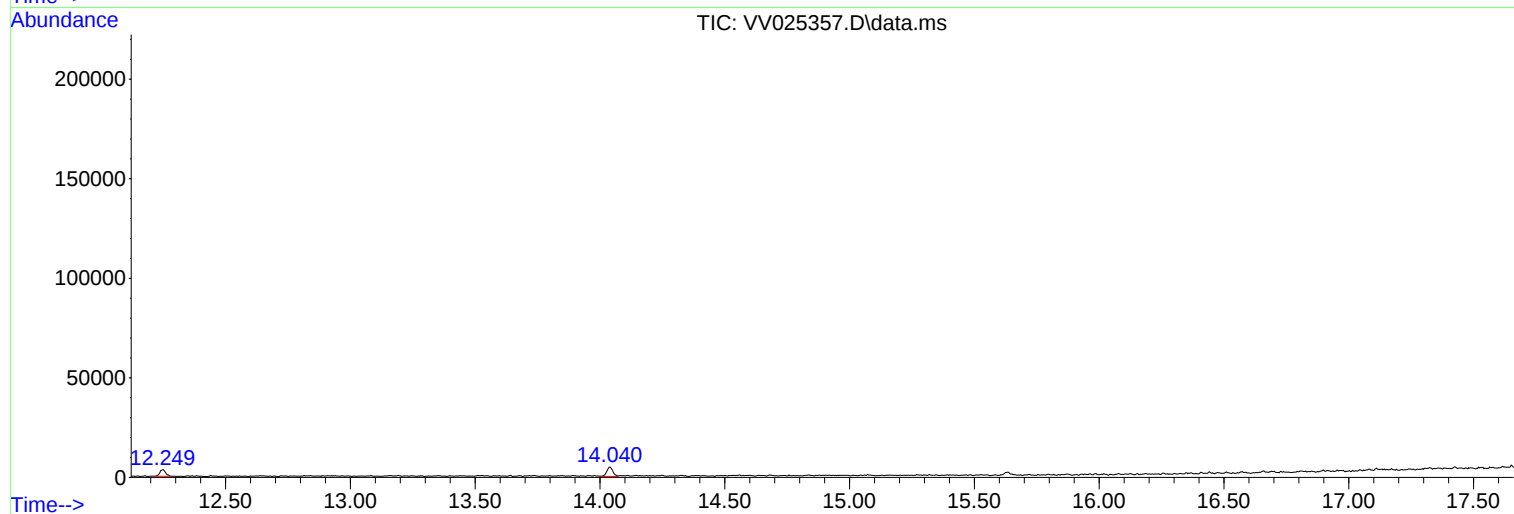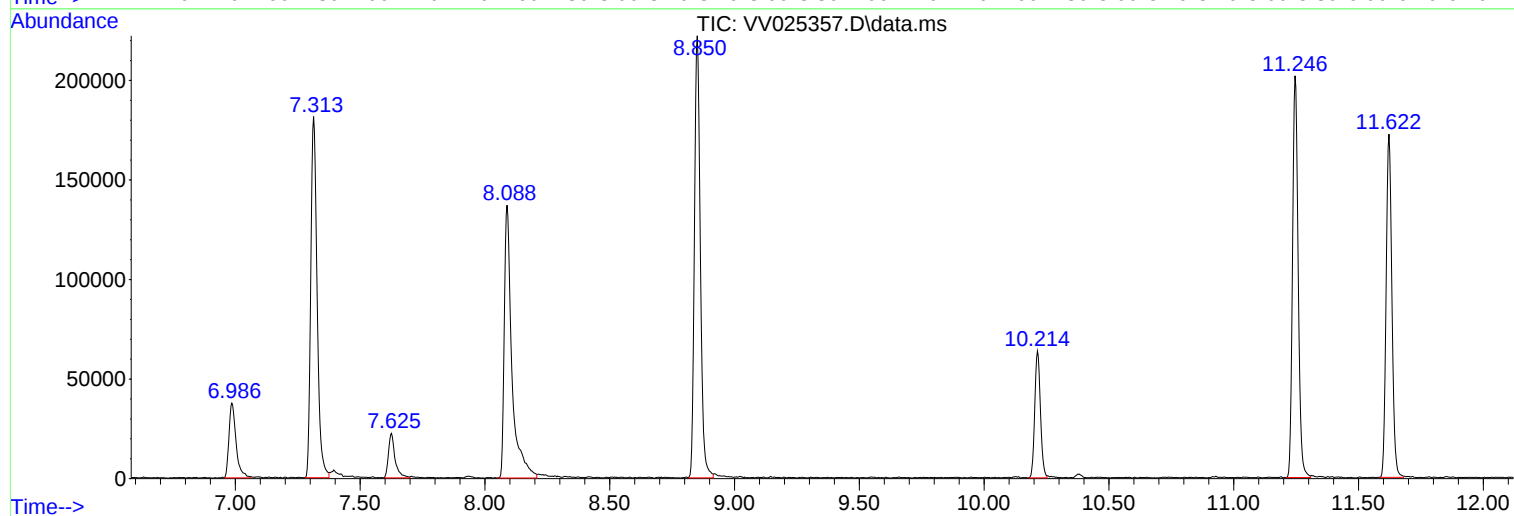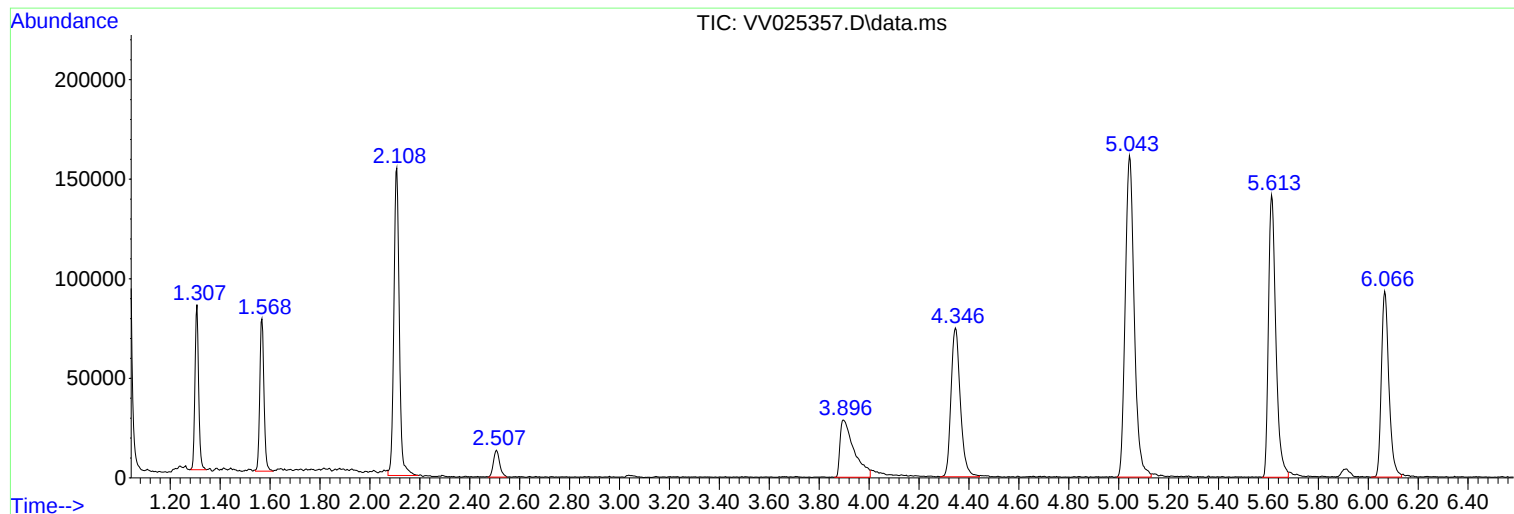

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040622\
Data File : VV025357.D
Acq On : 06 Apr 2022 11:50
Operator : SY/MD
Sample : VV0406WBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK335

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040622\
Data File : VV025357.D
Acq On : 06 Apr 2022 11:50
Operator : SY/MD
Sample : VV0406WBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK335

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc