

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040622\
 Data File : VV025361.D
 Acq On : 06 Apr 2022 14:14
 Operator : SY/MD
 Sample : N2289-03
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFFD0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV025361.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	98	rVB	86694	84956	19.05%	2.224%
2	1.568	157	164	180	rVB	84068	95648	21.44%	2.504%
3	2.108	320	332	346	rBV	158585	233953	52.45%	6.125%
4	3.883	873	884	909	rBV	45360	126629	28.39%	3.315%
5	4.349	1013	1029	1060	rBV2	85955	236537	53.03%	6.192%
6	5.050	1230	1247	1274	rBV3	175487	446044	100.00%	11.677%
7	5.616	1413	1423	1444	rBV	155088	317242	71.12%	8.305%
8	6.069	1550	1564	1586	rBV	104575	216253	48.48%	5.661%
9	6.989	1840	1850	1867	rBV2	42322	80739	18.10%	2.114%
10	7.317	1939	1952	1970	rBV	202677	358561	80.39%	9.387%
11	7.629	2036	2049	2064	rBV2	24234	44056	9.88%	1.153%
12	7.940	2137	2146	2155	rVB3	2894	4962	1.11%	0.130%
13	8.088	2182	2192	2231	rBV	163026	326283	73.15%	8.542%
14	8.854	2417	2430	2454	rBV	236815	396581	88.91%	10.382%
15	10.217	2843	2854	2868	rBV	68816	111019	24.89%	2.906%
16	10.378	2897	2904	2916	rBV3	6100	10321	2.31%	0.270%
17	11.249	3163	3175	3195	rBV	231909	361587	81.07%	9.466%
18	11.622	3280	3291	3308	rBV	199994	313378	70.26%	8.204%
19	12.345	3508	3516	3528	rBV5	8317	12747	2.86%	0.334%
20	13.898	3990	3999	4009	rBV5	5438	8187	1.84%	0.214%
21	14.037	4033	4042	4050	rVB3	3478	5500	1.23%	0.144%
22	14.844	4282	4293	4299	rBV3	9274	13474	3.02%	0.353%
23	15.413	4463	4470	4481	rBV7	3923	5837	1.31%	0.153%
24	15.728	4558	4568	4577	rBV6	6356	9289	2.08%	0.243%




Sum of corrected areas: 3819783

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040622\
Data File : VV025361.D
Acq On : 06 Apr 2022 14:14
Operator : SY/MD
Sample : N2289-03
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFFD0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

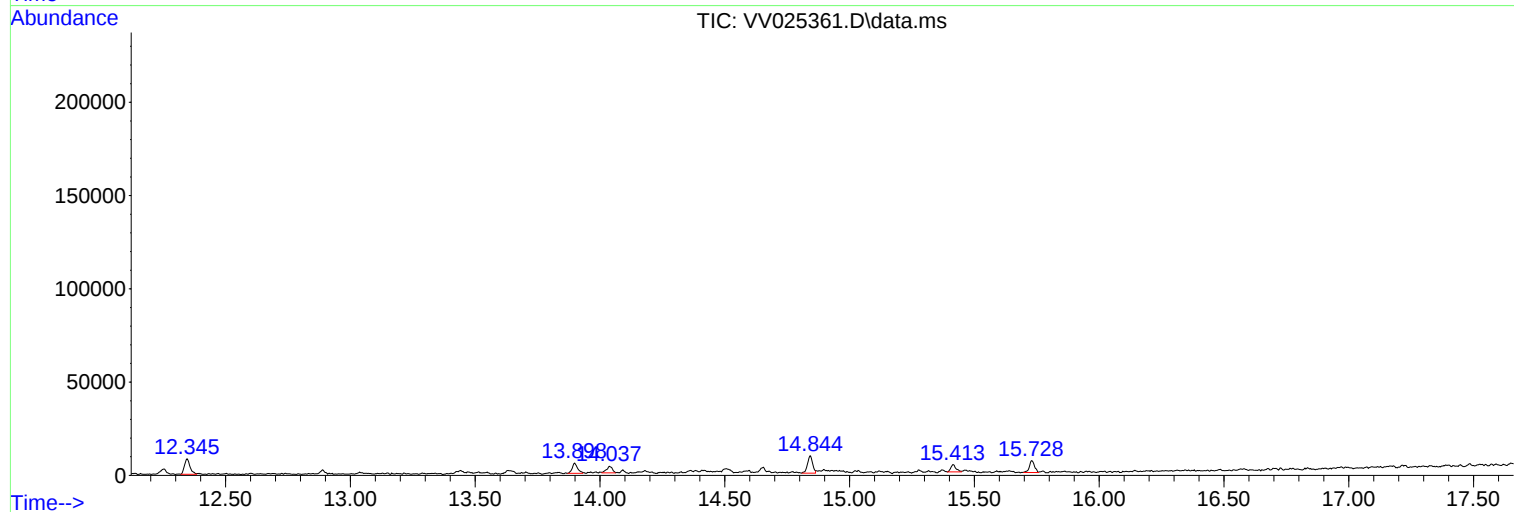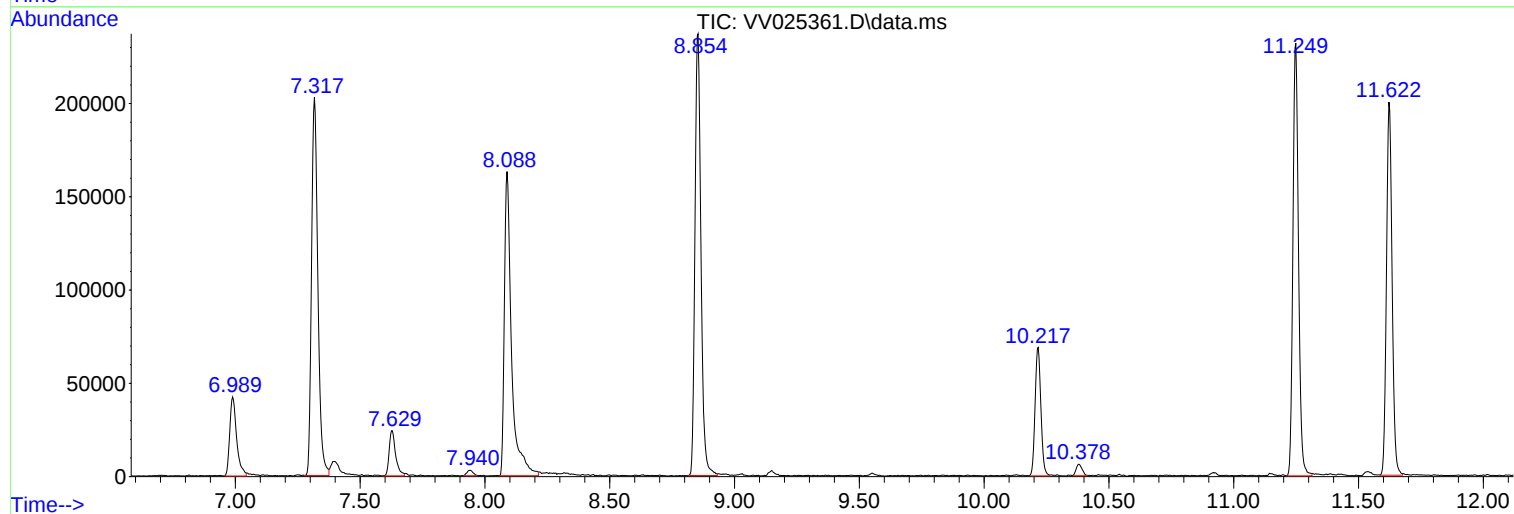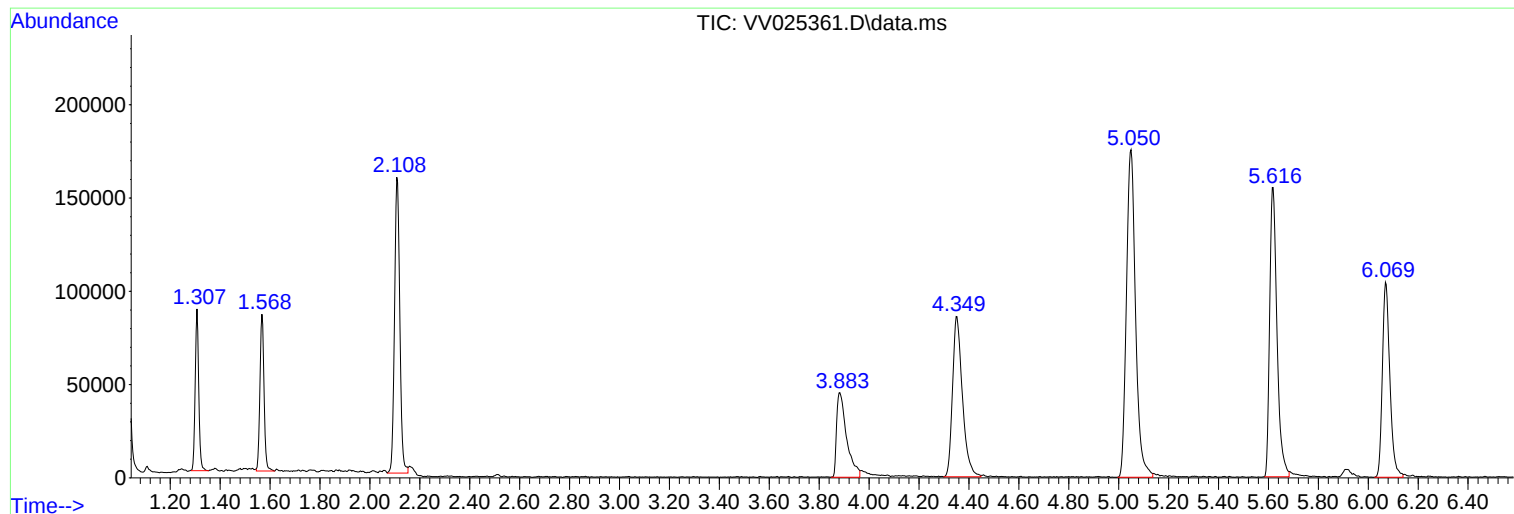

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040622\
Data File : VV025361.D
Acq On : 06 Apr 2022 14:14
Operator : SY/MD
Sample : N2289-03
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFFD0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040622\
Data File : VV025361.D
Acq On : 06 Apr 2022 14:14
Operator : SY/MD
Sample : N2289-03
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFFD0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------