


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040622\
Data File : VV025355.D
Acq On : 06 Apr 2022 09:40
Operator : SY/MD
Sample : BFB296
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB296

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Thu Apr 07 01:24:47 2022

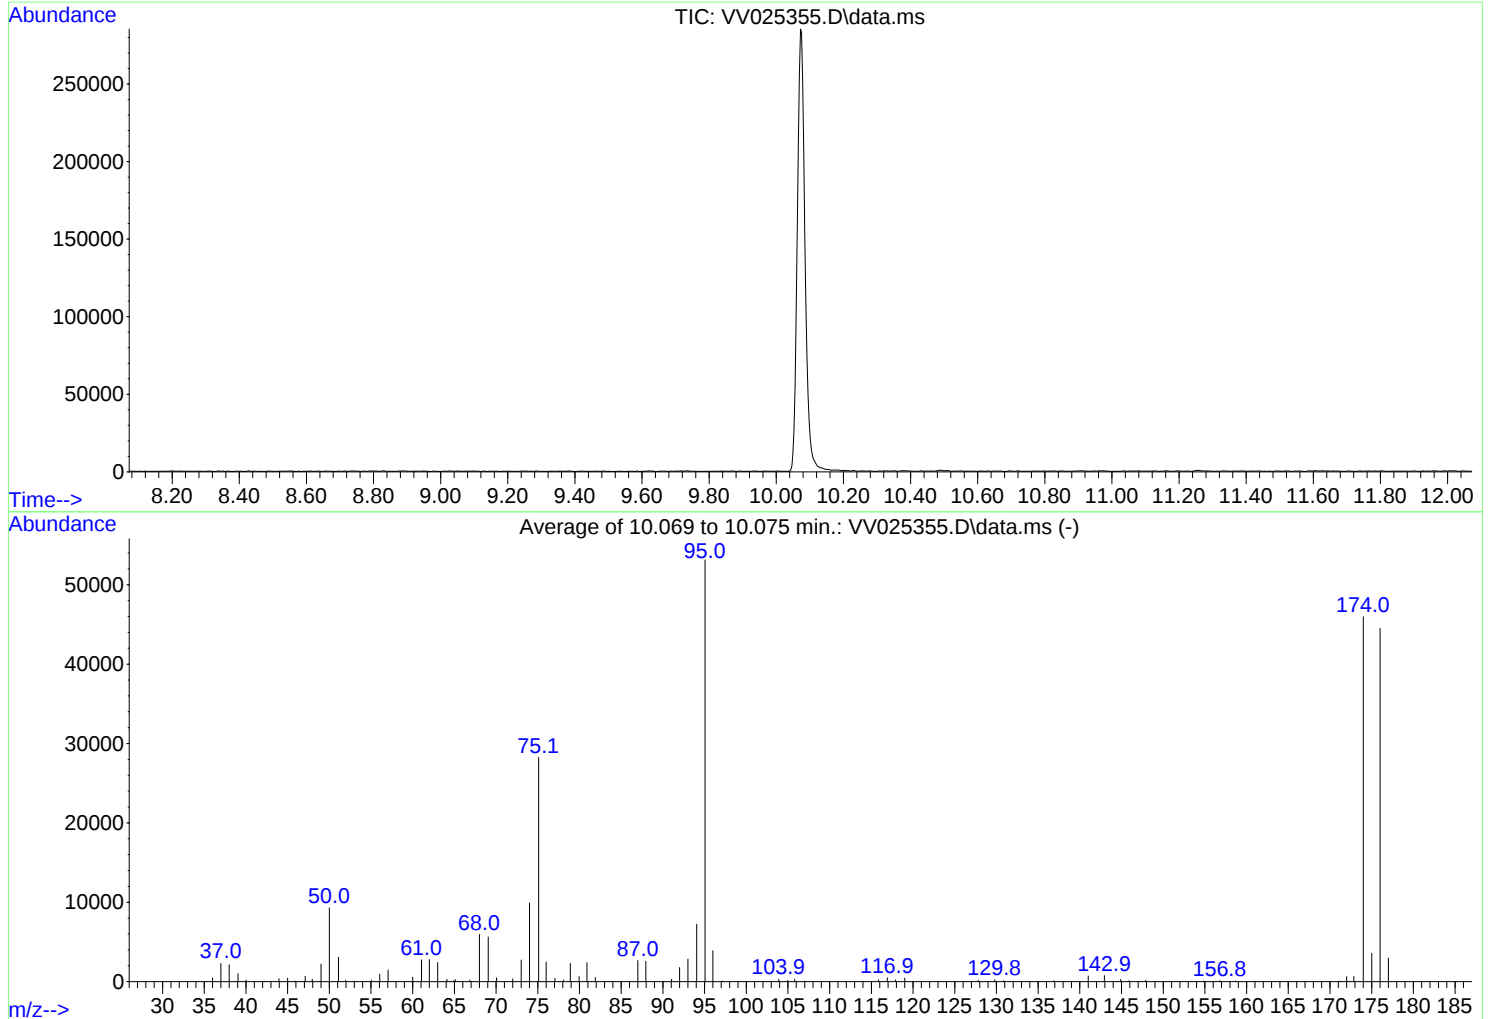

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2797

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.5	9292	PASS
75	95	30	80	53.1	28240	PASS
95	95	100	100	100.0	53139	PASS
96	95	5	9	7.3	3895	PASS
173	174	0.00	2	1.4	639	PASS
174	95	50	120	86.5	45989	PASS
175	174	5	9	7.8	3578	PASS
176	174	95	105	96.8	44517	PASS
177	176	5	10	6.6	2955	PASS

m/z	Abundance
43.90	271.0

Instrument :
MSVOA_V
ClientSampleId :
BFB296

m/z	Abundance
36.00	457.0
37.00	2123.0
38.00	2007.0
39.00	901.0
40.00	163.0
44.00	613.0
45.00	431.0
47.10	566.0
47.90	325.0
49.00	2149.0
50.00	8914.0
51.10	2939.0
51.90	147.0
55.10	208.0
56.00	886.0
57.00	1326.0
60.00	526.0
61.10	2612.0
62.00	2728.0
63.00	2331.0
64.10	284.0
64.90	328.0
66.80	216.0
68.00	5741.0
69.10	5187.0
70.00	506.0
72.00	346.0
73.00	2599.0
74.00	9308.0
75.10	26272.0
76.00	2320.0
77.10	348.0
78.10	207.0
78.90	2328.0
80.00	577.0
80.90	2245.0
81.90	492.0
87.00	2442.0
87.90	2431.0
91.00	305.0
92.00	1683.0
93.00	2652.0
94.10	6948.0
95.10	50512.0
96.00	3899.0
103.90	291.0
104.90	111.0
105.80	298.0
115.80	219.0
116.90	475.0
117.90	255.0
119.00	384.0
127.80	186.0
129.80	257.0
130.80	131.0
136.90	122.0
141.00	731.0
142.90	775.0
144.90	278.0
145.90	112.0
147.90	157.0
156.80	107.0
158.70	110.0
172.00	592.0
172.80	612.0
174.00	42424.0
175.00	3449.0
176.00	40448.0
177.00	2722.0

Instrument :
MSVOA_V
ClientSampleId :
BFB296

m/z	Abundance
36.00	514.0
37.00	2375.0
38.00	2156.0
39.10	1050.0
40.00	210.0
44.00	646.0
45.00	480.0
45.90	108.0
47.10	711.0
48.00	300.0
49.00	2277.0
50.00	9623.0
51.10	3091.0
51.90	160.0
53.00	127.0
55.10	167.0
56.10	968.0
57.10	1518.0
60.00	578.0
61.10	2873.0
62.00	2916.0
63.00	2468.0
64.10	314.0
65.10	359.0
66.80	202.0
68.00	6203.0
69.00	5846.0
70.10	499.0
72.00	353.0
73.00	2812.0
74.00	10191.0
75.10	29312.0
76.00	2655.0
77.00	395.0
78.10	189.0
78.90	2389.0
80.00	630.0
80.90	2515.0
81.90	525.0
87.00	2783.0
88.00	2669.0
91.00	324.0
92.00	1835.0
93.00	2965.0
94.00	7540.0
95.00	54912.0
96.00	4026.0
97.10	118.0
103.90	317.0
105.00	122.0
105.80	329.0
107.00	101.0
115.80	236.0
116.90	508.0
117.90	233.0
119.00	480.0
127.80	186.0
129.80	222.0
130.80	130.0
136.90	133.0
141.00	754.0
142.90	771.0
144.90	301.0
145.90	137.0
147.90	181.0
154.90	105.0
156.80	109.0
158.70	112.0
171.10	113.0
172.00	663.0
172.90	642.0
174.00	47656.0
175.00	3737.0
176.00	46232.0
177.00	3039.0

Instrument :
MSVOA_V
ClientSampleId :
BFB296

m/z	Abundance
36.00	481.0
37.00	2415.0
38.00	2228.0
39.10	1081.0
40.00	230.0
42.20	106.0
44.00	650.0
45.00	437.0
45.90	122.0
47.10	777.0
48.00	293.0
49.00	2209.0
50.00	9338.0
51.10	3152.0
52.00	178.0
53.00	122.0
54.90	183.0
56.00	936.0
57.10	1585.0
60.00	622.0
61.00	2770.0
62.00	2725.0
63.00	2422.0
64.10	301.0
65.10	419.0
66.90	164.0
68.00	5890.0
69.00	5852.0
70.10	447.0
72.00	359.0
73.00	2756.0
74.00	10171.0
75.10	29136.0
76.00	2475.0
77.00	443.0
78.10	208.0
78.90	2208.0
79.90	650.0
80.90	2458.0
81.90	555.0
87.00	2773.0
88.00	2597.0
91.10	268.0
92.00	1814.0
93.00	2931.0
94.10	7213.0
95.00	53992.0
96.00	3761.0
97.10	105.0
103.90	331.0
104.80	109.0
105.00	106.0
105.80	281.0
107.00	122.0
111.90	102.0
115.90	217.0
116.90	468.0
117.90	188.0
119.00	473.0
127.80	184.0
129.80	227.0
130.90	111.0
134.90	108.0
136.90	122.0
141.00	650.0
143.00	743.0
144.90	275.0
145.90	133.0
147.90	179.0
154.80	102.0
156.80	130.0
171.10	118.0
172.00	635.0
172.90	663.0
174.00	47888.0
175.00	3549.0
176.00	46872.0
177.00	3104.0

Instrument :
MSVOA_V
ClientSampleId :
BFB296