




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040722\
 Data File : VV025384.D
 Acq On : 07 Apr 2022 14:28
 Operator : SY/MD
 Sample : N2261-09
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFY45

Manual IntegrationsAPPROVED

Quant Time: Apr 08 01:22:05 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Apr 08 01:19:10 2022
 Response via : Initial Calibration

Reviewed By :John Carlone 04/08/2022
 Supervised By :Mahesh Dadoda 04/08/2022

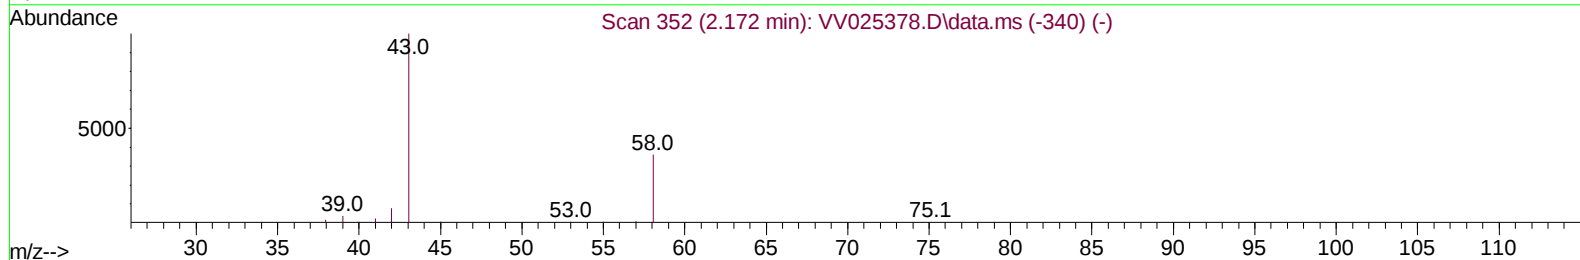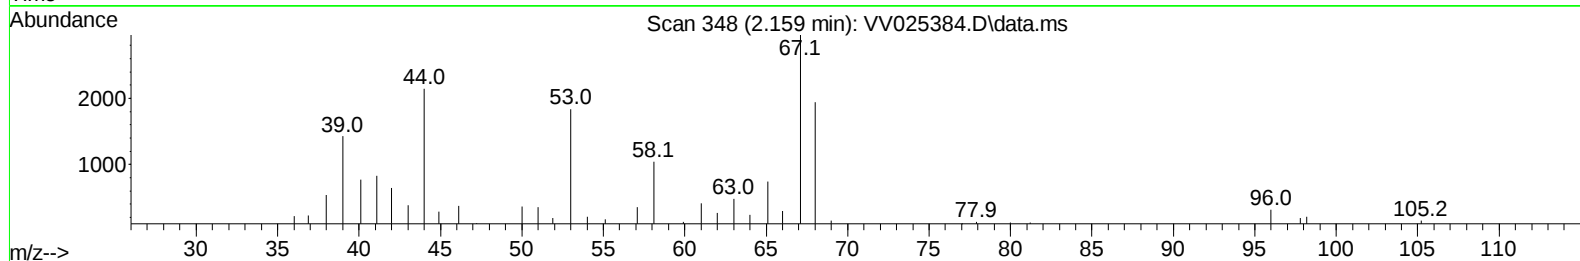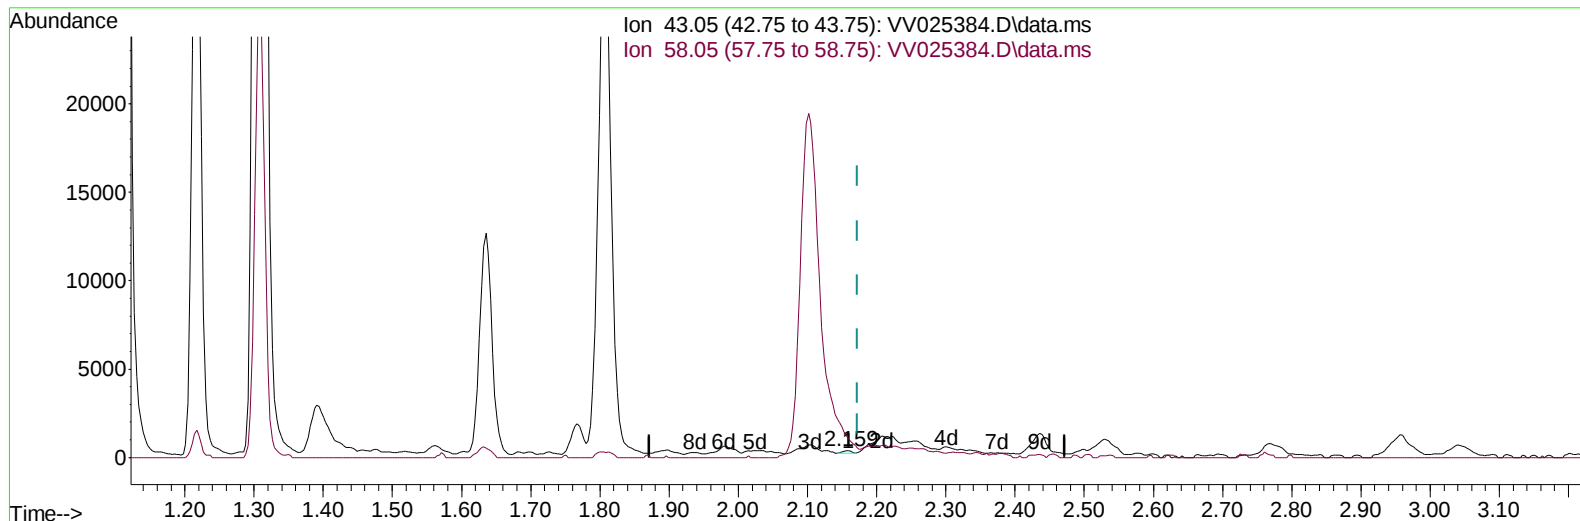

TIC: VV025384.D\data.ms

(13) Acetone (T)

2.159min (-0.013) 0.11 ug/L

response 127

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	25.60	0.00
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040722\
 Data File : VV025384.D
 Acq On : 07 Apr 2022 14:28
 Operator : SY/MD
 Sample : N2261-09
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFY45

Manual IntegrationsAPPROVED

Quant Time: Apr 08 01:22:05 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Apr 08 01:19:10 2022
 Response via : Initial Calibration

Reviewed By :John Carlone 04/08/2022
 Supervised By :Mahesh Dadoda 04/08/2022

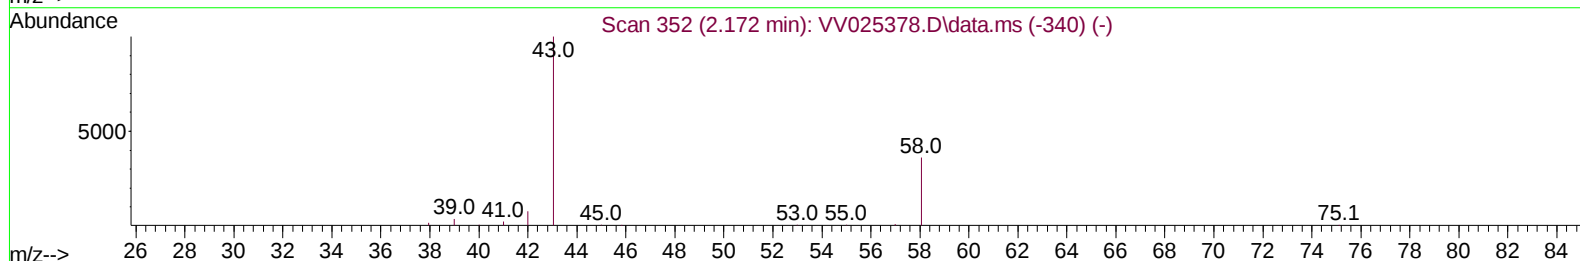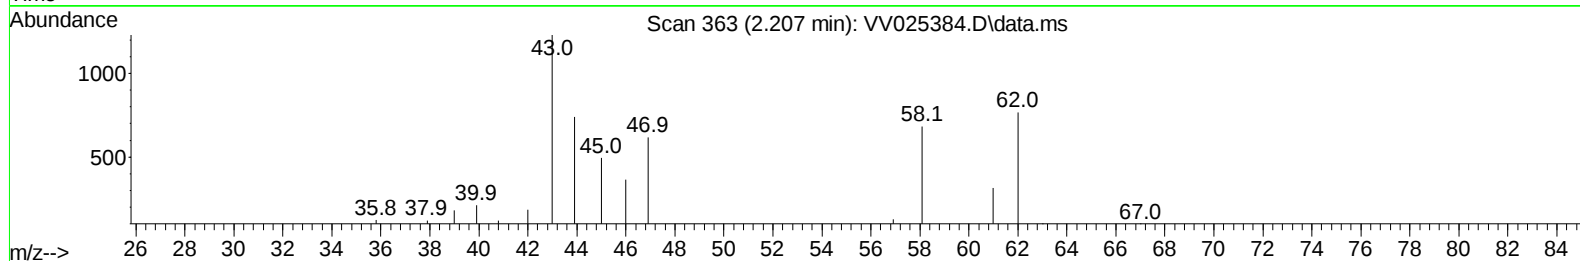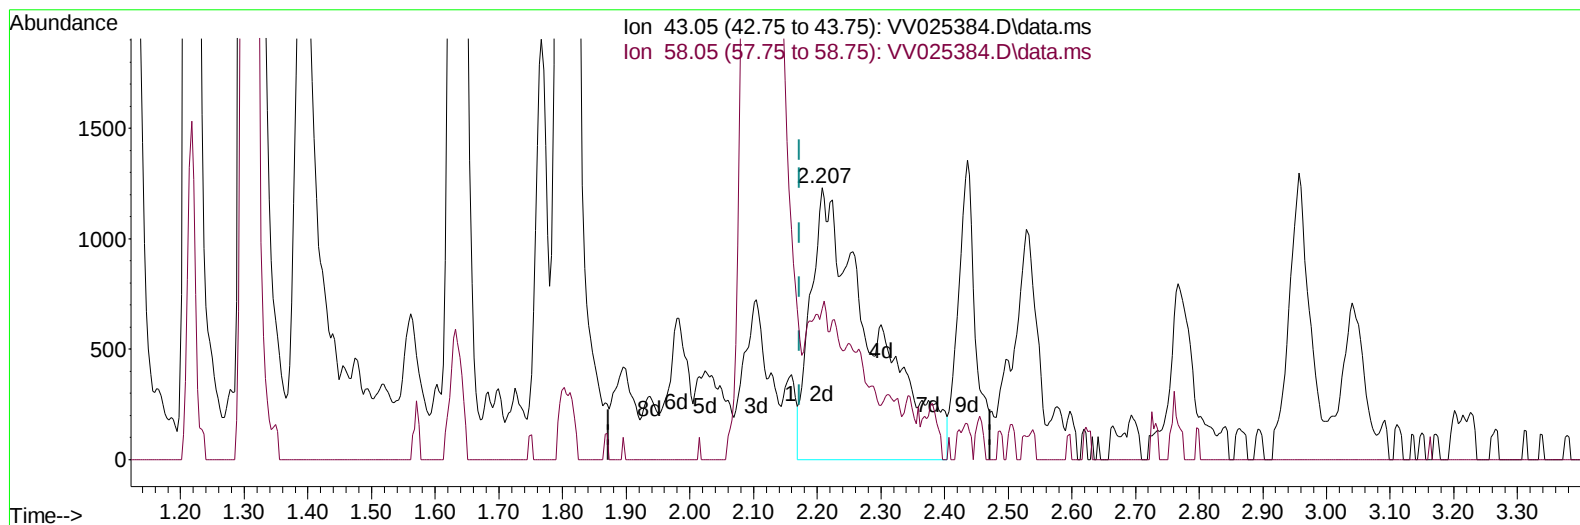

TIC: VV025384.D\data.ms

(13) Acetone (T)

2.207min (+ 0.035) 7.15 ug/L m

response 8191

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	25.60	0.00
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040722\
Data File : VV025384.D
Acq On : 07 Apr 2022 14:28
Operator : SY/MD
Sample : N2261-09
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFY45

Manual IntegrationsAPPROVED

Quant Time: Apr 08 01:22:05 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Apr 08 01:19:10 2022
Response via : Initial Calibration

Reviewed By :John Carlone 04/08/2022
Supervised By :Mahesh Dadoda 04/08/2022

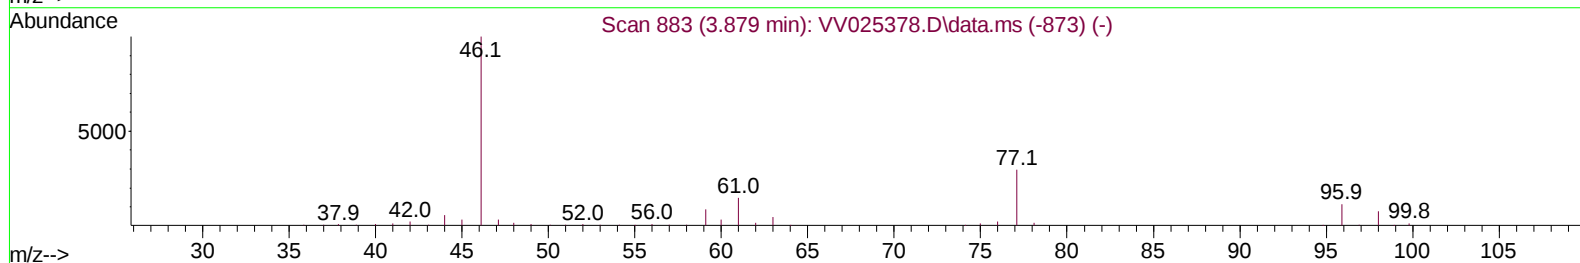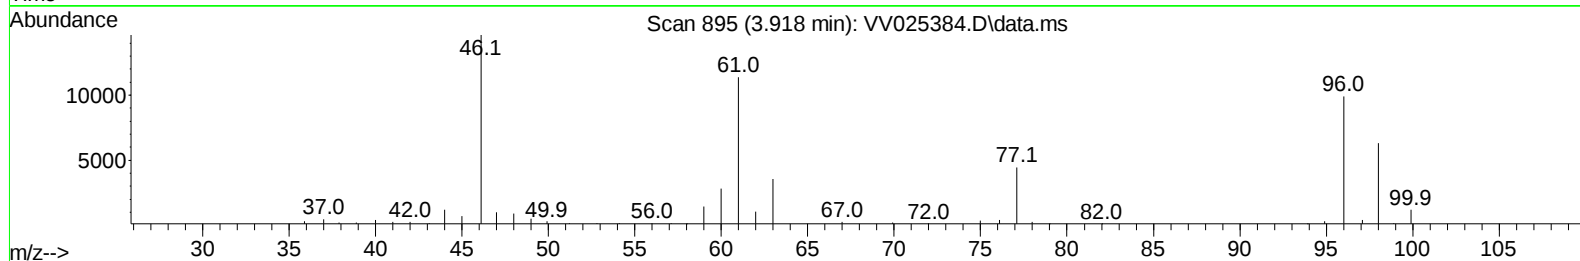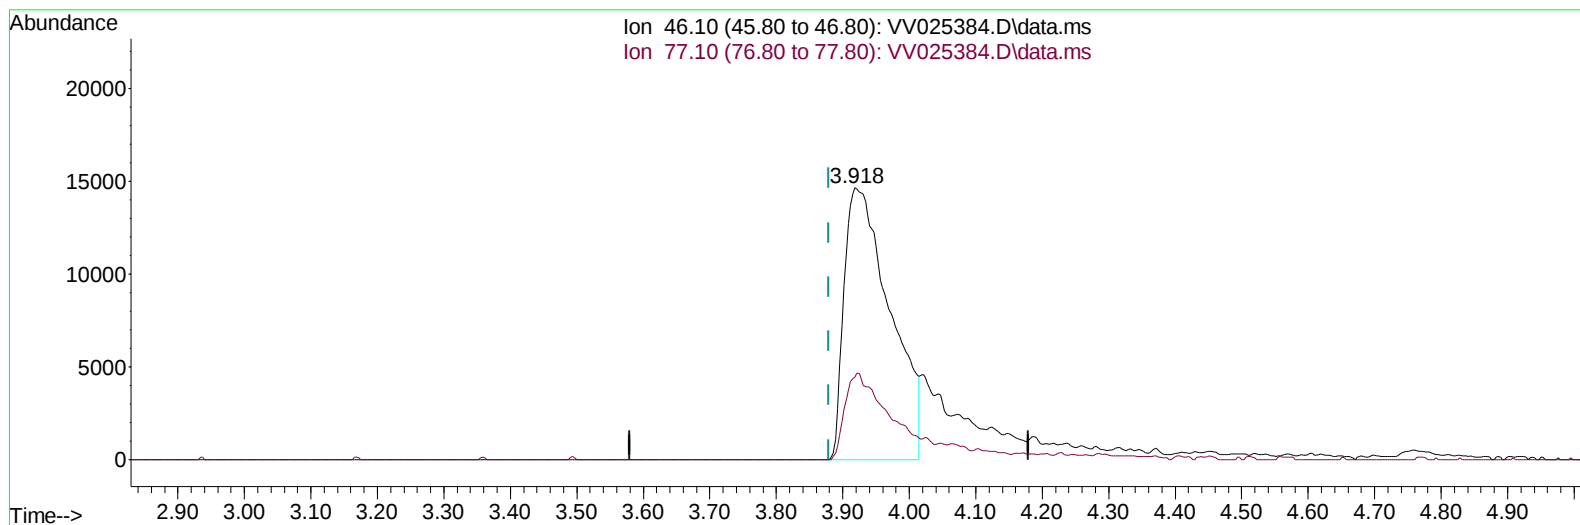

TIC: VV025384.D\data.ms

(20) 2-Butanone-d5 (S)

3.918min (+ 0.039) 46.84 ug/L

response 70367

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	24.90	29.80
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040722\
Data File : VV025384.D
Acq On : 07 Apr 2022 14:28
Operator : SY/MD
Sample : N2261-09
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFY45

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 04/08/2022
Supervised By :Mahesh Dadoda 04/08/2022

Quant Time: Apr 08 01:22:05 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Apr 08 01:19:10 2022
Response via : Initial Calibration

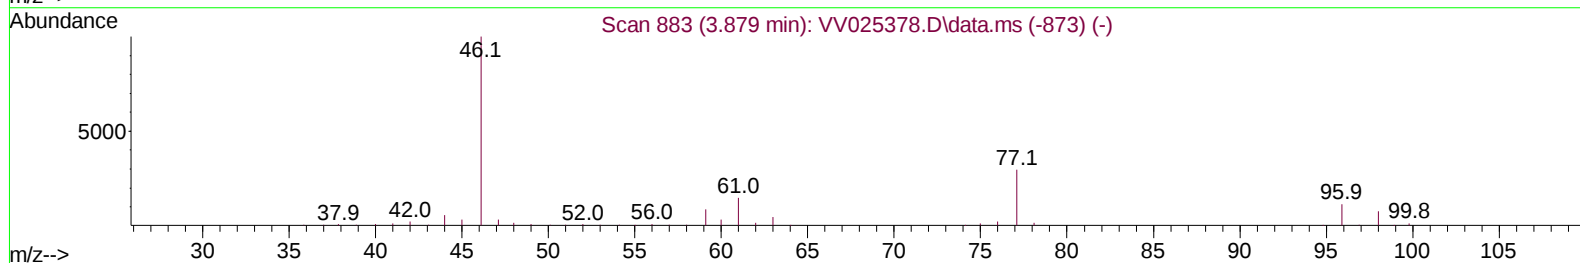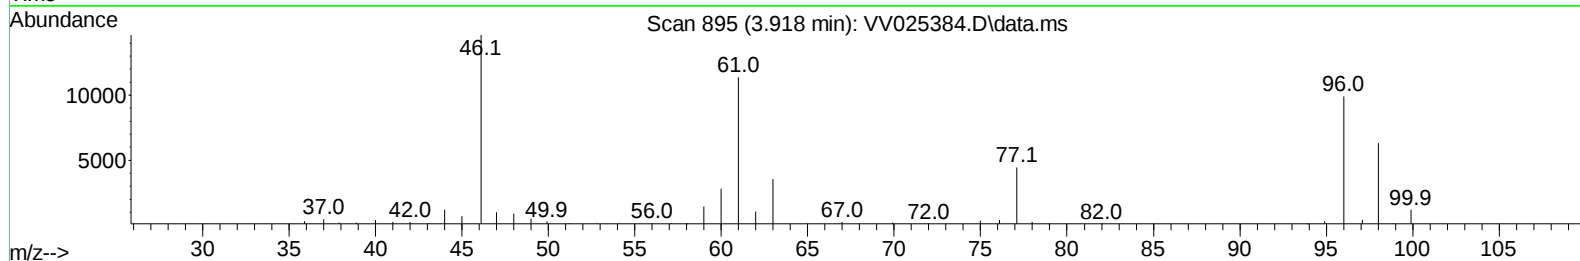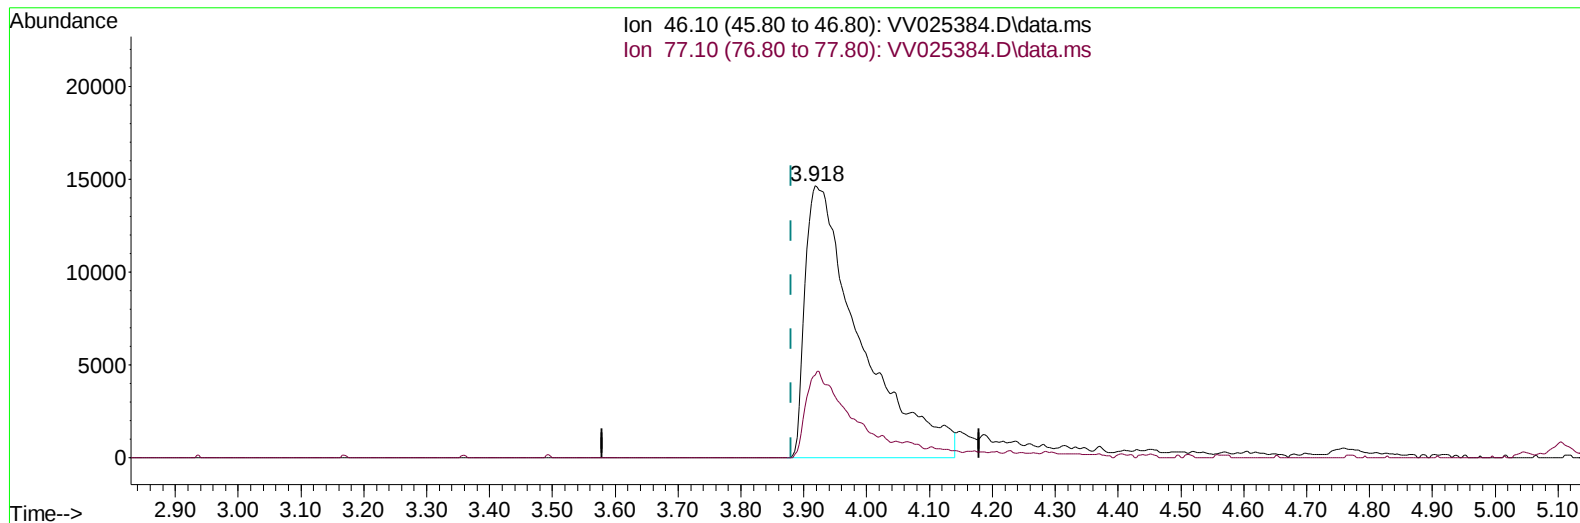

TIC: VV025384.D\data.ms

(20) 2-Butanone-d5 (S)**3.918min (+ 0.039) 59.31 ug/L m****response 89109**

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	24.90	23.53
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040722\
 Data File : VV025384.D
 Acq On : 07 Apr 2022 14:28
 Operator : SY/MD
 Sample : N2261-09
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFY45

Manual IntegrationsAPPROVED

Quant Time: Apr 08 01:22:05 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Apr 08 01:19:10 2022
 Response via : Initial Calibration

Reviewed By : John Carlone 04/08/2022
 Supervised By : Mahesh Dadoda 04/08/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	161463	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	150499	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	77258	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	59586	3.951	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130	Recovery	=	79.000%	
7) Chloroethane-d5	1.568	69	58893	4.653	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130	Recovery	=	93.000%	
11) 1,1-Dichloroethene-d2	2.111	63	117873	3.608	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125	Recovery	=	72.200%	
20) 2-Butanone-d5	3.918	46	89109m	59.313	ug/L	0.04
Spiked Amount 50.000	Range 40	- 130	Recovery	=	118.620%	
24) Chloroform-d	4.352	84	103987	5.283	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	105.600%	
26) 1,2-Dichloroethane-d4	5.037	65	45645	5.247	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	105.000%	
32) Benzene-d6	5.050	84	197406	5.185	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	103.600%	
36) 1,2-Dichloropropane-d6	6.072	67	61070	5.723	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140	Recovery	=	114.400%	
41) Toluene-d8	7.317	98	170342	4.878	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	97.600%	
43) trans-1,3-Dichloroprop...	7.625	79	18574	5.336	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130	Recovery	=	106.800%	
46) 2-Hexanone-d5	8.091	63	81765	65.036	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130	Recovery	=	130.080%#	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	41414	5.821	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120	Recovery	=	116.400%	
66) 1,2-Dichlorobenzene-d4	11.622	152	65380	5.269	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120	Recovery	=	105.400%	
Target Compounds						
					Qvalue	
12) 1,1-Dichloroethene	2.121	96	39389	2.423	ug/L #	83
13) Acetone	2.207	43	8191m	7.145	ug/L	
17) Methyl tert-butyl Ether	2.770	73	5779	0.281	ug/L #	25
19) 1,1-Dichloroethane	3.191	63	74504	3.825	ug/L	99
22) cis-1,2-Dichloroethene	3.915	96	24219	2.043	ug/L	96
25) Chloroform	4.384	83	4311	0.199	ug/L	91
29) 1,1,1-Trichloroethane	4.613	97	15399	0.846	ug/L	98
33) Benzene	5.108	78	7317	0.166	ug/L	100
34) Trichloroethene	5.915	95	17225	1.421	ug/L	95
42) Toluene	7.394	91	32205	0.683	ug/L	96
47) Tetrachloroethene	7.976	164	18744	2.097	ug/L	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040722\
Data File : VV025384.D
Acq On : 07 Apr 2022 14:28
Operator : SY/MD
Sample : N2261-09
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFY45

Manual IntegrationsAPPROVED

Quant Time: Apr 08 01:22:05 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Apr 08 01:19:10 2022
Response via : Initial Calibration

Reviewed By :John Carlone 04/08/2022
Supervised By :Mahesh Dadoda 04/08/2022

