




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040722\
 Data File : VV025386.D
 Acq On : 07 Apr 2022 15:15
 Operator : SY/MD
 Sample : N2289-03
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFFD0

Manual IntegrationsAPPROVED

Quant Time: Apr 08 01:22:38 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Apr 08 01:19:10 2022
 Response via : Initial Calibration

Reviewed By :John Carlone 04/08/2022
 Supervised By :Mahesh Dadoda 04/08/2022

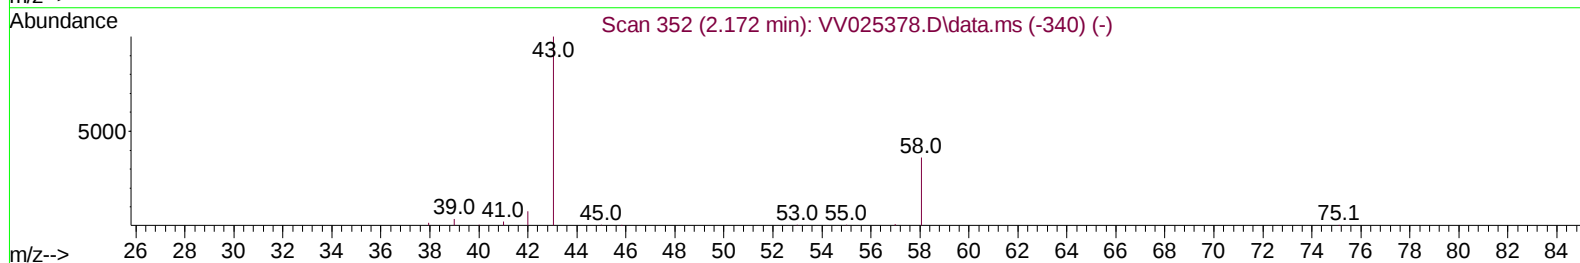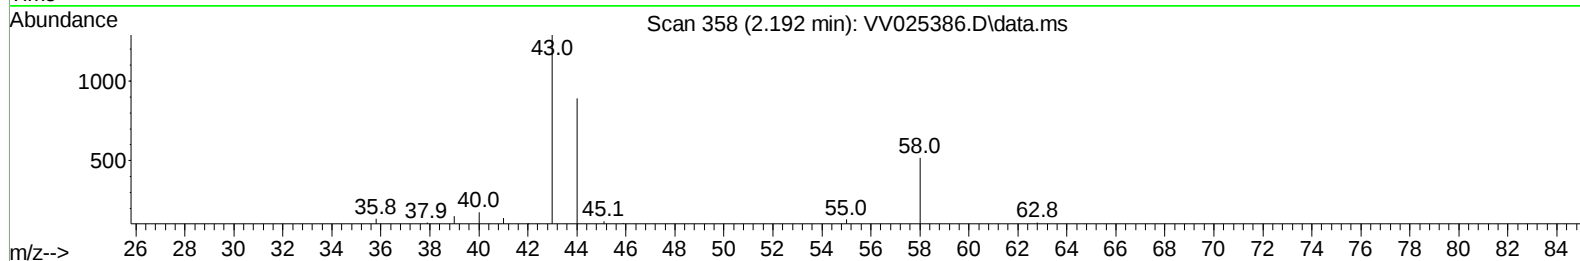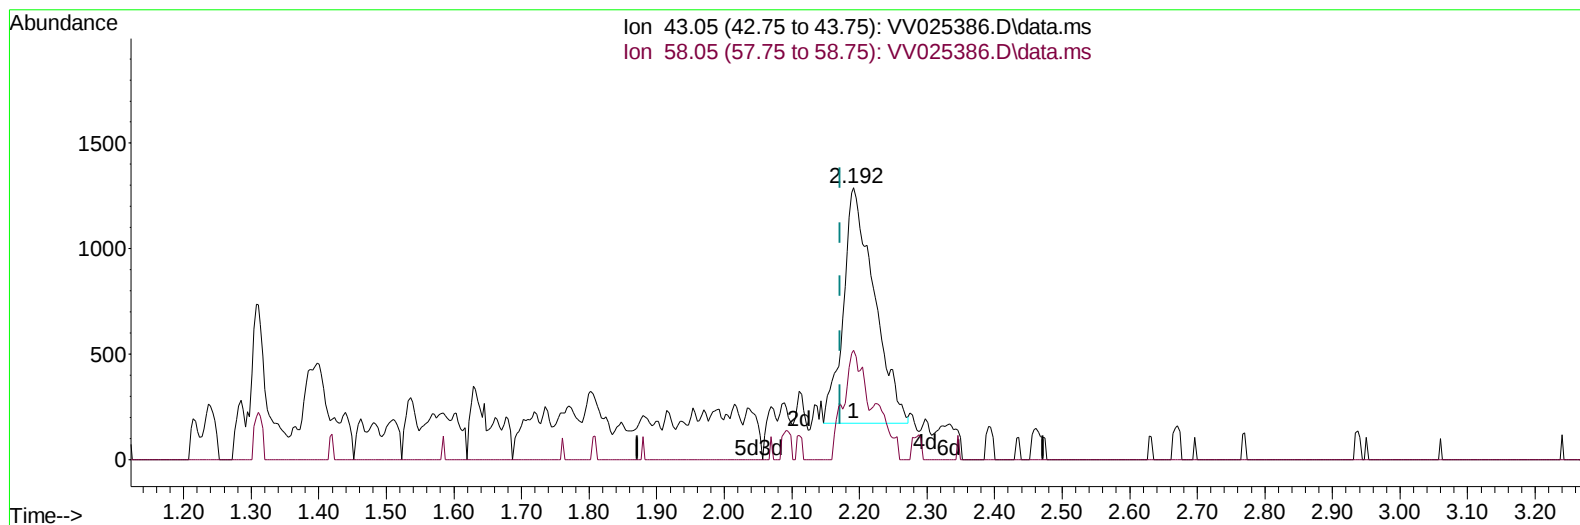

TIC: VV025386.D\data.ms

(13) Acetone (T)

2.192min (+ 0.019) 2.95 ug/L

response 3533

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	25.60	32.80
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040722\
 Data File : VV025386.D
 Acq On : 07 Apr 2022 15:15
 Operator : SY/MD
 Sample : N2289-03
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFFD0

Manual IntegrationsAPPROVED

Quant Time: Apr 08 01:22:38 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Apr 08 01:19:10 2022
 Response via : Initial Calibration

Reviewed By :John Carlone 04/08/2022
 Supervised By :Mahesh Dadoda 04/08/2022

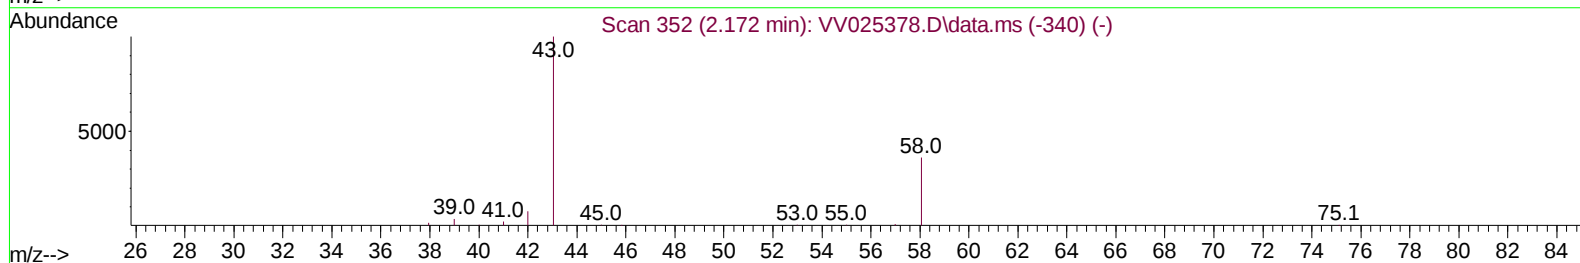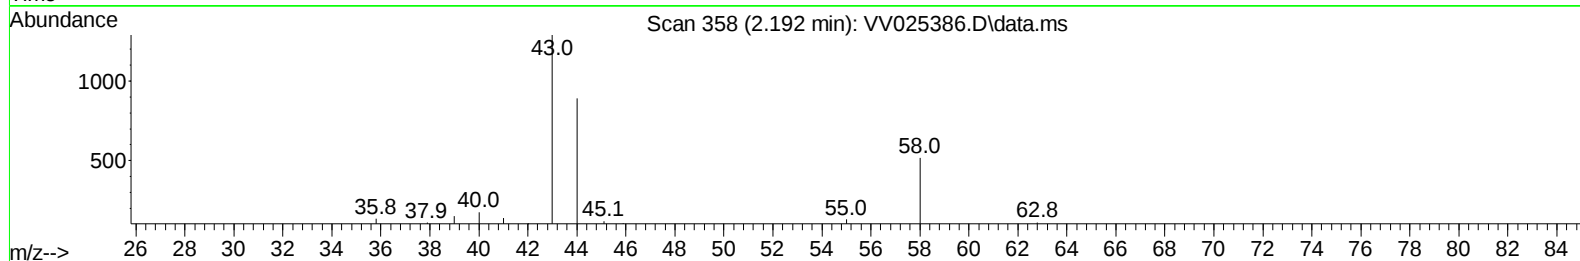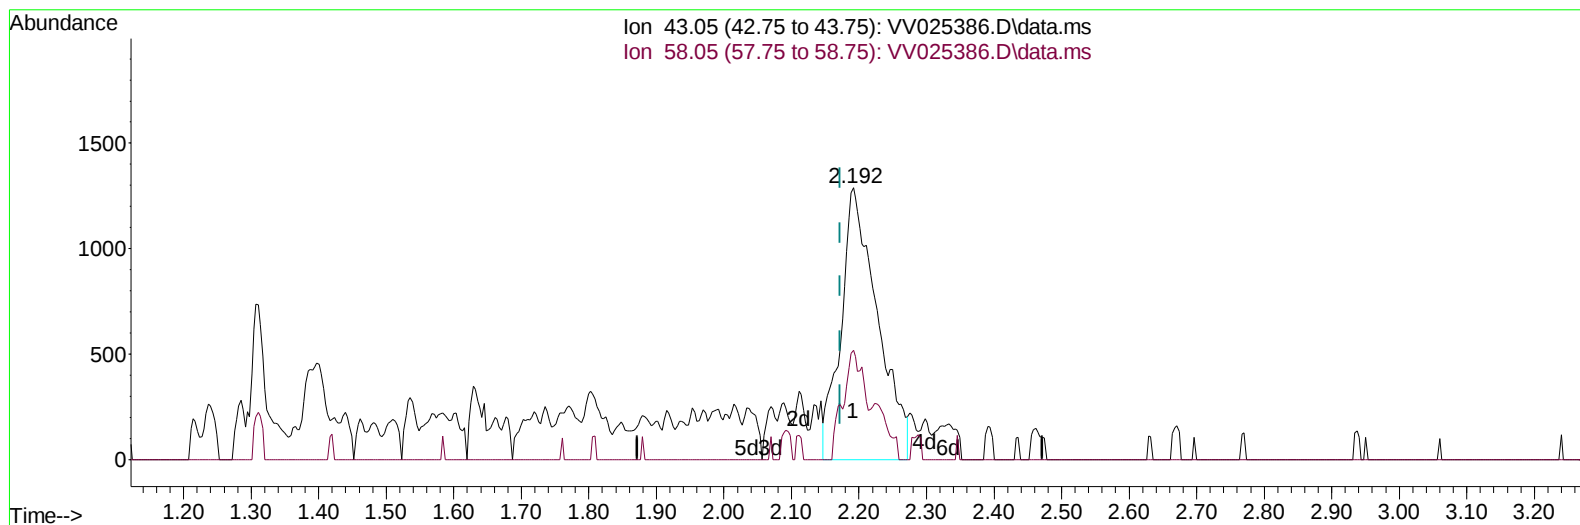

TIC: VV025386.D\data.ms

(13) Acetone (T)

2.192min (+ 0.019) 4.04 ug/L m

response 4835

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	25.60	23.97
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040722\
 Data File : VV025386.D
 Acq On : 07 Apr 2022 15:15
 Operator : SY/MD
 Sample : N2289-03
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFFD0

Manual IntegrationsAPPROVED

Quant Time: Apr 08 01:22:38 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Apr 08 01:19:10 2022
 Response via : Initial Calibration

Reviewed By :John Carlone 04/08/2022
 Supervised By :Mahesh Dadoda 04/08/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	168734	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	157959	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	75584	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	80544	5.110	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130	Recovery	=	102.200%	
7) Chloroethane-d5	1.571	69	67361	5.092	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130	Recovery	=	101.800%	
11) 1,1-Dichloroethene-d2	2.111	63	117756	3.449	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125	Recovery	=	69.000%	
20) 2-Butanone-d5	3.899	46	90971	57.943	ug/L	0.02
Spiked Amount 50.000	Range 40	- 130	Recovery	=	115.880%	
24) Chloroform-d	4.349	84	109038	5.301	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	106.000%	
26) 1,2-Dichloroethane-d4	5.034	65	50949	5.604	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	112.000%	
32) Benzene-d6	5.050	84	231617	5.796	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	116.000%	
36) 1,2-Dichloropropane-d6	6.072	67	63429	5.664	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140	Recovery	=	113.200%	
41) Toluene-d8	7.317	98	205982	5.620	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	112.400%	
43) trans-1,3-Dichloroprop...	7.625	79	20242	5.540	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130	Recovery	=	110.800%	
46) 2-Hexanone-d5	8.088	63	74861	56.732	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130	Recovery	=	113.460%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	40869	5.473	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120	Recovery	=	109.400%	
66) 1,2-Dichlorobenzene-d4	11.622	152	69081	5.691	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120	Recovery	=	113.800%	
Target Compounds						
13) Acetone	2.192	43	4835m	4.036	ug/L	
25) Chloroform	4.381	83	15138	0.670	ug/L	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040722\
Data File : VV025386.D
Acq On : 07 Apr 2022 15:15
Operator : SY/MD
Sample : N2289-03
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFFD0

Manual IntegrationsAPPROVED

Quant Time: Apr 08 01:22:38 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Apr 08 01:19:10 2022
Response via : Initial Calibration

Reviewed By :John Carlone 04/08/2022
Supervised By :Mahesh Dadoda 04/08/2022

