




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040722\
 Data File : VV025393.D
 Acq On : 07 Apr 2022 18:25
 Operator : SY/MD
 Sample : N2291-05DL 5X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B32DL

Manual IntegrationsAPPROVED

Quant Time: Apr 08 01:24:18 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Apr 08 01:19:10 2022
 Response via : Initial Calibration

Reviewed By :John Carlone 04/08/2022
 Supervised By :Mahesh Dadoda 04/08/2022

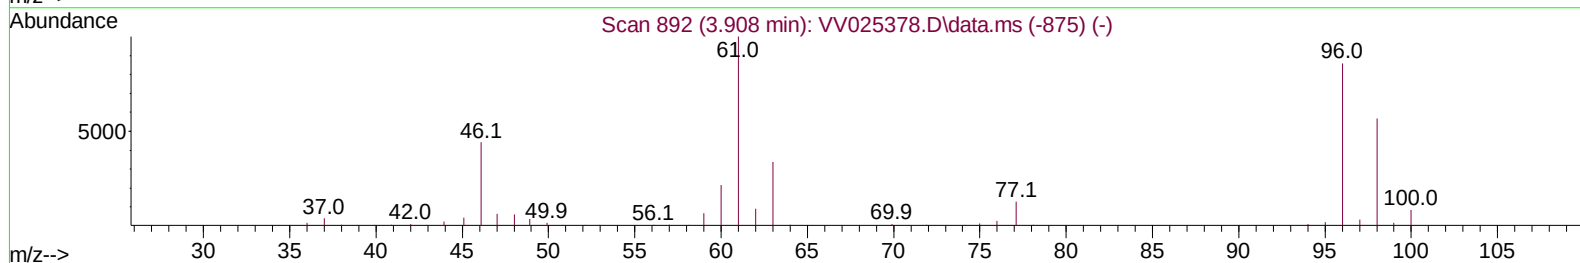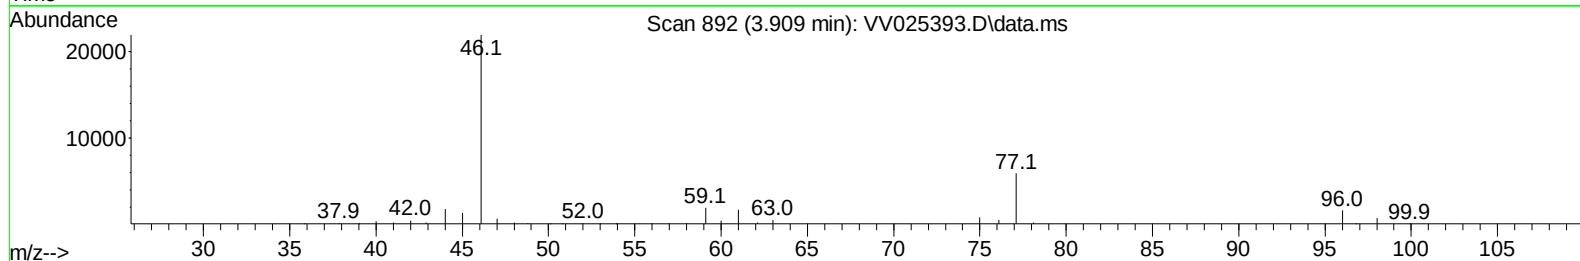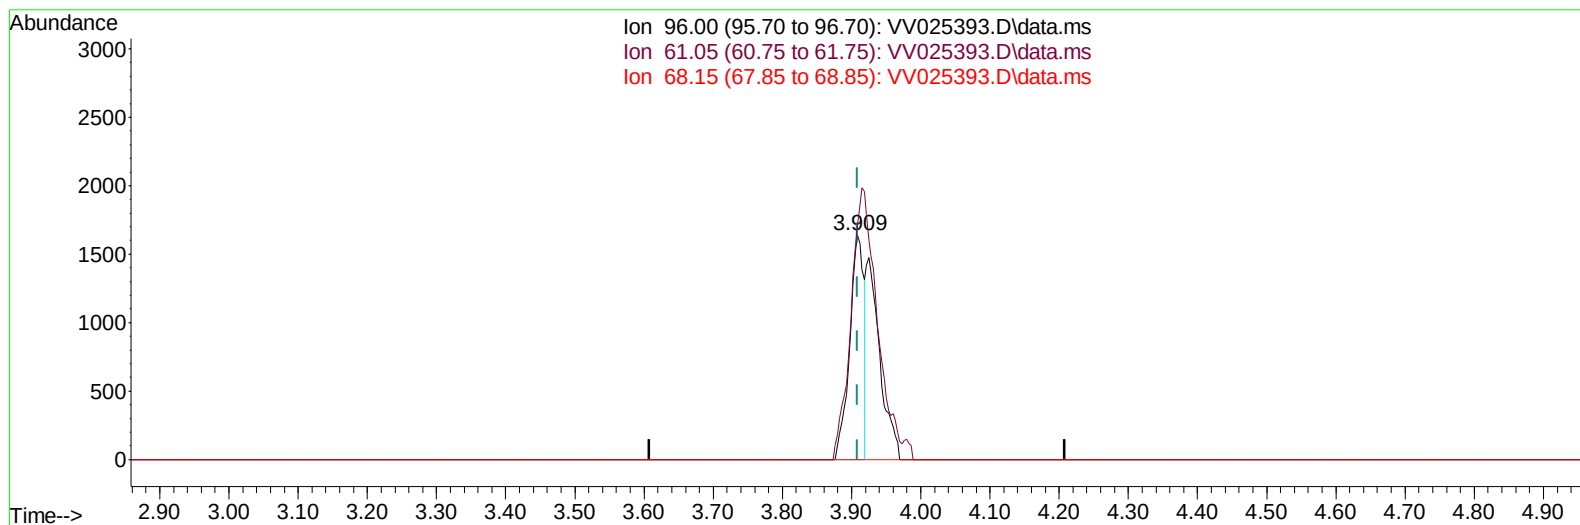

TIC: VV025393.D\data.ms

(22) cis-1,2-Dichloroethene (T)

3.909min (+ 0.000) 0.20 ug/L

response 2277

Ion	Exp%	Act%
96.00	100.00	100.00
61.05	120.10	104.14
68.15	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040722\
Data File : VV025393.D
Acq On : 07 Apr 2022 18:25
Operator : SY/MD
Sample : N2291-05DL 5X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B32DL

Manual IntegrationsAPPROVED

Quant Time: Apr 08 01:24:18 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Apr 08 01:19:10 2022
Response via : Initial Calibration

Reviewed By :John Carlone 04/08/2022
Supervised By :Mahesh Dadoda 04/08/2022

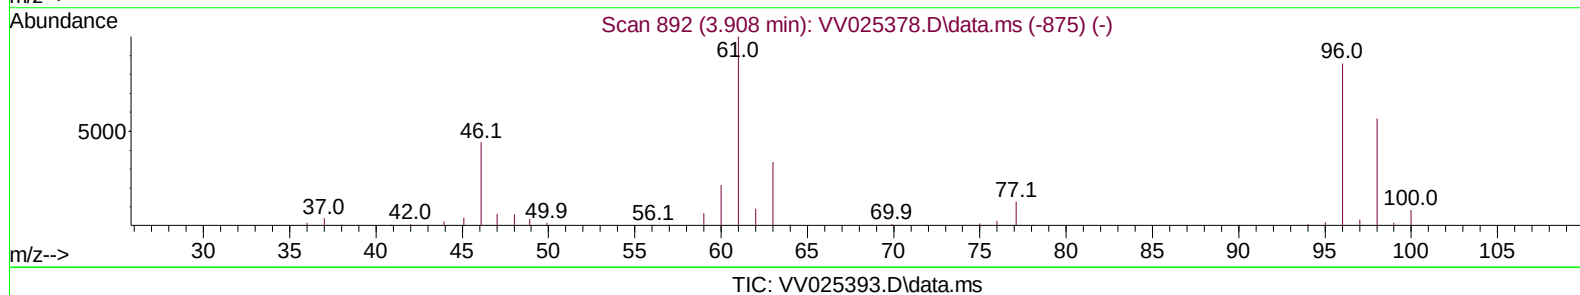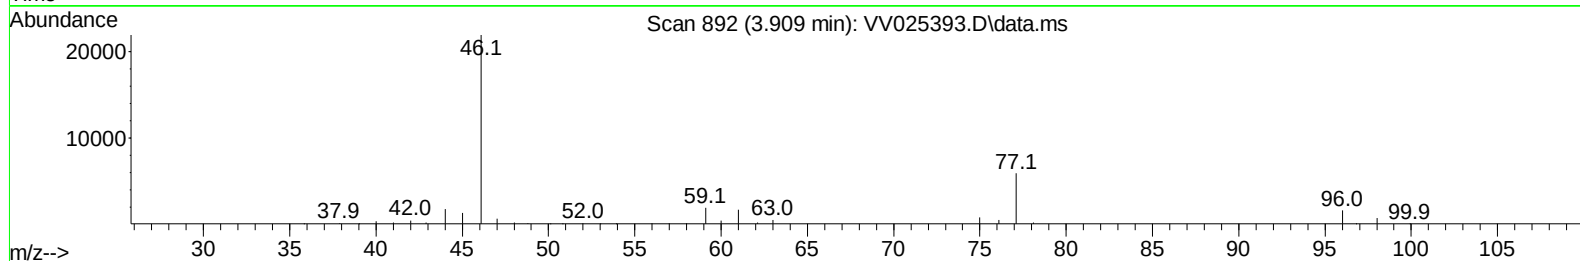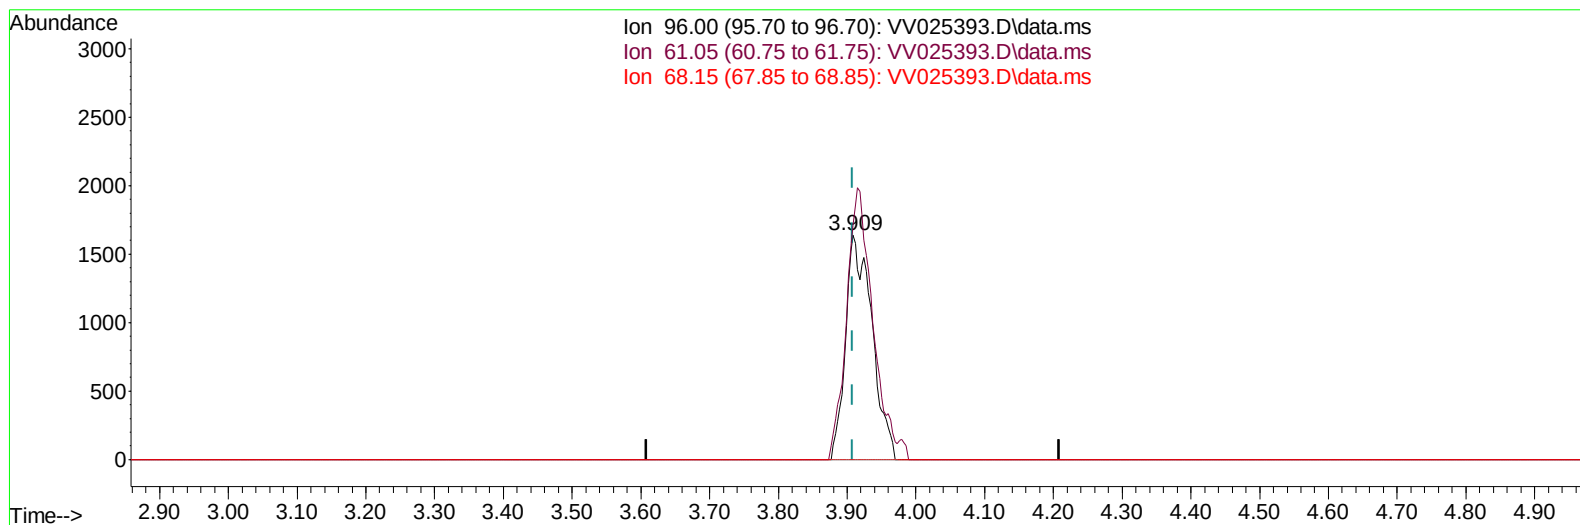

(22) cis-1,2-Dichloroethene (T)

3.909min (+ 0.000) 0.38 ug/L m

response 4362

Ion	Exp%	Act%
96.00	100.00	100.00
61.05	120.10	104.14
68.15	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040722\
 Data File : VV025393.D
 Acq On : 07 Apr 2022 18:25
 Operator : SY/MD
 Sample : N2291-05DL 5X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B32DL

Manual IntegrationsAPPROVED

Quant Time: Apr 08 01:24:18 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Apr 08 01:19:10 2022
 Response via : Initial Calibration

Reviewed By : John Carlone 04/08/2022
 Supervised By : Mahesh Dadoda 04/08/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	156115	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	145490	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	69072	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	77554	5.318	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130	Recovery	=	106.400%	
7) Chloroethane-d5	1.568	69	87934	7.185	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130	Recovery	=	143.600%#	
11) 1,1-Dichloroethene-d2	2.105	63	113663	3.598	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125	Recovery	=	72.000%	
20) 2-Butanone-d5	3.892	46	86576	59.601	ug/L	0.01
Spiked Amount 50.000	Range 40	- 130	Recovery	=	119.200%	
24) Chloroform-d	4.349	84	107365	5.642	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	112.800%	
26) 1,2-Dichloroethane-d4	5.034	65	51319	6.101	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	122.000%	
32) Benzene-d6	5.050	84	235425	6.396	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	128.000%#	
36) 1,2-Dichloropropane-d6	6.069	67	65158	6.317	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140	Recovery	=	126.400%	
41) Toluene-d8	7.317	98	207852	6.157	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	123.200%	
43) trans-1,3-Dichloroprop...	7.625	79	19032	5.656	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130	Recovery	=	113.200%	
46) 2-Hexanone-d5	8.092	63	73649	60.597	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130	Recovery	=	121.200%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	39465	5.738	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120	Recovery	=	114.800%	
66) 1,2-Dichlorobenzene-d4	11.625	152	70854	6.387	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120	Recovery	=	127.800%#	
Target Compounds						
					Qvalue	
9) Trichlorofluoromethane	1.748	101	68754	2.476	ug/L	99
16) Methylene chloride	2.507	84	3004	0.243	ug/L	96
22) cis-1,2-Dichloroethene	3.909	96	4362m	0.381	ug/L	
34) Trichloroethene	5.918	95	19055	1.626	ug/L	96
47) Tetrachloroethene	7.976	164	83343	9.645	ug/L	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040722\
Data File : VV025393.D
Acq On : 07 Apr 2022 18:25
Operator : SY/MD
Sample : N2291-05DL 5X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B32DL

Manual IntegrationsAPPROVED

Quant Time: Apr 08 01:24:18 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Apr 08 01:19:10 2022
Response via : Initial Calibration

Reviewed By :John Carlone 04/08/2022
Supervised By :Mahesh Dadoda 04/08/2022

