




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040722\
 Data File : VV025394.D
 Acq On : 07 Apr 2022 18:49
 Operator : SY/MD
 Sample : N2320-01
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YB2P3

Manual IntegrationsAPPROVED

Quant Time: Apr 08 01:24:33 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Apr 08 01:19:10 2022
 Response via : Initial Calibration

Reviewed By :John Carlone 04/08/2022
 Supervised By :Mahesh Dadoda 04/08/2022

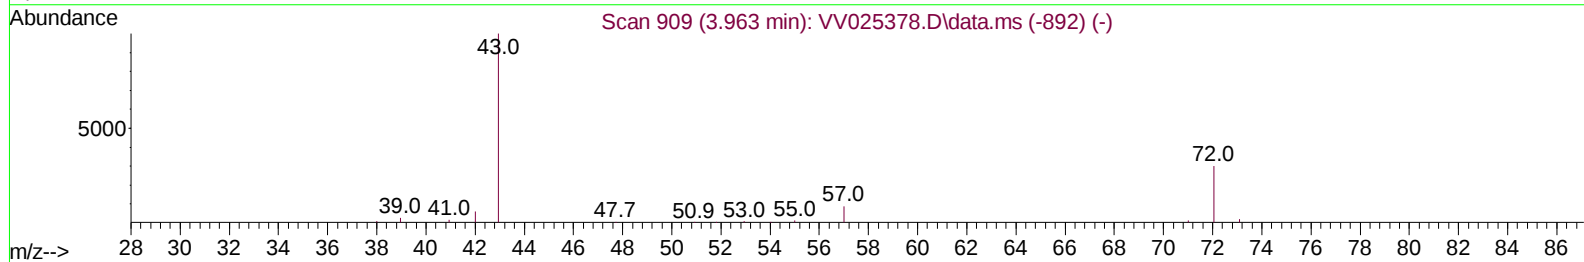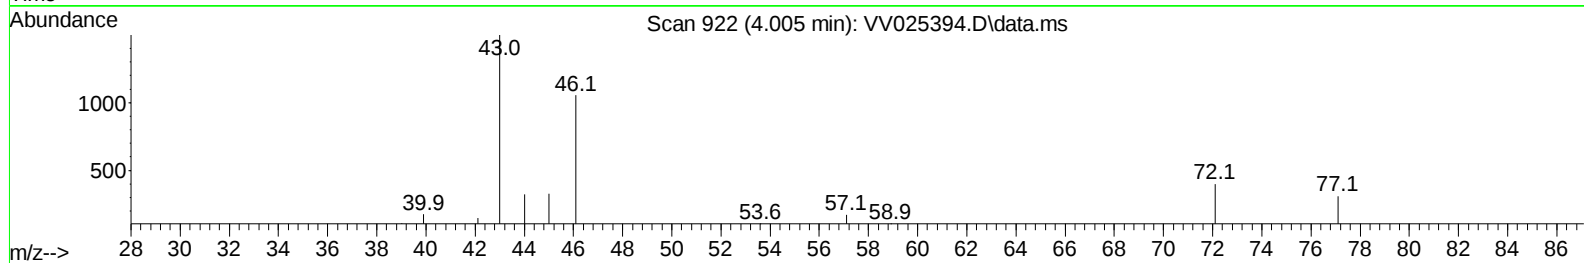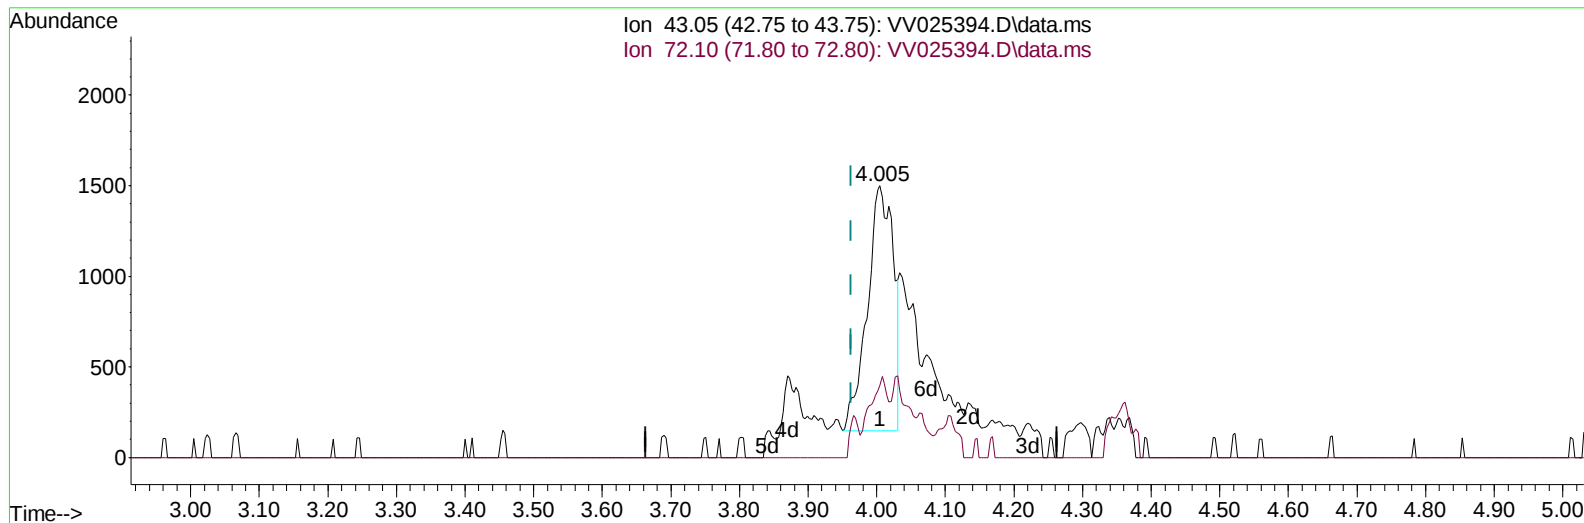

TIC: VV025394.D\data.ms

(21) 2-Butanone (T)

4.005min (+ 0.042) 2.25 ug/L

response 3558

Ion	Exp%	Act%
43.05	100.00	100.00
72.10	23.60	16.47
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040722\
 Data File : VV025394.D
 Acq On : 07 Apr 2022 18:49
 Operator : SY/MD
 Sample : N2320-01
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YB2P3

Manual IntegrationsAPPROVED

Quant Time: Apr 08 01:24:33 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Apr 08 01:19:10 2022
 Response via : Initial Calibration

Reviewed By :John Carlone 04/08/2022
 Supervised By :Mahesh Dadoda 04/08/2022

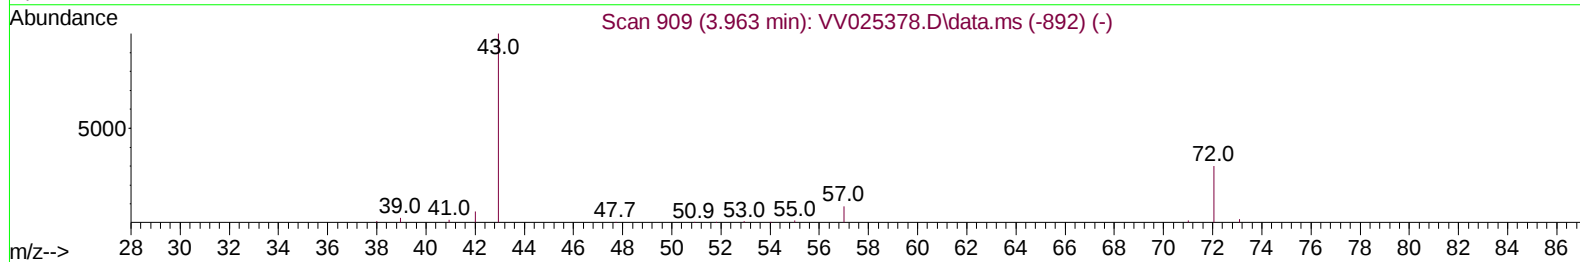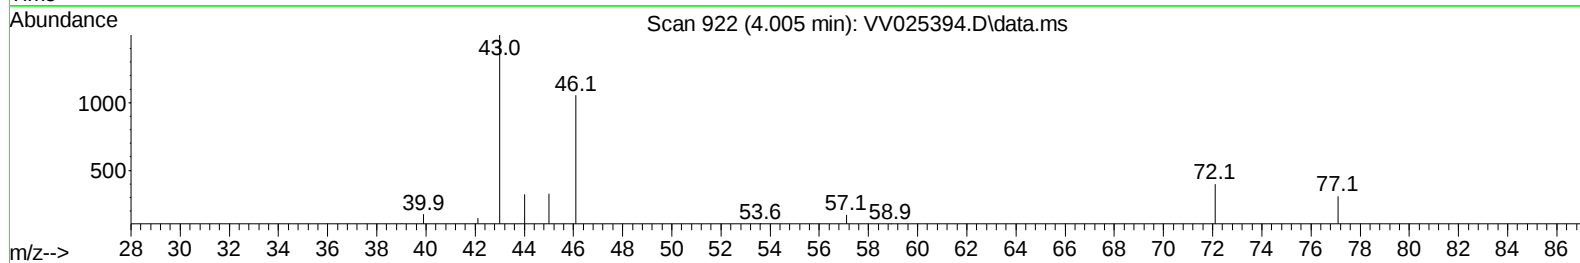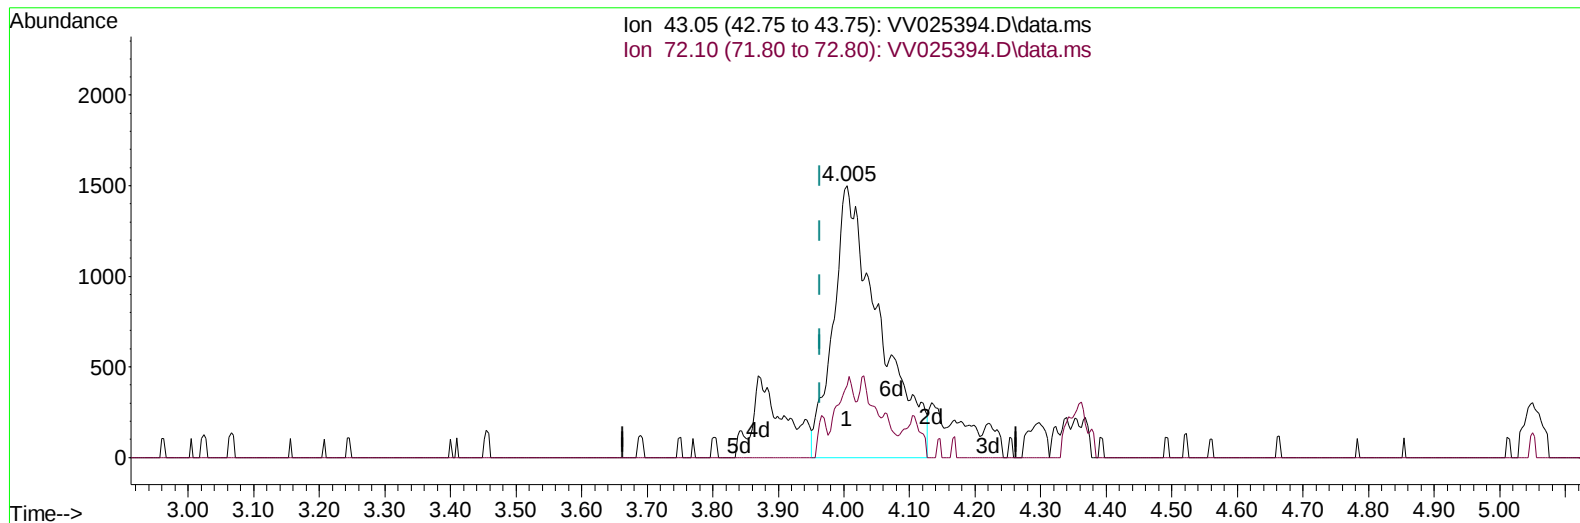

TIC: VV025394.D\data.ms

(21) 2-Butanone (T)

4.005min (+ 0.042) 4.65 ug/L m

response 7360

Ion	Exp%	Act%
43.05	100.00	100.00
72.10	23.60	7.96#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040722\
 Data File : VV025394.D
 Acq On : 07 Apr 2022 18:49
 Operator : SY/MD
 Sample : N2320-01
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YB2P3

Manual IntegrationsAPPROVED

Quant Time: Apr 08 01:24:33 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Apr 08 01:19:10 2022
 Response via : Initial Calibration

Reviewed By :John Carlone 04/08/2022
 Supervised By :Mahesh Dadoda 04/08/2022

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.619	114		161843	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117		153195	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152		69710	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.307	65		67329	4.454	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	89.000%	
7) Chloroethane-d5	1.568	69		62636	4.937	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	98.800%	
11) 1,1-Dichloroethene-d2	2.111	63		101208	3.091	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	61.800%	
20) 2-Butanone-d5	3.889	46		77432	51.420	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	102.840%	
24) Chloroform-d	4.352	84		94748	4.802	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.000%	
26) 1,2-Dichloroethane-d4	5.034	65		43272	4.962	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	99.200%	
32) Benzene-d6	5.053	84		199987	5.160	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	103.200%	
36) 1,2-Dichloropropane-d6	6.072	67		56032	5.159	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	103.200%	
41) Toluene-d8	7.317	98		177015	4.980	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	99.600%	
43) trans-1,3-Dichloroprop...	7.625	79		16627	4.692	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	93.800%	
46) 2-Hexanone-d5	8.088	63		57080	44.602	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	89.200%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84		33244	4.590	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	91.800%	
66) 1,2-Dichlorobenzene-d4	11.622	152		58663	5.240	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	104.800%	
Target Compounds							
21) 2-Butanone	4.005	43		7360m	4.655	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040722\
Data File : VV025394.D
Acq On : 07 Apr 2022 18:49
Operator : SY/MD
Sample : N2320-01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YB2P3

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 04/08/2022
Supervised By :Mahesh Dadoda 04/08/2022

Quant Time: Apr 08 01:24:33 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Apr 08 01:19:10 2022
Response via : Initial Calibration

