




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040722\
 Data File : VV025397.D
 Acq On : 07 Apr 2022 19:59
 Operator : SY/MD
 Sample : N2320-04
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YB2P6

Manual IntegrationsAPPROVED

Quant Time: Apr 08 01:25:19 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Apr 08 01:19:10 2022
 Response via : Initial Calibration

Reviewed By :John Carlone 04/08/2022
 Supervised By :Mahesh Dadoda 04/08/2022

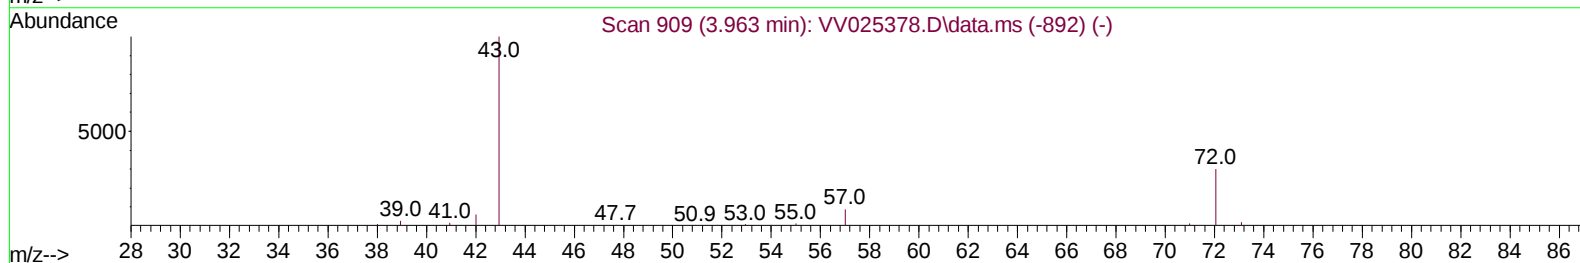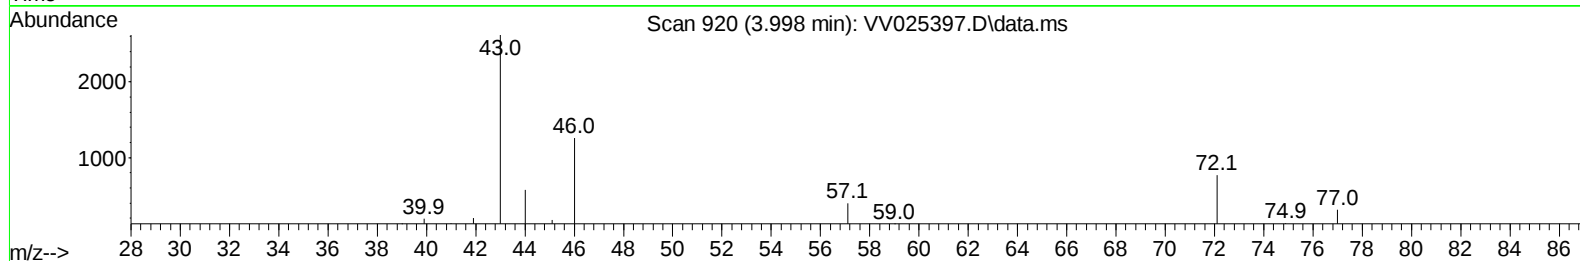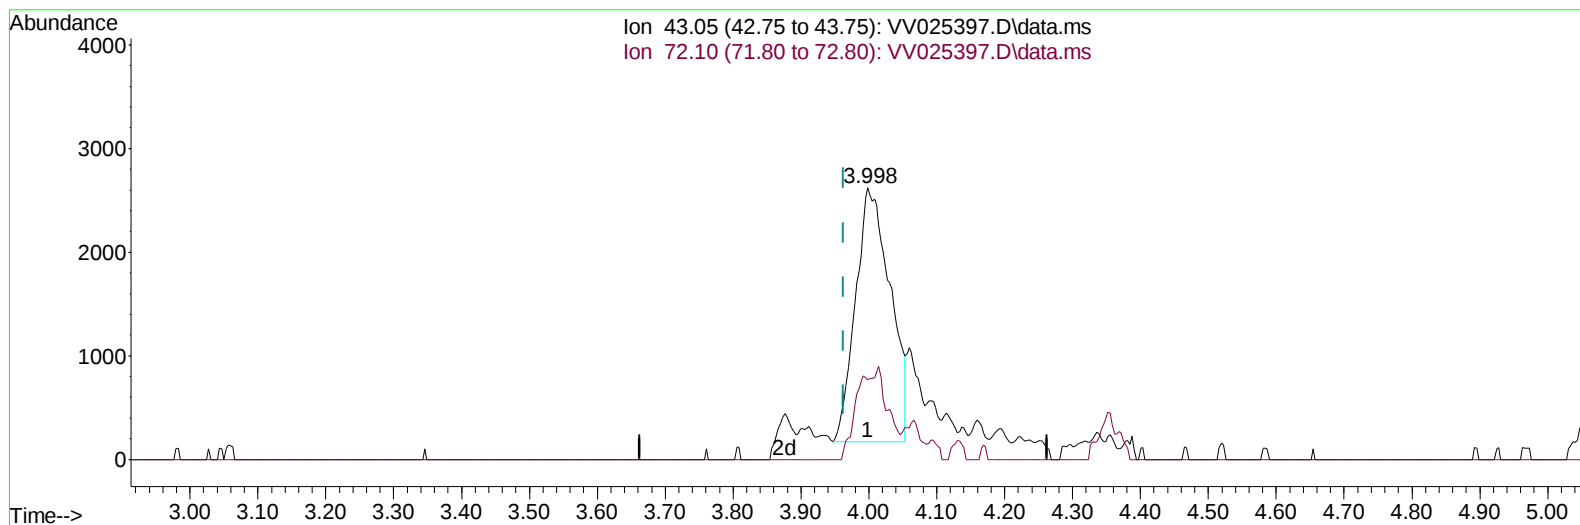

TIC: VV025397.D\data.ms

(21) 2-Butanone (T)

3.998min (+ 0.035) 5.63 ug/L

response 8667

Ion	Exp%	Act%
43.05	100.00	100.00
72.10	23.60	13.37
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040722\
 Data File : VV025397.D
 Acq On : 07 Apr 2022 19:59
 Operator : SY/MD
 Sample : N2320-04
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YB2P6

Manual IntegrationsAPPROVED

Quant Time: Apr 08 01:25:19 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Apr 08 01:19:10 2022
 Response via : Initial Calibration

Reviewed By :John Carlone 04/08/2022
 Supervised By :Mahesh Dadoda 04/08/2022

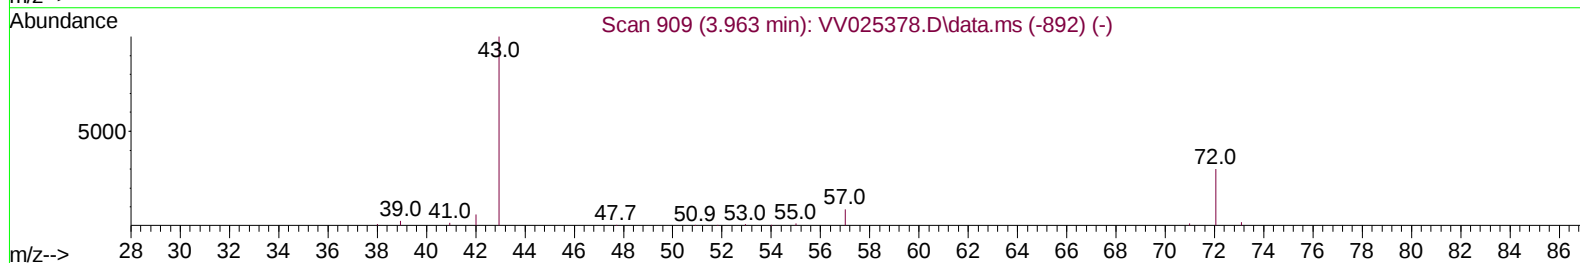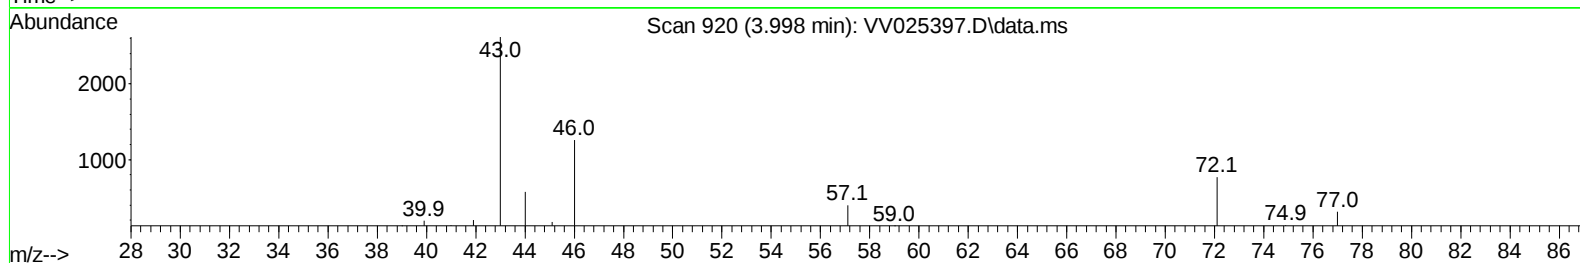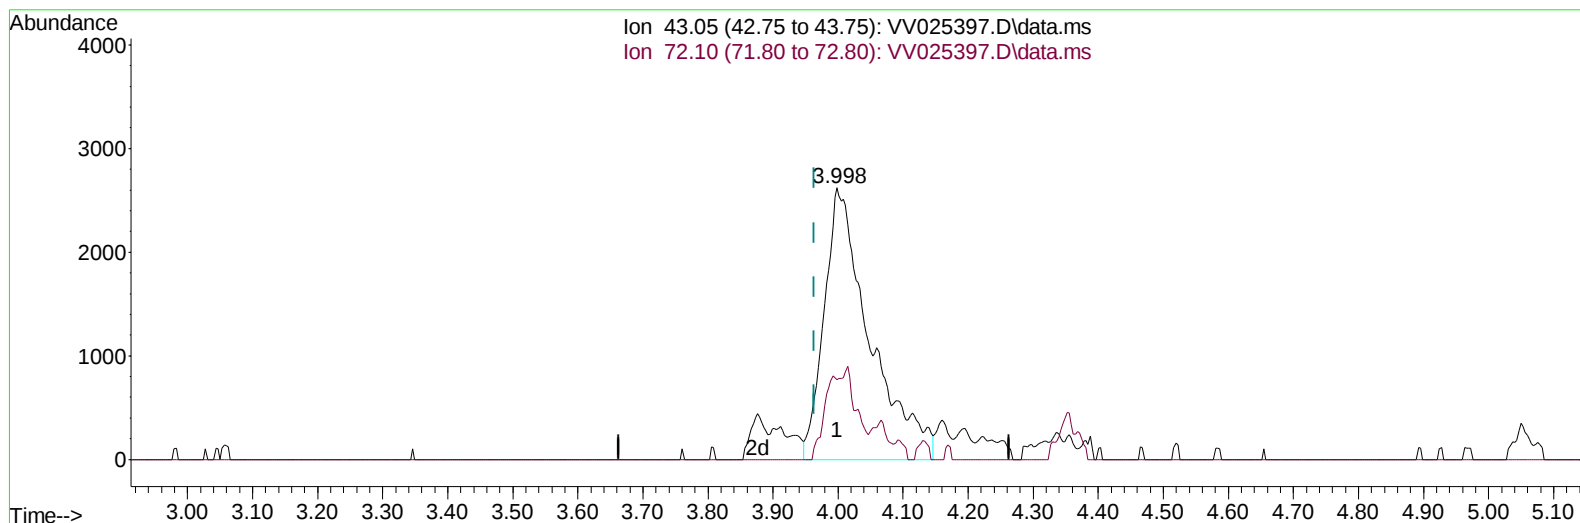

TIC: VV025397.D\data.ms

(21) 2-Butanone (T)

3.998min (+ 0.035) 8.26 ug/L m

response 12712

Ion	Exp%	Act%
43.05	100.00	100.00
72.10	23.60	9.12#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040722\
 Data File : VV025397.D
 Acq On : 07 Apr 2022 19:59
 Operator : SY/MD
 Sample : N2320-04
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YB2P6

Manual IntegrationsAPPROVED

Quant Time: Apr 08 01:25:19 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Apr 08 01:19:10 2022
 Response via : Initial Calibration

Reviewed By :John Carlone 04/08/2022
 Supervised By :Mahesh Dadoda 04/08/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	157610	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	149526	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	68753	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.310	65	75778	5.147	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130	Recovery	=	103.000%	
7) Chloroethane-d5	1.571	69	69315	5.610	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130	Recovery	=	112.200%	
11) 1,1-Dichloroethene-d2	2.111	63	113973	3.574	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125	Recovery	=	71.400%	
20) 2-Butanone-d5	3.889	46	88404	60.283	ug/L	0.00
Spiked Amount 50.000	Range 40	- 130	Recovery	=	120.560%	
24) Chloroform-d	4.352	84	106702	5.554	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	111.000%	
26) 1,2-Dichloroethane-d4	5.037	65	49014	5.772	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	115.400%	
32) Benzene-d6	5.050	84	227518	6.014	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	120.200%	
36) 1,2-Dichloropropane-d6	6.072	67	63357	5.976	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140	Recovery	=	119.600%	
41) Toluene-d8	7.317	98	199458	5.749	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	115.000%	
43) trans-1,3-Dichloroprop...	7.625	79	19064	5.512	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130	Recovery	=	110.200%	
46) 2-Hexanone-d5	8.088	63	66394	53.153	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130	Recovery	=	106.300%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	36431	5.154	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120	Recovery	=	103.000%	
66) 1,2-Dichlorobenzene-d4	11.622	152	67474	6.110	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120	Recovery	=	122.200%#	
Target Compounds						
14) Carbon disulfide	2.298	76	29625	0.901	ug/L	95
21) 2-Butanone	3.998	43	12712m	8.256	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040722\
Data File : VV025397.D
Acq On : 07 Apr 2022 19:59
Operator : SY/MD
Sample : N2320-04
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YB2P6

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 04/08/2022
Supervised By :Mahesh Dadoda 04/08/2022

Quant Time: Apr 08 01:25:19 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Apr 08 01:19:10 2022
Response via : Initial Calibration

