

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040722\
 Data File : VV025379.D
 Acq On : 07 Apr 2022 12:19
 Operator : SY/MD
 Sample : VV0407WBL01
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK336

Quant Time: Apr 07 15:10:13 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Apr 07 01:24:47 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	153421	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	144512	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	64735	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.310	65	76745	5.355	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	107.200%	
7) Chloroethane-d5	1.571	69	69490	5.777	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	115.600%	
11) 1,1-Dichloroethene-d2	2.108	63	113114	3.644	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	72.800%	
20) 2-Butanone-d5	3.883	46	76441	53.548	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	107.100%	
24) Chloroform-d	4.346	84	102266	5.468	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	109.400%	
26) 1,2-Dichloroethane-d4	5.031	65	45019	5.446	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	109.000%	
32) Benzene-d6	5.047	84	212031	5.800	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	116.000%	
36) 1,2-Dichloropropane-d6	6.066	67	59656	5.822	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	116.400%	
41) Toluene-d8	7.313	98	187278	5.585	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	111.600%	
43) trans-1,3-Dichloroprop...	7.622	79	18255	5.461	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	109.200%	
46) 2-Hexanone-d5	8.085	63	59124	48.976	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	97.960%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	35456	5.190	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	103.800%	
66) 1,2-Dichlorobenzene-d4	11.622	152	62001	5.963	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	119.200%	
Target Compounds						Qvalue
16) Methylene chloride	2.506	84	5419	0.447	ug/L	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040722\
Data File : VV025379.D
Acq On : 07 Apr 2022 12:19
Operator : SY/MD
Sample : VV0407WBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK336


Quant Time: Apr 07 15:10:13 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Apr 07 01:24:47 2022
Response via : Initial Calibration

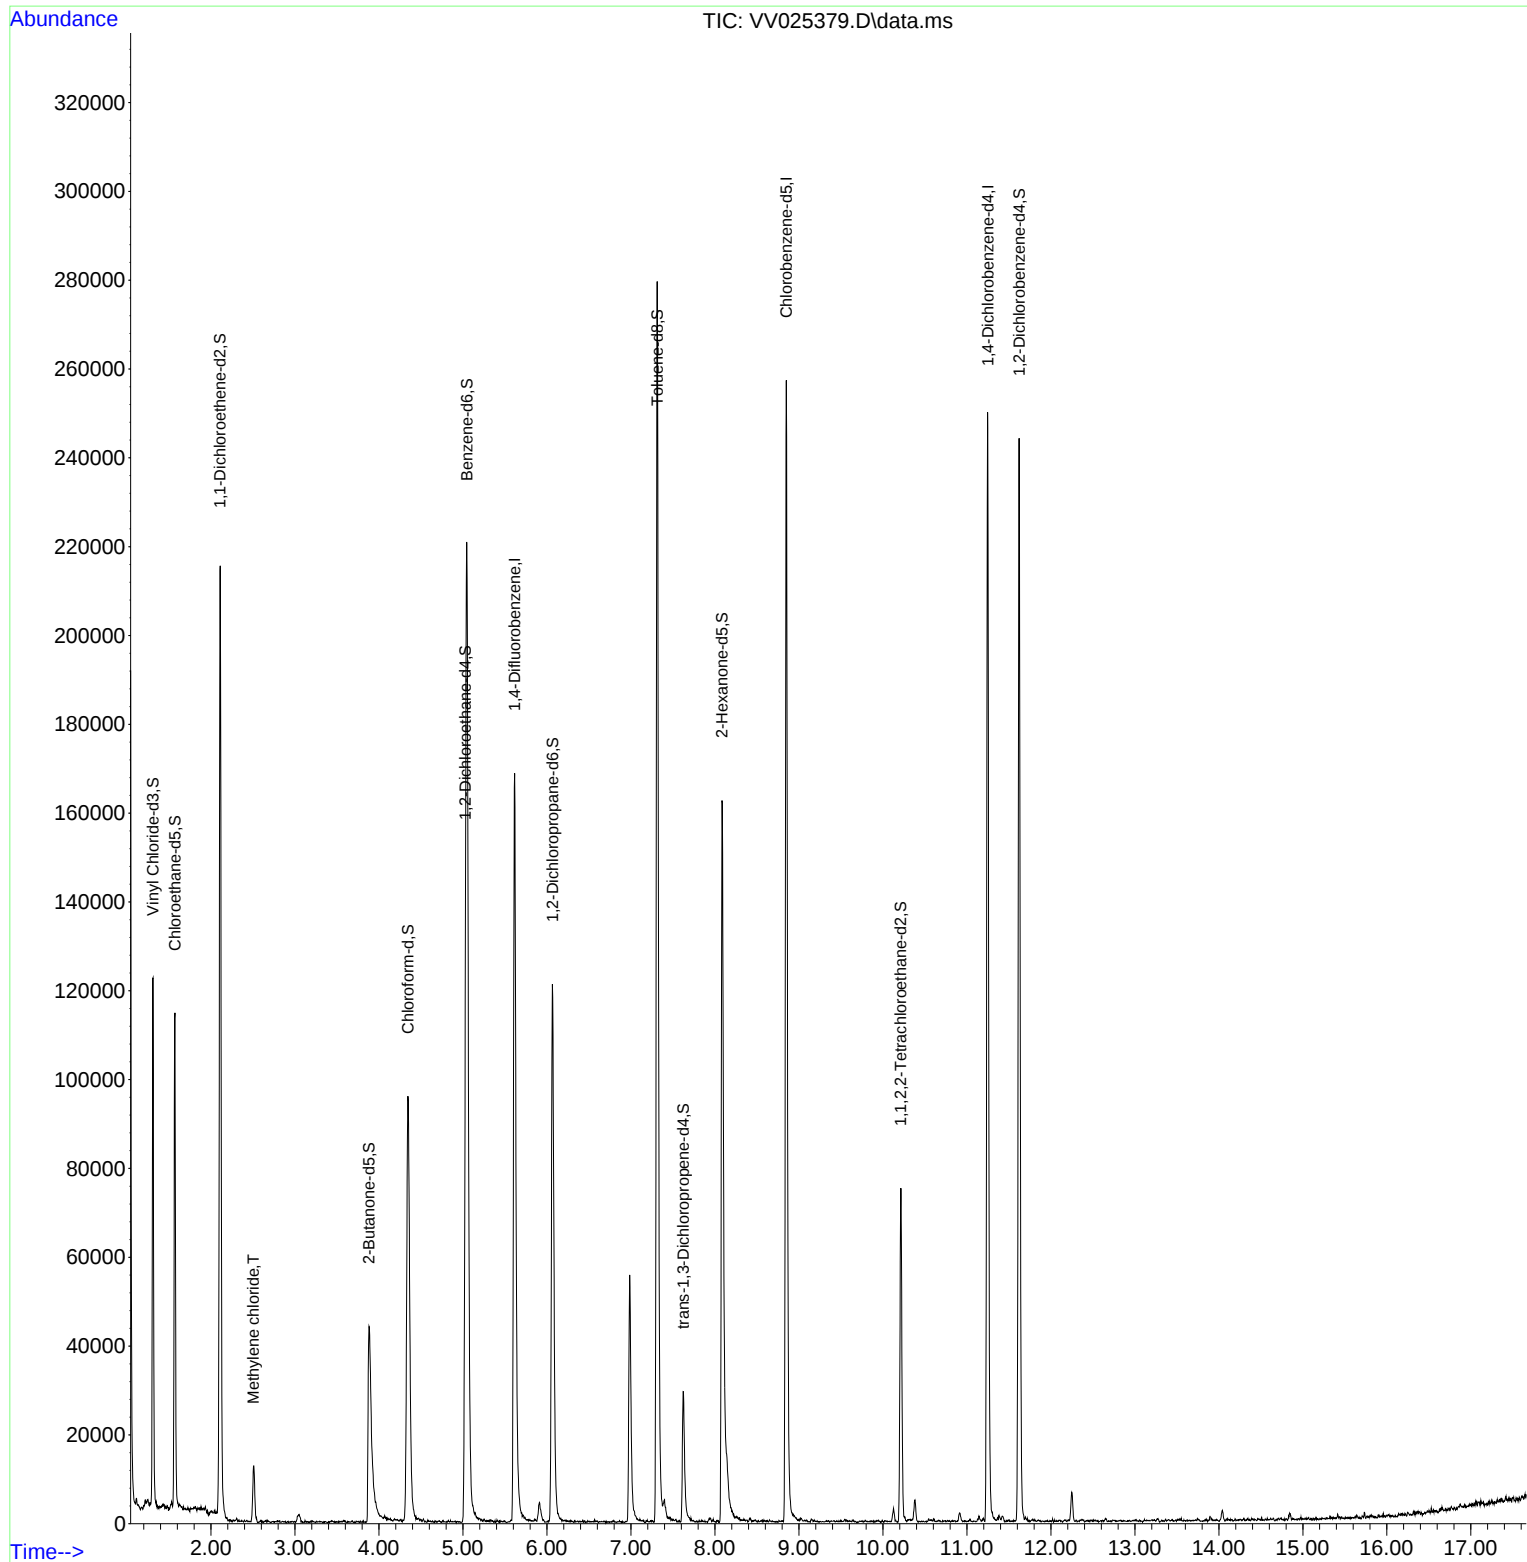

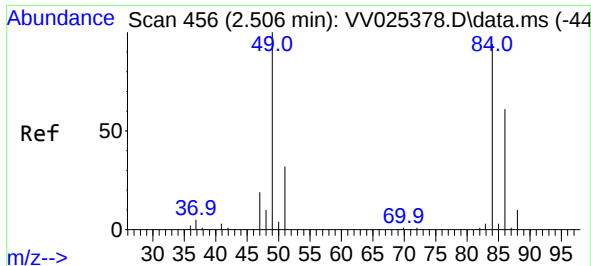

#16
Methylene chloride
Concen: 0.447 ug/L
RT: 2.506 min Scan# 4
Delta R.T. 0.003 min
Lab File: VV025379.D
Acq: 07 Apr 2022 12:19

Instrument :
MSVOA_V
ClientSampleId :
VBLK336

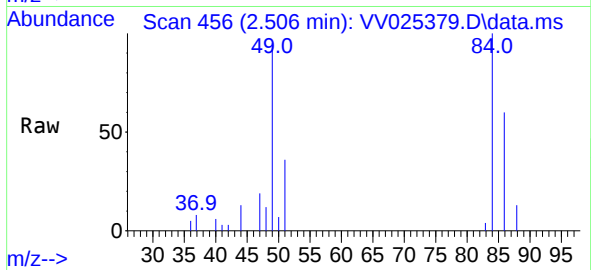

Tgt Ion: 84 Resp: 5419

Ion	Ratio	Lower	Upper
84	100		
86	59.8	43.5	80.7
49	95.2	74.5	138.3

