

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW040722\
 Data File : VW025388.D
 Acq On : 07 Apr 2022 16:28
 Operator : SY/MD
 Sample : N2262-21
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW6R2

Quant Time: Apr 08 01:23:06 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Apr 08 01:19:10 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	168125	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	157753	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	71130	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	80790	5.144	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	102.800%
7) Chloroethane-d5	1.571	69	71495	5.424	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	108.400%
11) 1,1-Dichloroethene-d2	2.111	63	121161	3.562	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	71.200%
20) 2-Butanone-d5	3.892	46	99132	63.370	ug/L	0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	126.740%
24) Chloroform-d	4.352	84	114963	5.609	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	112.200%
26) 1,2-Dichloroethane-d4	5.037	65	52328	5.777	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	115.600%
32) Benzene-d6	5.050	84	247719	6.207	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	124.200%
36) 1,2-Dichloropropane-d6	6.069	67	69316	6.197	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	124.000%
41) Toluene-d8	7.317	98	218042	5.956	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	119.200%
43) trans-1,3-Dichloroprop...	7.625	79	22042	6.041	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	120.800%
46) 2-Hexanone-d5	8.088	63	78687	59.710	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	119.420%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	42143	5.651	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	113.000%
66) 1,2-Dichlorobenzene-d4	11.622	152	72038	6.306	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	126.200%#
Target Compounds						
16) Methylene chloride	2.510	84	7185	0.541	ug/L	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040722\
Data File : VV025388.D
Acq On : 07 Apr 2022 16:28
Operator : SY/MD
Sample : N2262-21
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6R2

Quant Time: Apr 08 01:23:06 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Apr 08 01:19:10 2022
Response via : Initial Calibration

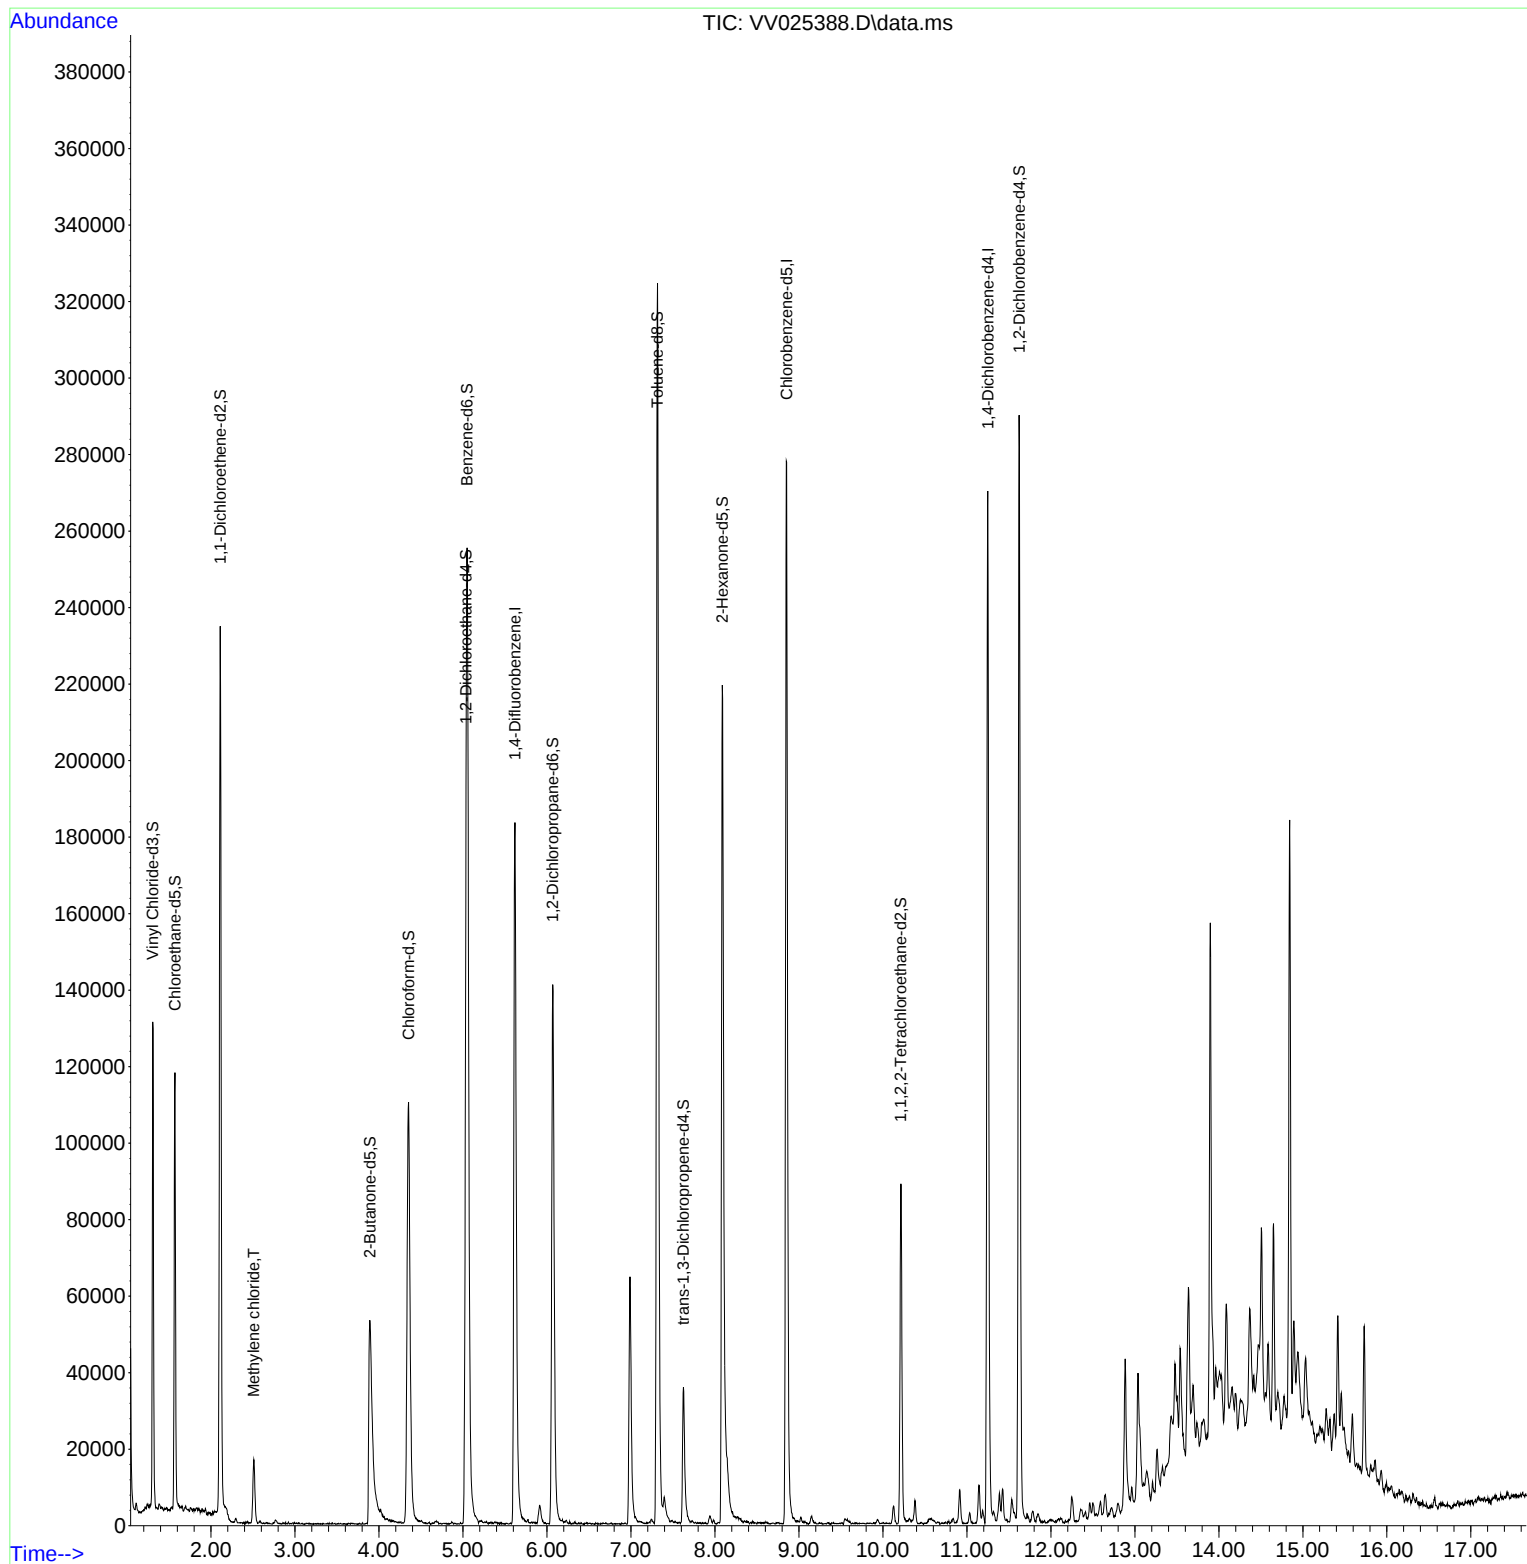

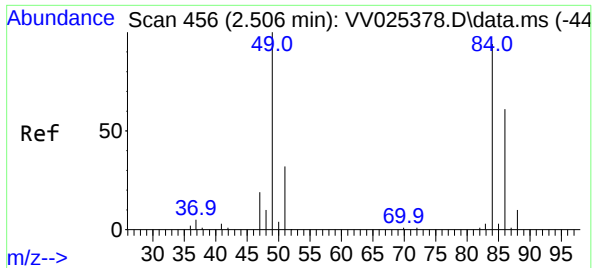

#16
Methylene chloride
Concen: 0.541 ug/L
RT: 2.510 min Scan# 4
Delta R.T. 0.003 min
Lab File: VV025388.D
Acq: 07 Apr 2022 16:28

Instrument :
MSVOA_V
ClientSampleId :
EW6R2

Tgt Ion: 84 Resp: 7185
Ion Ratio Lower Upper
84 100
86 62.5 43.5 80.7
49 103.9 74.5 138.3

