

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040722\
 Data File : VV025394.D
 Acq On : 07 Apr 2022 18:49
 Operator : SY/MD
 Sample : N2320-01
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YB2P3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV025394.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.217	50	55	60	rBV	8649	7040	1.36%	0.151%
2	1.307	74	83	101	rVB	110094	118980	22.91%	2.545%
3	1.571	157	165	180	rVB	103510	114261	22.00%	2.444%
4	2.111	323	333	346	rVV	193135	279396	53.79%	5.977%
5	3.889	873	886	912	rBV2	43730	129687	24.97%	2.774%
6	4.352	1010	1030	1056	rBV2	88408	223260	42.98%	4.776%
7	5.050	1231	1247	1272	rBV2	209603	519395	100.00%	11.111%
8	5.619	1411	1424	1452	rBV	180614	370298	71.29%	7.921%
9	5.911	1506	1515	1518	rBV6	3712	5603	1.08%	0.120%
10	6.072	1552	1565	1585	rBV2	113383	238582	45.93%	5.104%
11	6.989	1838	1850	1873	rBV2	49478	94786	18.25%	2.028%
12	7.317	1940	1952	1970	rBV	260147	457733	88.13%	9.792%
13	7.400	1973	1978	1994	rVB2	8525	15905	3.06%	0.340%
14	7.625	2038	2048	2070	rBV	26097	49243	9.48%	1.053%
15	7.937	2136	2145	2153	rBV5	3068	5492	1.06%	0.117%
16	8.088	2183	2192	2233	rBV	156219	329886	63.51%	7.057%
17	8.853	2418	2430	2454	rBV	267563	444104	85.50%	9.500%
18	9.146	2513	2521	2535	rVB4	4468	8011	1.54%	0.171%
19	9.551	2638	2647	2657	rBV2	6569	11288	2.17%	0.241%
20	10.217	2839	2854	2873	rBV	70198	112830	21.72%	2.414%
21	10.381	2897	2905	2917	rVB5	6248	10028	1.93%	0.215%
22	11.143	3134	3142	3154	rBV8	3373	6470	1.25%	0.138%
23	11.246	3164	3174	3195	rBV	264850	419507	80.77%	8.974%
24	11.532	3252	3263	3280	rBV3	18869	37519	7.22%	0.803%
25	11.622	3280	3291	3313	rVB	233307	371971	71.62%	7.957%
26	12.252	3475	3487	3495	rBV2	4617	6702	1.29%	0.143%
27	12.342	3508	3515	3527	rBV5	8834	14184	2.73%	0.303%
28	12.885	3672	3684	3695	rBV6	11188	20236	3.90%	0.433%
29	13.037	3721	3731	3749	rBV8	8960	21610	4.16%	0.462%
30	13.538	3881	3887	3900	rVB10	6258	11339	2.18%	0.243%
31	13.641	3906	3919	3926	rBV5	12929	26055	5.02%	0.557%
32	13.898	3990	3999	4006	rBV	37152	53753	10.35%	1.150%
33	14.088	4051	4058	4067	rVB6	8399	12481	2.40%	0.267%
34	14.506	4182	4188	4198	rVB4	12211	18951	3.65%	0.405%
35	14.651	4226	4233	4242	rVB3	12540	15827	3.05%	0.339%
36	14.844	4284	4293	4301	rBV3	40285	57171	11.01%	1.223%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040722\
Data File : VV025394.D
Acq On : 07 Apr 2022 18:49
Operator : SY/MD
Sample : N2320-01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YB2P3

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.1 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Title : TRACE VOA SFAM1.0

37	14.889	4303	4307	4315	rVV8	5333	7419	1.43%	0.159%
38	15.413	4465	4470	4478	rBV5	7040	9609	1.85%	0.206%
39	15.596	4520	4527	4534	rVB10	4198	6724	1.29%	0.144%
40	15.731	4561	4569	4578	rBV4	8021	11344	2.18%	0.243%


Sum of corrected areas: 4674680

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040722\
Data File : VV025394.D
Acq On : 07 Apr 2022 18:49
Operator : SY/MD
Sample : N2320-01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YB2P3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

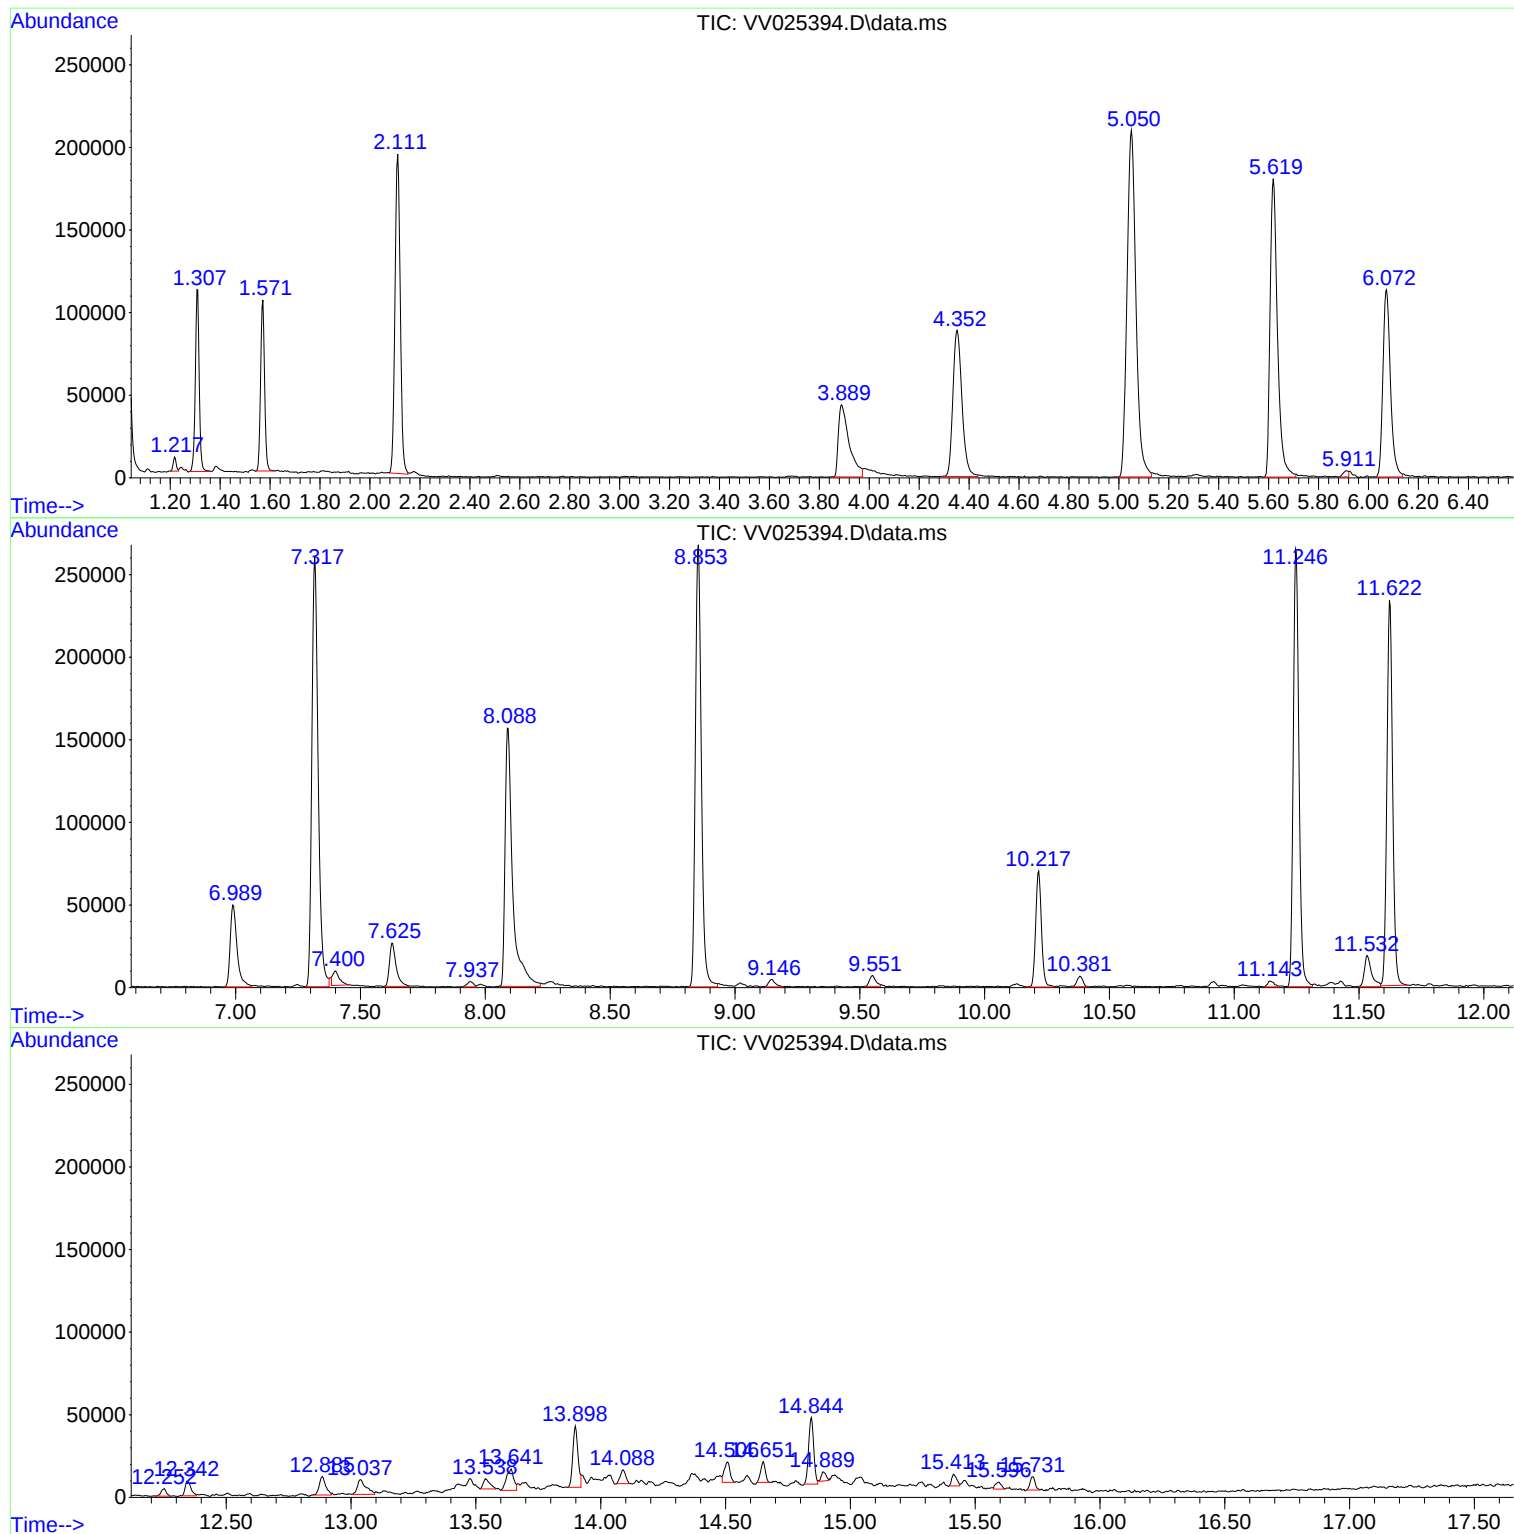

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040722\
Data File : VV025394.D
Acq On : 07 Apr 2022 18:49
Operator : SY/MD
Sample : N2320-01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YB2P3










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 (DEL) Alkane: Straight-Chai... Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
13.898	0.64 ug/L	53753	1,4-Dichlorobenzene-d4	11.249

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Tridecane	184	C13H28	000629-50-5	94
2			Tetradecane	198	C14H30	000629-59-4	80
3			Carbonic acid, nonyl vinyl ester	214	C12H22O3	1000383-25-6	80
4			Tetradecane	198	C14H30	000629-59-4	72
5			Hexadecane	226	C16H34	000544-76-3	72

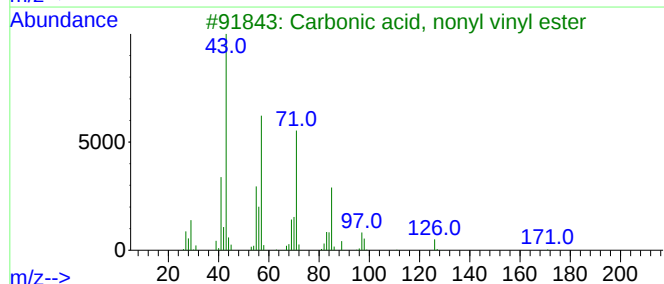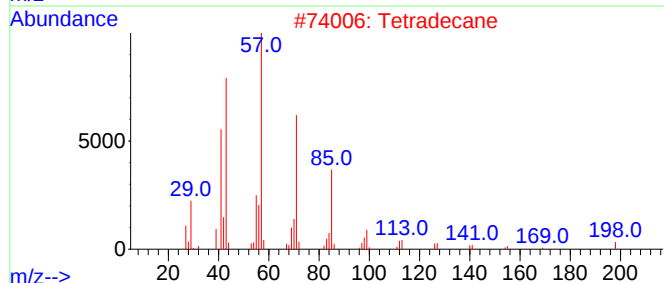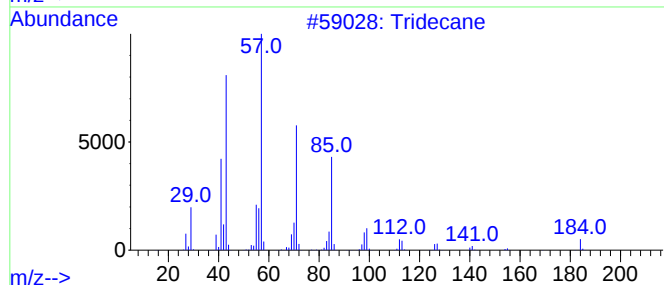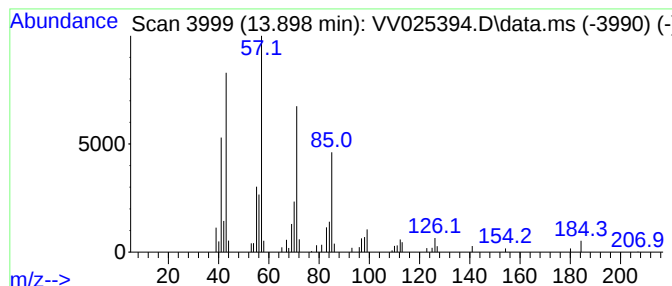

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040722\
Data File : VV025394.D
Acq On : 07 Apr 2022 18:49
Operator : SY/MD
Sample : N2320-01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YB2P3










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 3 (DEL) Alkane: Straight-Chai... Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
14.844	0.68 ug/L	57171	1,4-Dichlorobenzene-d4	11.249

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Tetradecane	198	C14H30	000629-59-4	97
2			Tetradecane	198	C14H30	000629-59-4	96
3			Tetradecane	198	C14H30	000629-59-4	89
4			Carbonic acid, undecyl vinyl ester	242	C14H26O3	1000382-54-9	86
5			Hexadecane	226	C16H34	000544-76-3	83

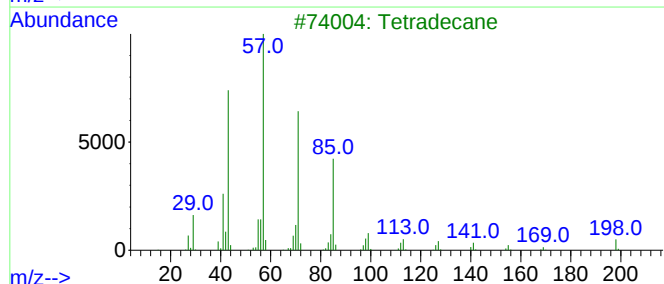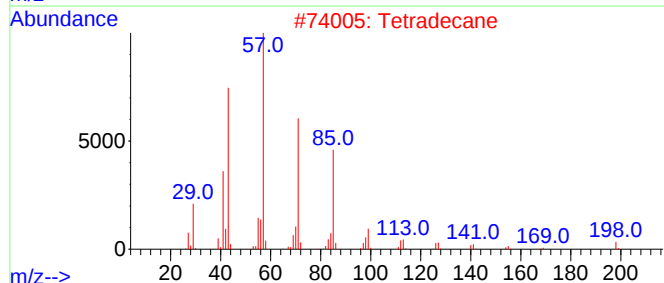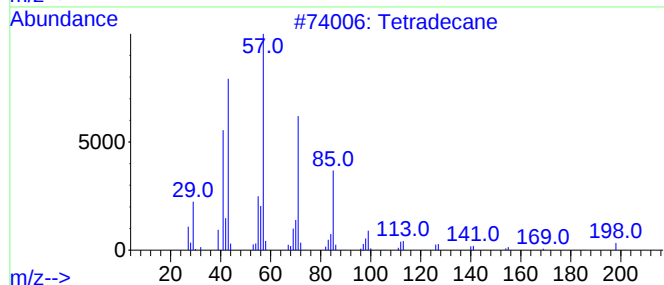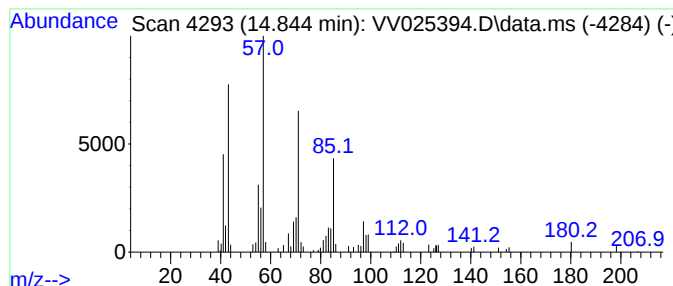

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040722\
Data File : VV025394.D
Acq On : 07 Apr 2022 18:49
Operator : SY/MD
Sample : N2320-01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YB2P3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	13.898	0.6	ug/L	53753	3	11.249	419507	5.0
(DEL) Alkane: S...	14.844	0.7	ug/L	57171	3	11.249	419507	5.0