
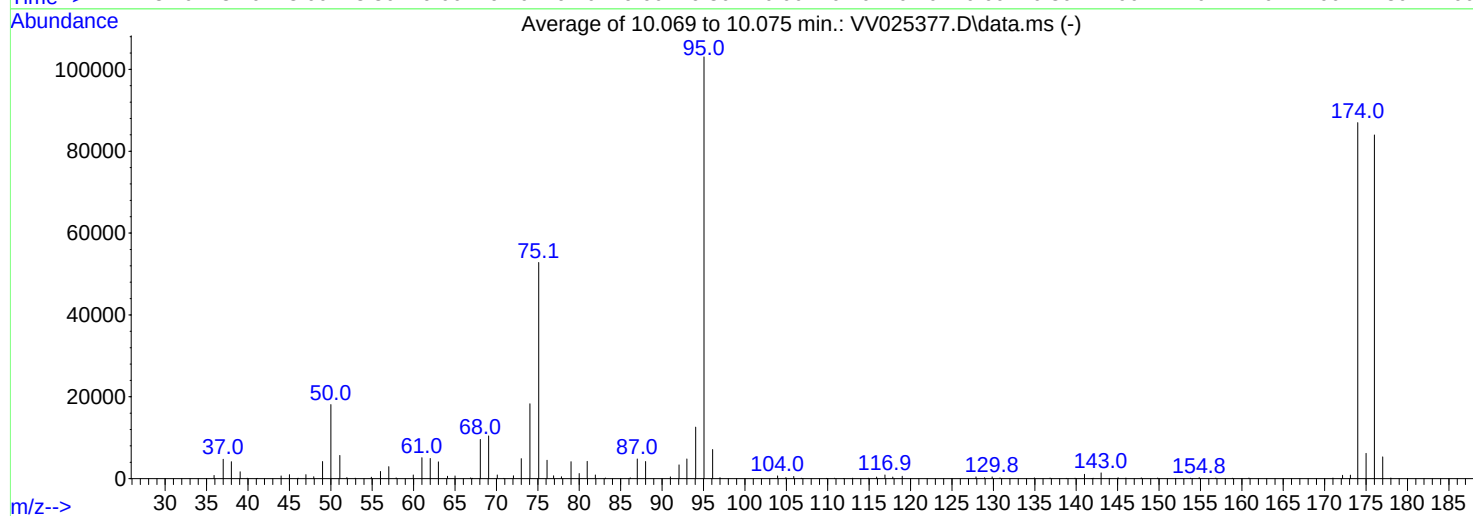


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040722\
 Data File : VV025377.D
 Acq On : 07 Apr 2022 09:38
 Operator : SY/MD
 Sample : BFB297
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB297

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Fri Apr 08 01:19:10 2022

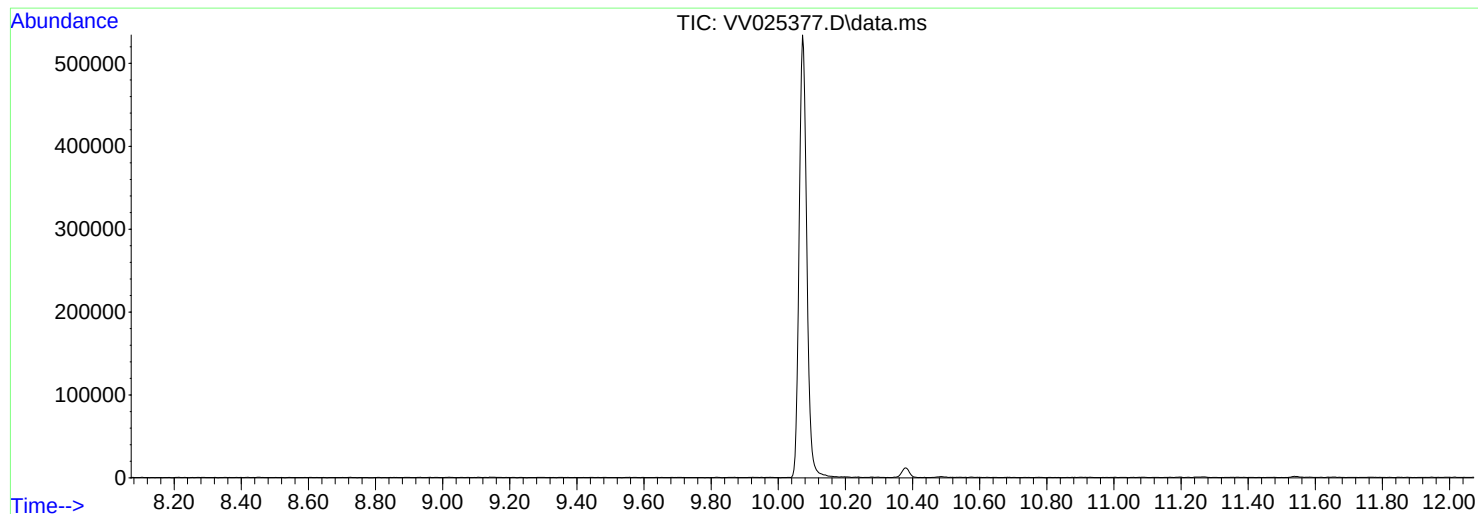

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.6	18104	PASS
75	95	30	80	51.2	52808	PASS
95	95	100	100	100.0	103064	PASS
96	95	5	9	6.9	7121	PASS
173	174	0.00	2	1.0	858	PASS
174	95	50	120	84.4	87000	PASS
175	174	5	9	7.1	6183	PASS
176	174	95	105	96.5	83971	PASS
177	176	5	10	6.3	5308	PASS

m/z	Abundance
35.90	126.0
39.90	141.0
41.60	112.0
44.00	298.0

Instrument :
MSVOA_V
ClientSampleId :
BFB297

m/z	Abundance
35.90	897.0
37.00	4643.0
38.00	4171.0
39.00	1784.0
39.90	287.0
44.00	942.0
45.00	925.0
46.10	131.0
47.00	915.0
47.90	478.0
49.00	4272.0
50.00	17768.0
51.10	5476.0
52.00	276.0
52.90	104.0
54.90	405.0
56.00	1725.0
57.00	2707.0
57.90	174.0
60.00	870.0
61.00	4906.0
62.00	4971.0
63.00	4193.0
64.10	605.0
65.00	607.0
66.90	277.0
68.10	9426.0
69.00	10152.0
70.10	914.0
72.10	606.0
73.00	5018.0
74.10	17912.0
75.10	50856.0
76.10	4397.0
76.90	695.0
77.80	484.0
79.00	3935.0
80.00	1274.0
81.00	4003.0
82.00	876.0
83.20	167.0
87.00	4696.0
88.00	3831.0
91.00	465.0
92.00	3218.0
93.00	4843.0
94.00	12186.0
95.10	99496.0
96.10	7271.0
97.00	265.0
104.00	700.0
104.90	247.0
105.90	554.0
106.80	151.0
109.90	120.0
111.00	115.0
114.90	145.0
115.90	365.0
116.90	937.0
117.90	374.0
119.00	561.0
127.90	402.0
129.00	214.0
129.80	412.0
130.80	115.0
134.90	251.0
136.80	202.0
138.80	112.0
139.90	128.0
141.00	996.0
141.90	153.0
143.00	1219.0
145.10	259.0
146.00	154.0
147.90	172.0
149.90	138.0
153.80	134.0
154.90	286.0
156.90	186.0
158.80	121.0
160.80	142.0
170.90	179.0
172.10	756.0
174.00	81968.0
175.00	5759.0
176.00	78696.0
177.00	5003.0
178.00	207.0

Instrument :
MSVOA_V
ClientSampleId :
BFB297

m/z	Abundance
35.90	962.0
37.00	4990.0
38.00	4274.0
39.00	1707.0
39.90	281.0
41.10	111.0
44.00	980.0
45.00	1045.0
46.10	133.0
47.00	1028.0
47.90	482.0
49.00	4329.0
50.00	18600.0
51.10	5848.0
52.00	277.0
53.00	107.0
54.90	337.0
56.00	1809.0
57.00	3072.0
57.90	221.0
59.90	927.0
61.00	5358.0
62.00	5152.0
63.00	4197.0
64.10	610.0
65.00	707.0
66.90	279.0
68.10	9926.0
69.00	10838.0
70.10	936.0
70.90	107.0
72.00	709.0
73.00	5087.0
74.10	18904.0
75.10	54680.0
76.10	4723.0
76.90	765.0
77.80	496.0
79.00	4323.0
80.00	1282.0
81.00	4373.0
81.90	909.0
83.20	157.0
86.20	268.0
87.00	5039.0
88.00	4294.0
91.00	451.0
92.10	3511.0
93.00	4939.0
94.00	13049.0
95.10	106360.0
96.10	7346.0
97.00	279.0
103.90	674.0
104.90	275.0
105.90	543.0
106.80	153.0
109.80	119.0
110.80	121.0
111.90	102.0
113.00	129.0
114.90	133.0
115.90	395.0
116.90	952.0
117.90	394.0
119.00	606.0
127.90	432.0
129.00	246.0
129.80	456.0
130.80	220.0
134.90	215.0
136.90	180.0
138.80	107.0
139.80	125.0
141.00	1116.0
142.10	153.0
143.00	1484.0
144.10	123.0
145.10	259.0
146.00	136.0
147.80	202.0
149.90	144.0
152.00	109.0
153.80	143.0
154.90	277.0
156.80	163.0
158.80	122.0
160.80	162.0
171.00	149.0
172.20	868.0
173.10	1284.0
174.00	89968.0

Instrument :
MSVOA_V
ClientSampleId :
BFB297

175.00	6346.0
176.00	87208.0
177.00	5464.0
178.00	183.0

Instrument :
MSVOA_V
ClientSampleId :
BFB297

m/z	Abundance
36.00	816.0
37.00	4585.0
38.00	4045.0
39.10	1537.0
40.00	225.0
41.10	117.0
44.00	964.0
45.00	993.0
46.00	136.0
47.00	999.0
48.00	483.0
49.00	3929.0
50.00	17944.0
51.10	5644.0
51.90	231.0
53.00	127.0
54.90	310.0
56.00	1715.0
57.00	2986.0
57.90	240.0
60.00	897.0
61.00	5151.0
62.00	4603.0
63.00	3912.0
64.10	539.0
65.00	679.0
67.10	297.0
68.00	9392.0
69.10	10376.0
70.10	879.0
70.90	104.0
72.00	750.0
73.00	4615.0
74.00	18136.0
75.10	52888.0
76.10	4413.0
76.90	673.0
77.90	460.0
79.00	4166.0
80.00	1174.0
80.90	4256.0
81.90	954.0
83.00	134.0
86.10	304.0
87.00	4729.0
88.00	4443.0
91.00	434.0
92.00	3397.0
93.00	4657.0
94.10	12573.0
95.00	103336.0
96.10	6746.0
97.00	220.0
103.90	577.0
105.00	251.0
105.90	519.0
107.00	130.0
110.80	118.0
113.00	175.0
114.90	125.0
115.90	387.0
116.90	858.0
117.80	453.0
119.00	595.0
127.90	401.0
128.90	252.0
129.90	460.0
130.80	289.0
135.00	178.0
136.90	152.0
139.80	101.0
141.00	1107.0
142.00	190.0
143.00	1541.0
144.00	124.0
145.00	244.0
146.00	145.0
147.90	225.0
149.80	140.0
152.00	116.0
153.80	117.0
154.80	233.0
156.80	137.0
158.90	115.0
160.90	164.0
171.10	135.0
172.20	853.0
173.10	1290.0
174.00	89064.0
175.00	6443.0
176.00	86008.0
177.00	5458.0

Instrument :
MSVOA_V
ClientSampleId :
BFB297

178.00

140.0

Instrument :
MSVOA_V
ClientSampleId :
BFB297