




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040822\
 Data File : VV025416.D
 Acq On : 08 Apr 2022 17:34
 Operator : SY/MD
 Sample : N2320-02
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YB2P4

Manual IntegrationsAPPROVED

Quant Time: Apr 09 05:10:12 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Apr 09 04:40:11 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 04/11/2022
 Supervised By :Mahesh Dadoda 04/13/2022

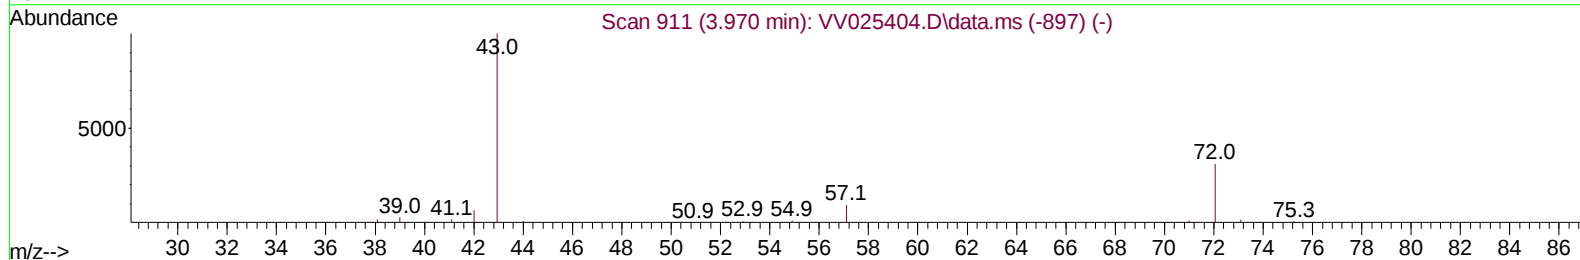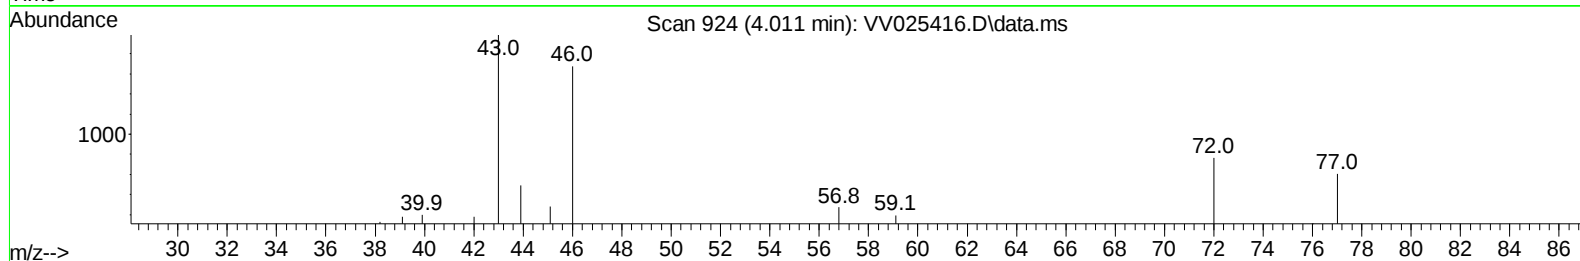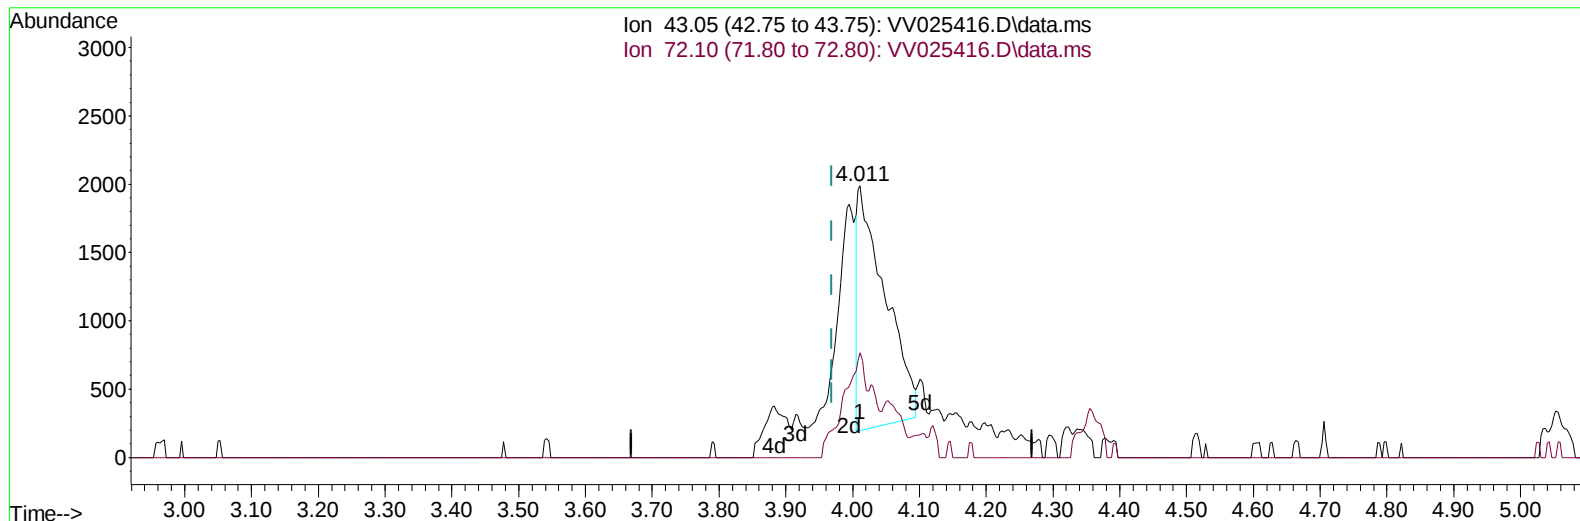

TIC: VV025416.D\data.ms

(21) 2-Butanone (T)

4.011min (+ 0.042) 2.85 ug/L

response 5087

Ion	Exp%	Act%
43.05	100.00	100.00
72.10	30.40	35.40
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040822\
 Data File : VV025416.D
 Acq On : 08 Apr 2022 17:34
 Operator : SY/MD
 Sample : N2320-02
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YB2P4

Manual IntegrationsAPPROVED

Quant Time: Apr 09 05:10:12 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Apr 09 04:40:11 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 04/11/2022
 Supervised By :Mahesh Dadoda 04/13/2022

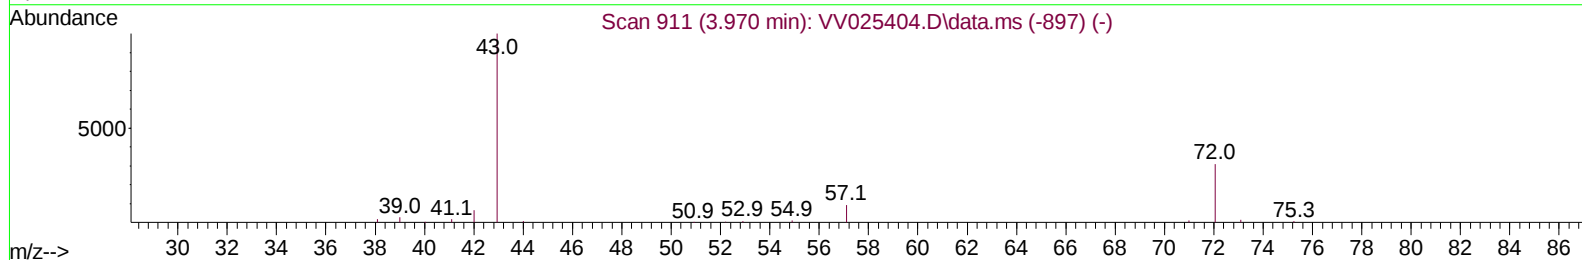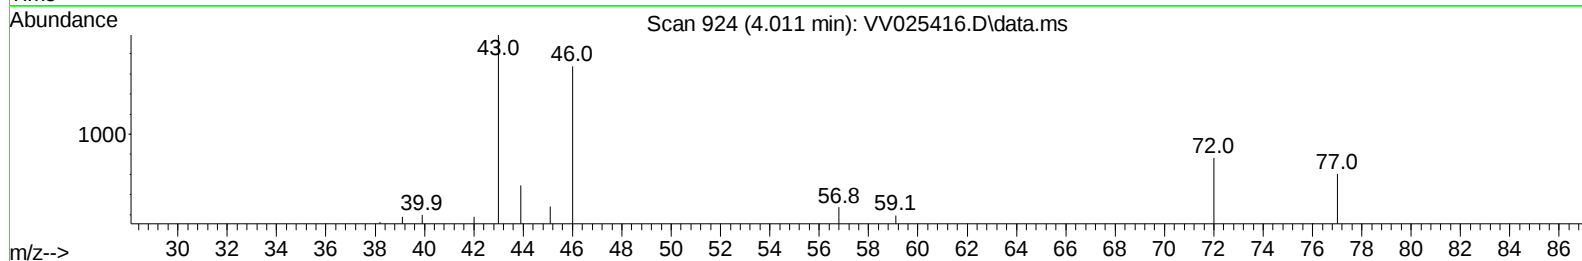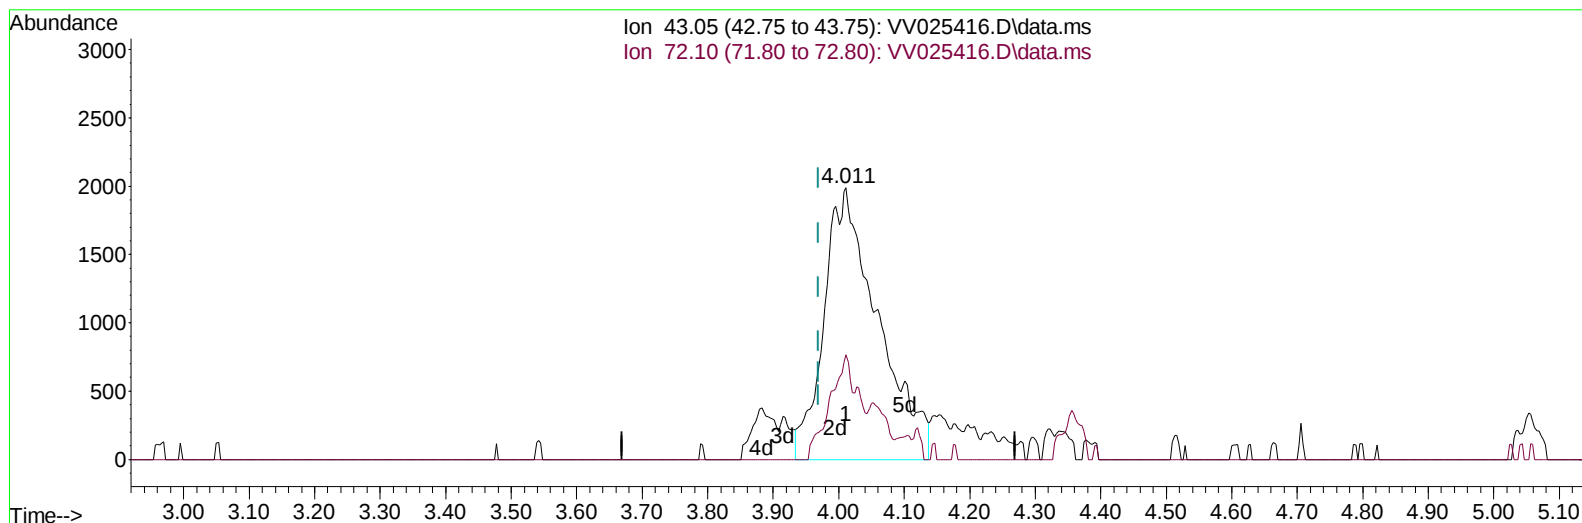

TIC: VV025416.D\data.ms

(21) 2-Butanone (T)

4.011min (+ 0.042) 6.35 ug/L m

response 11314

Ion	Exp%	Act%
43.05	100.00	100.00
72.10	30.40	15.92
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040822\
 Data File : VV025416.D
 Acq On : 08 Apr 2022 17:34
 Operator : SY/MD
 Sample : N2320-02
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YB2P4

Manual IntegrationsAPPROVED

Quant Time: Apr 09 05:10:12 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Apr 09 04:40:11 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 04/11/2022
 Supervised By :Mahesh Dadoda 04/13/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	167996	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	165514	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	79779	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.310	65	71496	4.578	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130	Recovery	=	91.600%	
7) Chloroethane-d5	1.571	69	65247	3.927	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130	Recovery	=	78.600%	
11) 1,1-Dichloroethene-d2	2.111	63	108614	3.471	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125	Recovery	=	69.400%	
20) 2-Butanone-d5	3.902	46	96282	50.678	ug/L	0.02
Spiked Amount 50.000	Range 40	- 130	Recovery	=	101.360%	
24) Chloroform-d	4.352	84	109338	4.633	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	92.600%	
26) 1,2-Dichloroethane-d4	5.037	65	51000	5.015	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	100.400%	
32) Benzene-d6	5.050	84	226340	4.726	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	94.600%	
36) 1,2-Dichloropropane-d6	6.069	67	63196	4.732	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140	Recovery	=	94.600%	
41) Toluene-d8	7.317	98	197543	4.445	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	88.800%	
43) trans-1,3-Dichloroprop...	7.625	79	20612	4.592	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130	Recovery	=	91.800%	
46) 2-Hexanone-d5	8.088	63	74966	47.582	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130	Recovery	=	95.160%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	38326	4.542	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120	Recovery	=	90.800%	
66) 1,2-Dichlorobenzene-d4	11.622	152	68810	5.144	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120	Recovery	=	102.800%	
Target Compounds						
14) Carbon disulfide	2.297	76	2638	0.076	ug/L #	91
21) 2-Butanone	4.011	43	11314m	6.350	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040822\
Data File : VV025416.D
Acq On : 08 Apr 2022 17:34
Operator : SY/MD
Sample : N2320-02
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YB2P4

Manual IntegrationsAPPROVED

Quant Time: Apr 09 05:10:12 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Apr 09 04:40:11 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 04/11/2022
Supervised By :Mahesh Dadoda 04/13/2022

