




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040822\
Data File : VV025418.D
Acq On : 08 Apr 2022 18:21
Operator : SY/MD
Sample : N2320-05
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YB2P7

Manual IntegrationsAPPROVED

Quant Time: Apr 09 05:10:37 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Apr 09 04:40:11 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 04/11/2022
Supervised By :Mahesh Dadoda 04/13/2022

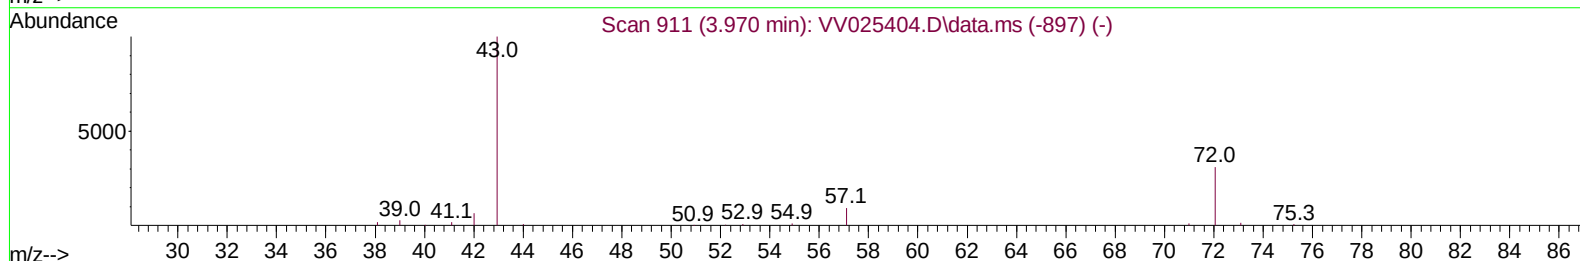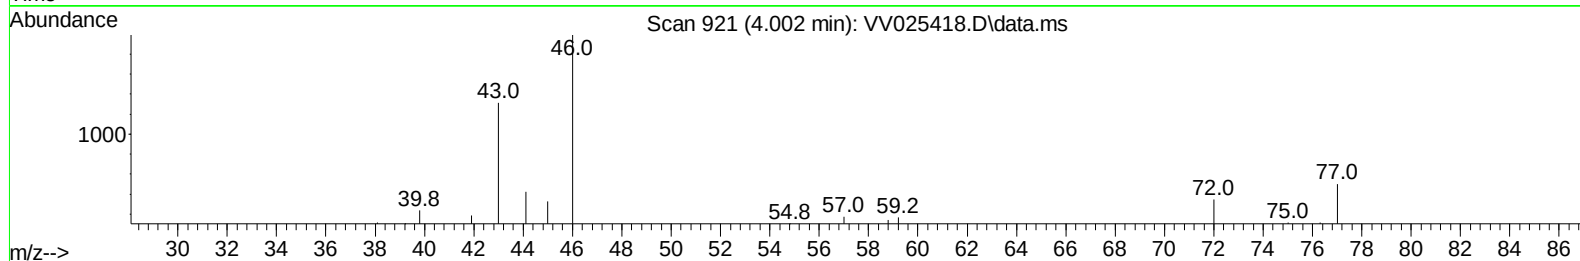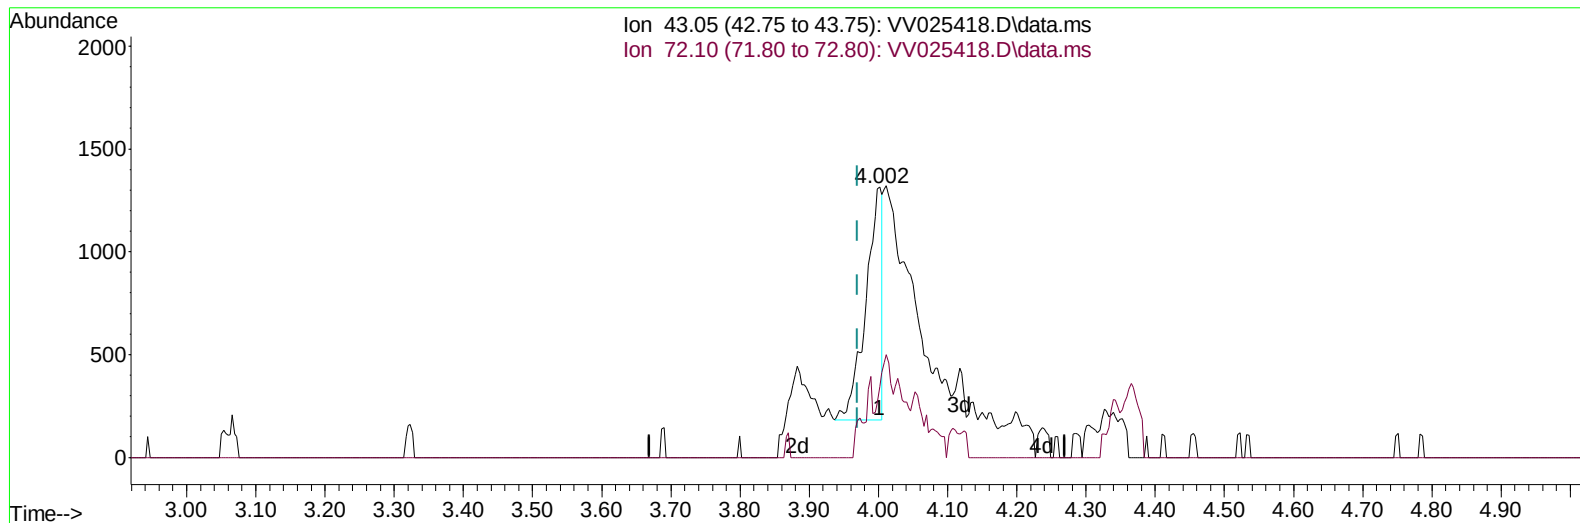

TIC: VV025418.D\data.ms

(21) 2-Butanone (T)

4.002min (+ 0.032) 1.00 ug/L

response 1858

Ion	Exp%	Act%
43.05	100.00	100.00
72.10	30.40	27.56
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040822\
 Data File : VV025418.D
 Acq On : 08 Apr 2022 18:21
 Operator : SY/MD
 Sample : N2320-05
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YB2P7

Manual IntegrationsAPPROVED

Quant Time: Apr 09 05:10:37 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Apr 09 04:40:11 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 04/11/2022
 Supervised By :Mahesh Dadoda 04/13/2022

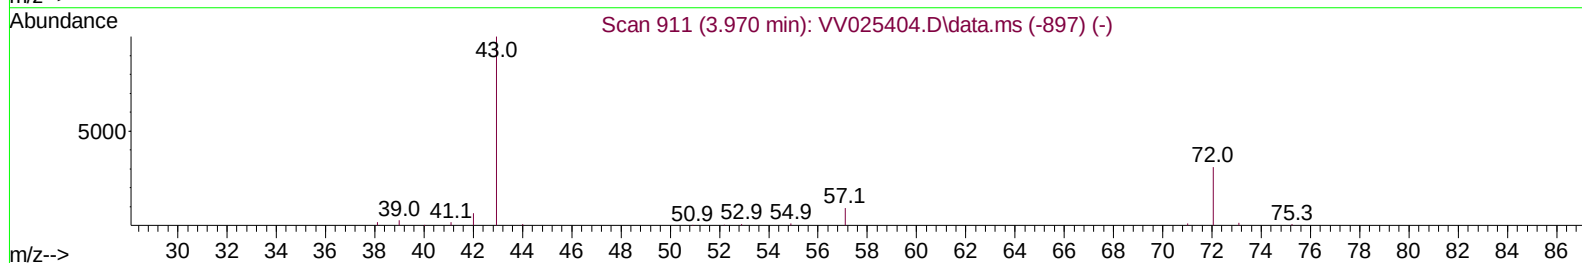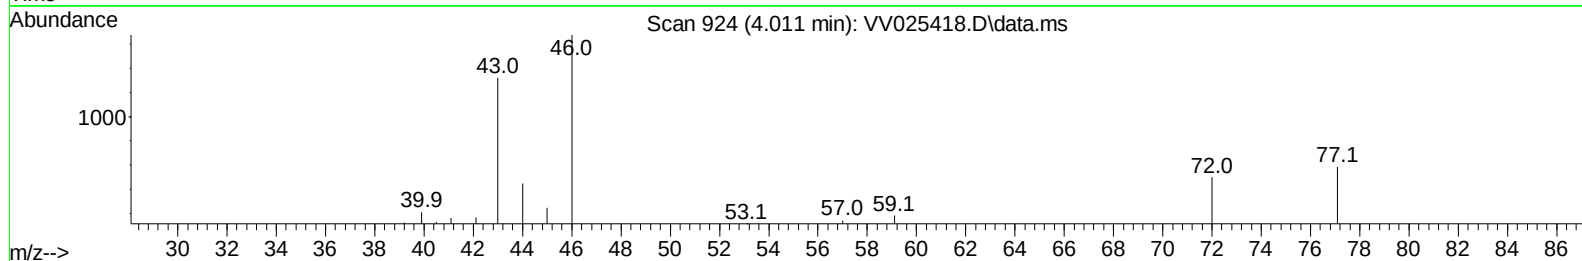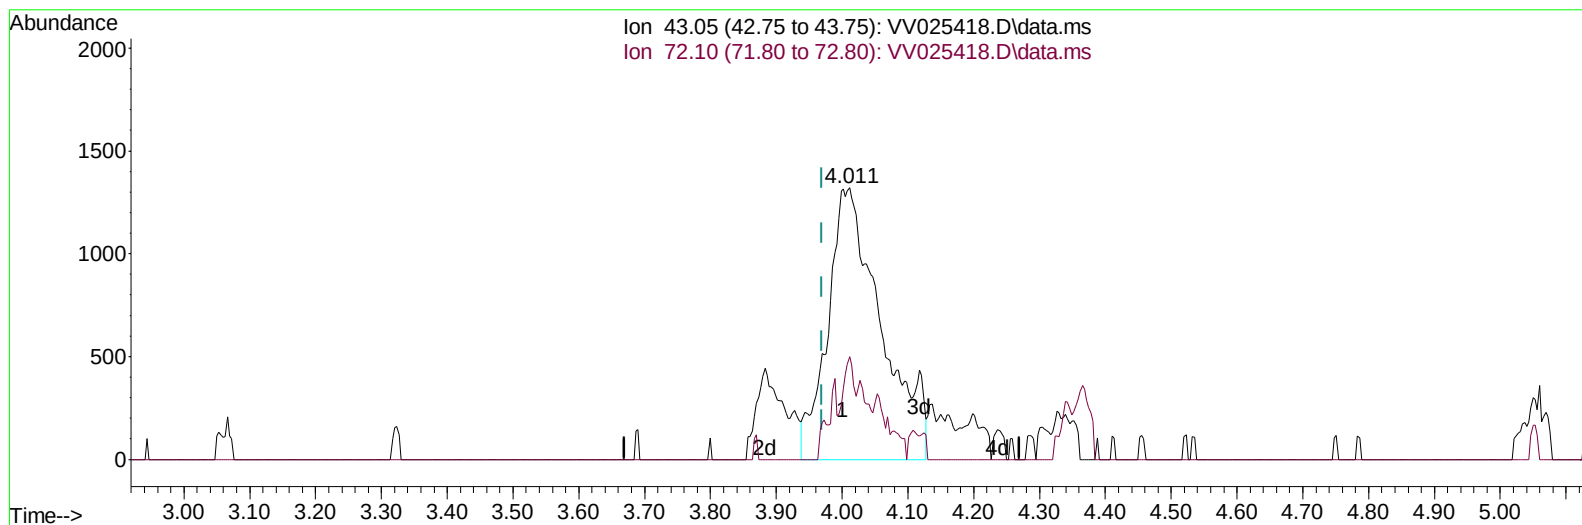

TIC: VV025418.D\data.ms

(21) 2-Butanone (T)

4.011min (+ 0.042) 3.98 ug/L m

response 7431

Ion	Exp%	Act%
43.05	100.00	100.00
72.10	30.40	6.89#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040822\
 Data File : VV025418.D
 Acq On : 08 Apr 2022 18:21
 Operator : SY/MD
 Sample : N2320-05
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YB2P7

Manual IntegrationsAPPROVED

Quant Time: Apr 09 05:10:37 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Apr 09 04:40:11 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 04/11/2022
 Supervised By :Mahesh Dadoda 04/13/2022

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.619	114		176037	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117		173767	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152		81360	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.307	65		77802	4.754	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	95.000%	
7) Chloroethane-d5	1.571	69		68552	3.937	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	78.800%	
11) 1,1-Dichloroethene-d2	2.111	63		113440	3.460	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	69.200%	
20) 2-Butanone-d5	3.896	46		101882	51.176	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	102.360%	
24) Chloroform-d	4.352	84		116864	4.725	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.600%	
26) 1,2-Dichloroethane-d4	5.034	65		54444	5.109	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	102.200%	
32) Benzene-d6	5.050	84		240410	4.782	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.600%	
36) 1,2-Dichloropropane-d6	6.069	67		69475	4.955	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	99.000%	
41) Toluene-d8	7.317	98		208385	4.466	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	89.400%	
43) trans-1,3-Dichloroprop...	7.622	79		21283	4.516	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	90.400%	
46) 2-Hexanone-d5	8.088	63		75728	45.783	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	91.560%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84		40055	4.522	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	90.400%	
66) 1,2-Dichlorobenzene-d4	11.622	152		71748	5.260	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	105.200%	
Target Compounds							
21) 2-Butanone	4.011	43		7431m	3.980	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040822\
Data File : VV025418.D
Acq On : 08 Apr 2022 18:21
Operator : SY/MD
Sample : N2320-05
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YB2P7

Manual IntegrationsAPPROVED

Quant Time: Apr 09 05:10:37 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Apr 09 04:40:11 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 04/11/2022
Supervised By :Mahesh Dadoda 04/13/2022

