




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040822\
 Data File : VV025424.D
 Acq On : 08 Apr 2022 21:04
 Operator : SY/MD
 Sample : N2319-04
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YB2H1

Manual IntegrationsAPPROVED

Quant Time: Apr 09 06:26:55 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Apr 09 06:16:16 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 04/11/2022
 Supervised By :Mahesh Dadoda 04/13/2022

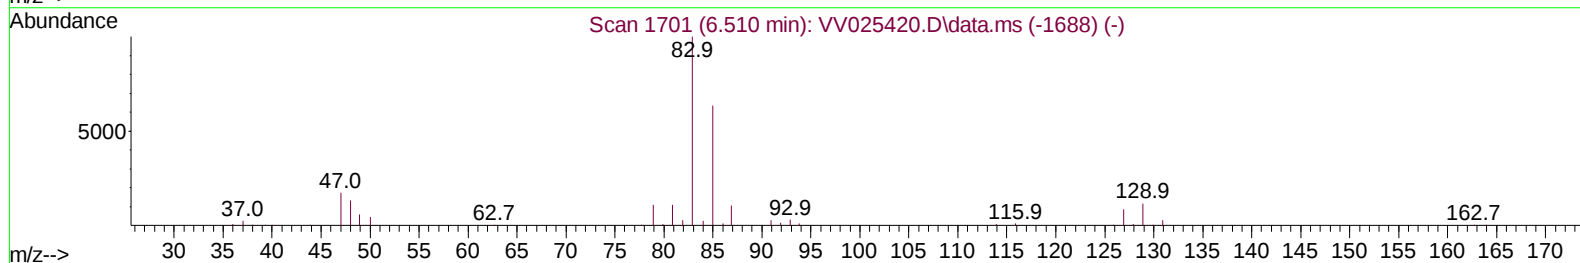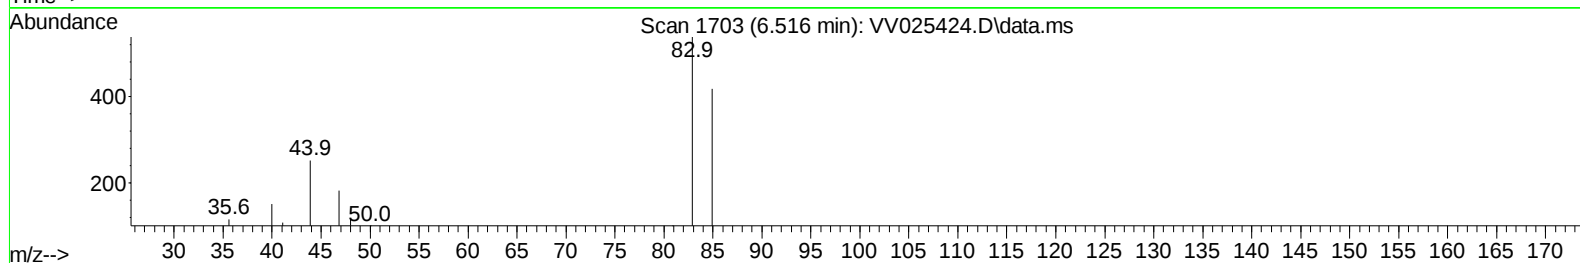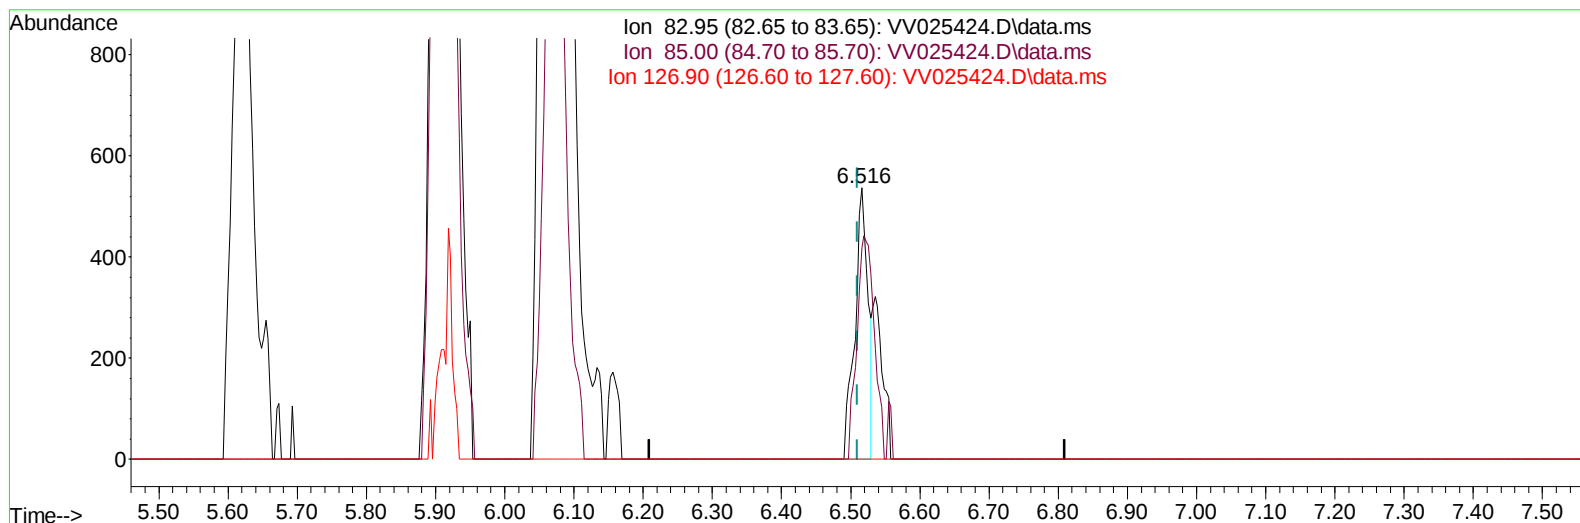

TIC: VV025424.D\data.ms

(38) Bromodichloromethane (T)

6.516min (+ 0.006) 0.07 ug/L

response 705

Ion	Exp%	Act%
82.95	100.00	100.00
85.00	63.40	77.84
126.90	9.00	0.00#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040822\
 Data File : VV025424.D
 Acq On : 08 Apr 2022 21:04
 Operator : SY/MD
 Sample : N2319-04
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YB2H1

Manual IntegrationsAPPROVED

Quant Time: Apr 09 06:26:55 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Apr 09 06:16:16 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 04/11/2022
 Supervised By :Mahesh Dadoda 04/13/2022

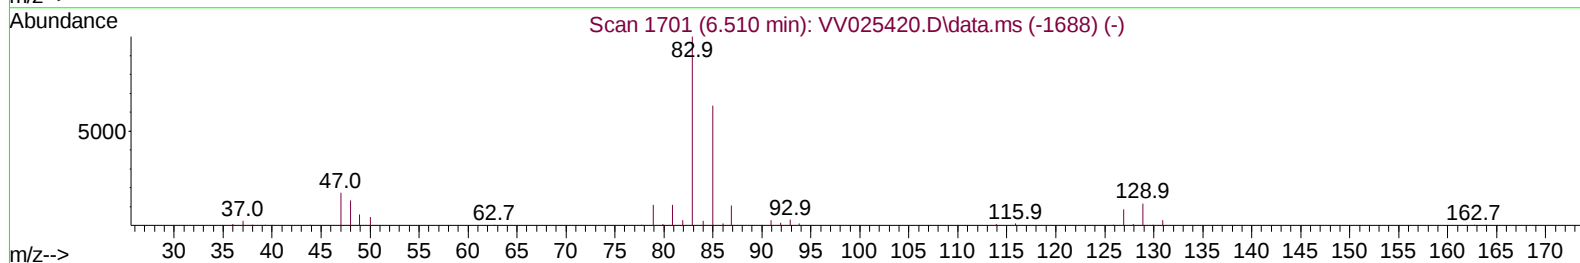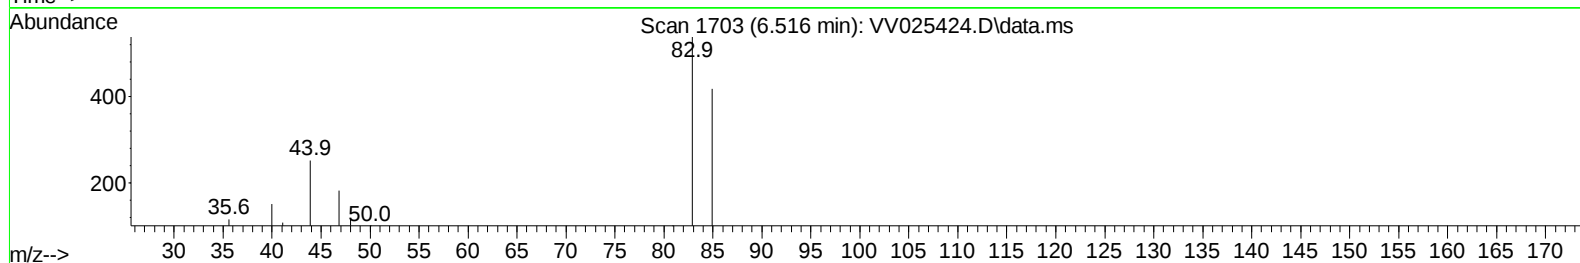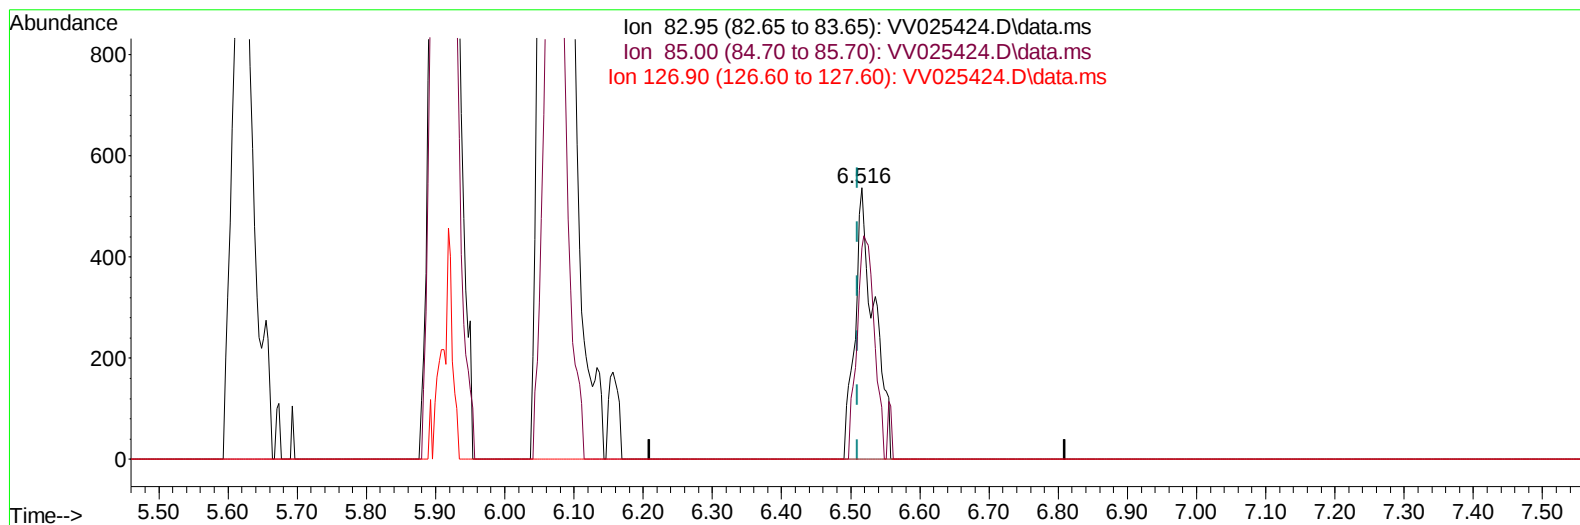

TIC: VV025424.D\data.ms

(38) Bromodichloromethane (T)

6.516min (+ 0.006) 0.10 ug/L m

response 1039

Ion	Exp%	Act%
82.95	100.00	100.00
85.00	63.40	77.84
126.90	9.00	0.00#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040822\
 Data File : VV025424.D
 Acq On : 08 Apr 2022 21:04
 Operator : SY/MD
 Sample : N2319-04
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YB2H1

Manual IntegrationsAPPROVED

Quant Time: Apr 09 06:26:55 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Apr 09 06:16:16 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 04/11/2022
 Supervised By :Mahesh Dadoda 04/13/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	127345	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	121365	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	55774	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	67095	5.667	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130	Recovery	=	113.400%	
7) Chloroethane-d5	1.568	69	60427	4.798	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130	Recovery	=	96.000%	
11) 1,1-Dichloroethene-d2	2.111	63	124430	5.246	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125	Recovery	=	105.000%	
20) 2-Butanone-d5	3.892	46	79910	55.488	ug/L	0.00
Spiked Amount 50.000	Range 40	- 130	Recovery	=	110.980%	
24) Chloroform-d	4.352	84	90333	5.049	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	101.000%	
26) 1,2-Dichloroethane-d4	5.034	65	42943	5.571	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	111.400%	
32) Benzene-d6	5.050	84	187980	5.353	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	107.000%	
36) 1,2-Dichloropropane-d6	6.069	67	53917	5.506	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140	Recovery	=	110.200%	
41) Toluene-d8	7.317	98	166123	5.098	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	102.000%	
43) trans-1,3-Dichloroprop...	7.625	79	15337	4.659	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130	Recovery	=	93.200%	
46) 2-Hexanone-d5	8.088	63	63287	54.781	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130	Recovery	=	109.560%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	33765	5.457	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120	Recovery	=	109.200%	
66) 1,2-Dichlorobenzene-d4	11.622	152	57291	6.127	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120	Recovery	=	122.600%#	
Target Compounds						
					Qvalue	
9) Trichlorofluoromethane	1.754	101	3455	0.174	ug/L	92
10) 1,1,2-Trichloro-1,2,2-...	2.114	101	4041	0.363	ug/L #	81
12) 1,1-Dichloroethene	2.121	96	41953	3.798	ug/L	97
18) trans-1,2-Dichloroethene	2.767	96	1064	0.115	ug/L	89
19) 1,1-Dichloroethane	3.201	63	5352	0.341	ug/L	98
22) cis-1,2-Dichloroethene	3.912	96	9796	1.005	ug/L	97
25) Chloroform	4.378	83	25319	1.530	ug/L	98
31) Carbon tetrachloride	4.831	117	11460	0.947	ug/L	98
34) Trichloroethene	5.912	95	669386	70.320	ug/L	99
38) Bromodichloromethane	6.516	83	1039m	0.101	ug/L	
47) Tetrachloroethene	7.976	164	90424	12.134	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

