

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040822\
 Data File : VV025409.D
 Acq On : 08 Apr 2022 14:44
 Operator : SY/MD
 Sample : VV0408WBL01
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK337

Quant Time: Apr 09 04:47:00 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Apr 09 04:40:11 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.612	114	212927	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	205351	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	106256	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	89626	4.527	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	90.600%
7) Chloroethane-d5	1.568	69	81283	3.860	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	77.200%
11) 1,1-Dichloroethene-d2	2.108	63	138383	3.490	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	69.800%
20) 2-Butanone-d5	3.892	46	111576	46.336	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	92.680%
24) Chloroform-d	4.346	84	134516	4.497	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.000%
26) 1,2-Dichloroethane-d4	5.030	65	60950	4.729	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.600%
32) Benzene-d6	5.047	84	278189	4.682	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.600%
36) 1,2-Dichloropropane-d6	6.066	67	79122	4.775	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	95.400%
41) Toluene-d8	7.313	98	254339	4.613	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.200%
43) trans-1,3-Dichloroprop...	7.622	79	24924	4.475	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	89.600%
46) 2-Hexanone-d5	8.085	63	89867	45.974	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	91.940%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	48187	4.603	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	92.000%
66) 1,2-Dichlorobenzene-d4	11.622	152	85334	4.790	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	95.800%
Target Compounds						Qvalue
16) Methylene chloride	2.510	84	6817	0.381	ug/L	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040822\
Data File : VV025409.D
Acq On : 08 Apr 2022 14:44
Operator : SY/MD
Sample : VV0408WBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK337


Quant Time: Apr 09 04:47:00 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Apr 09 04:40:11 2022
Response via : Initial Calibration

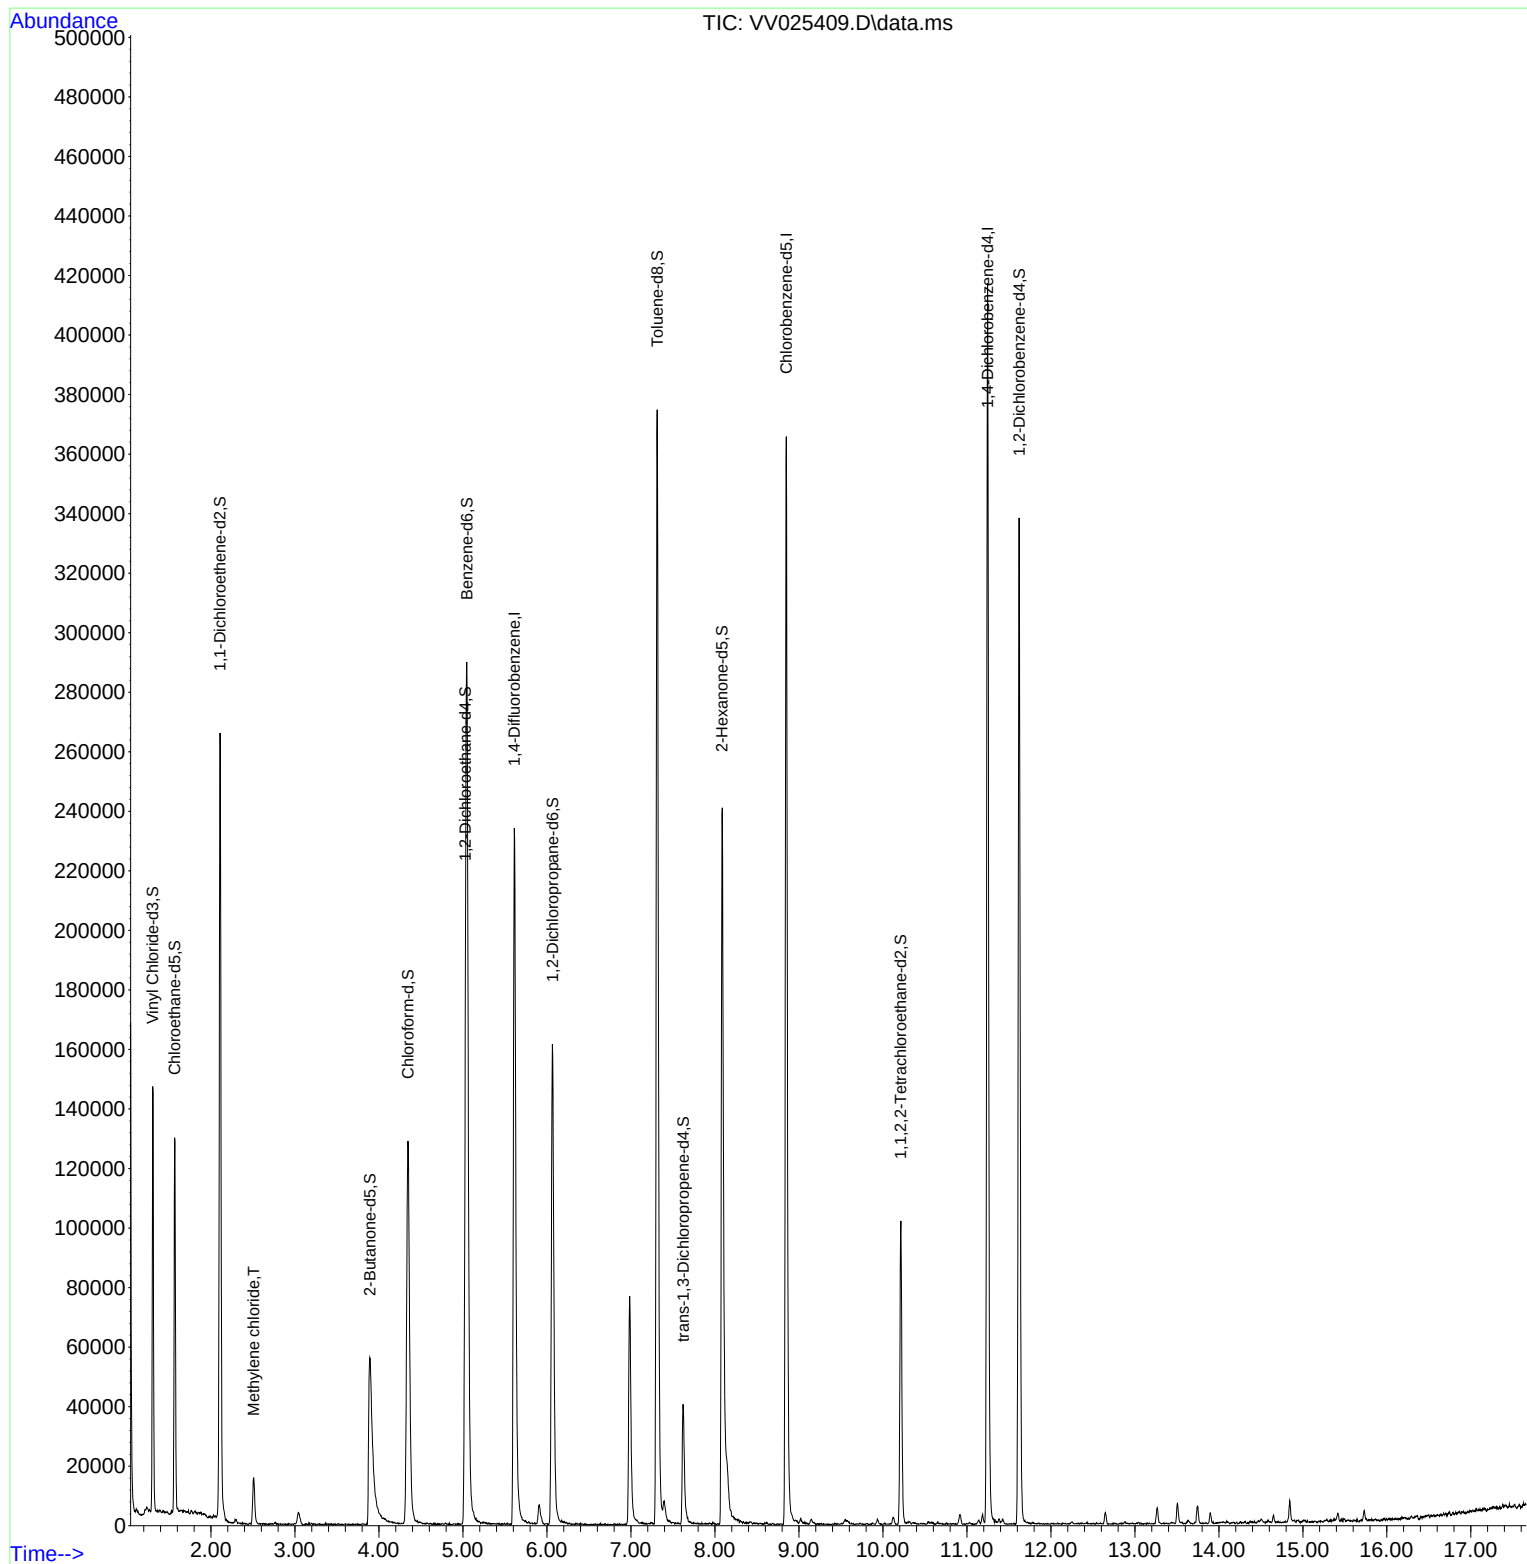

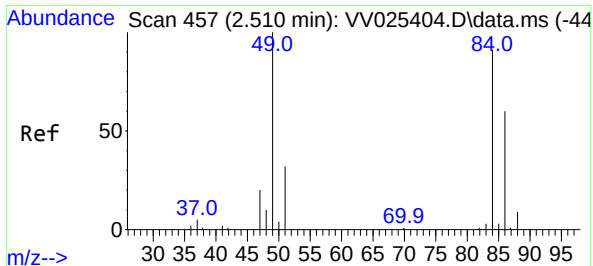

#16
Methylene chloride
Concen: 0.381 ug/L
RT: 2.510 min Scan# 4
Delta R.T. -0.000 min
Lab File: VV025409.D
Acq: 08 Apr 2022 14:44

Instrument :
MSVOA_V
ClientSampleId :
VBLK337

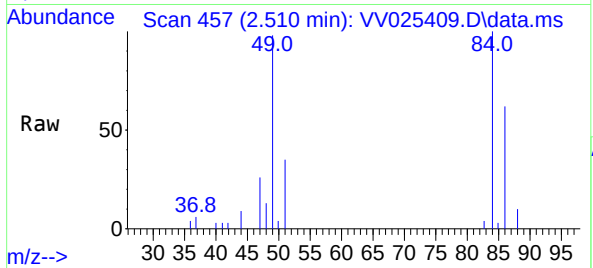

Tgt Ion: 84 Resp: 6817

Ion	Ratio	Lower	Upper
84	100		
86	62.1	45.9	85.3
49	97.6	76.6	142.3

