

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040822\
 Data File : VV025421.D
 Acq On : 08 Apr 2022 19:54
 Operator : SY/MD
 Sample : VV0408WBL02
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK338

Quant Time: Apr 09 06:16:55 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Apr 09 06:16:16 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	155853	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	152494	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	72297	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	71776	4.954	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	99.000%	
7) Chloroethane-d5	1.571	69	65997	4.281	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	85.600%	
11) 1,1-Dichloroethene-d2	2.111	63	109712	3.780	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	75.600%	
20) 2-Butanone-d5	3.892	46	91703	52.029	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	104.060%	
24) Chloroform-d	4.352	84	105943	4.839	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	96.800%	
26) 1,2-Dichloroethane-d4	5.034	65	50154	5.316	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	106.400%	
32) Benzene-d6	5.050	84	219870	4.983	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	99.600%	
36) 1,2-Dichloropropane-d6	6.069	67	62404	5.071	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	101.400%	
41) Toluene-d8	7.317	98	192773	4.708	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	94.200%	
43) trans-1,3-Dichloroprop...	7.625	79	18241	4.410	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	88.200%	
46) 2-Hexanone-d5	8.088	63	68682	47.315	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	94.640%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	38579	4.963	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	99.200%	
66) 1,2-Dichlorobenzene-d4	11.622	152	65292	5.387	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	107.800%	
Target Compounds						
					Qvalue	
16) Methylene chloride	2.510	84	2953	0.225	ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040822\
Data File : VV025421.D
Acq On : 08 Apr 2022 19:54
Operator : SY/MD
Sample : VV0408WBL02
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK338


Quant Time: Apr 09 06:16:55 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Apr 09 06:16:16 2022
Response via : Initial Calibration

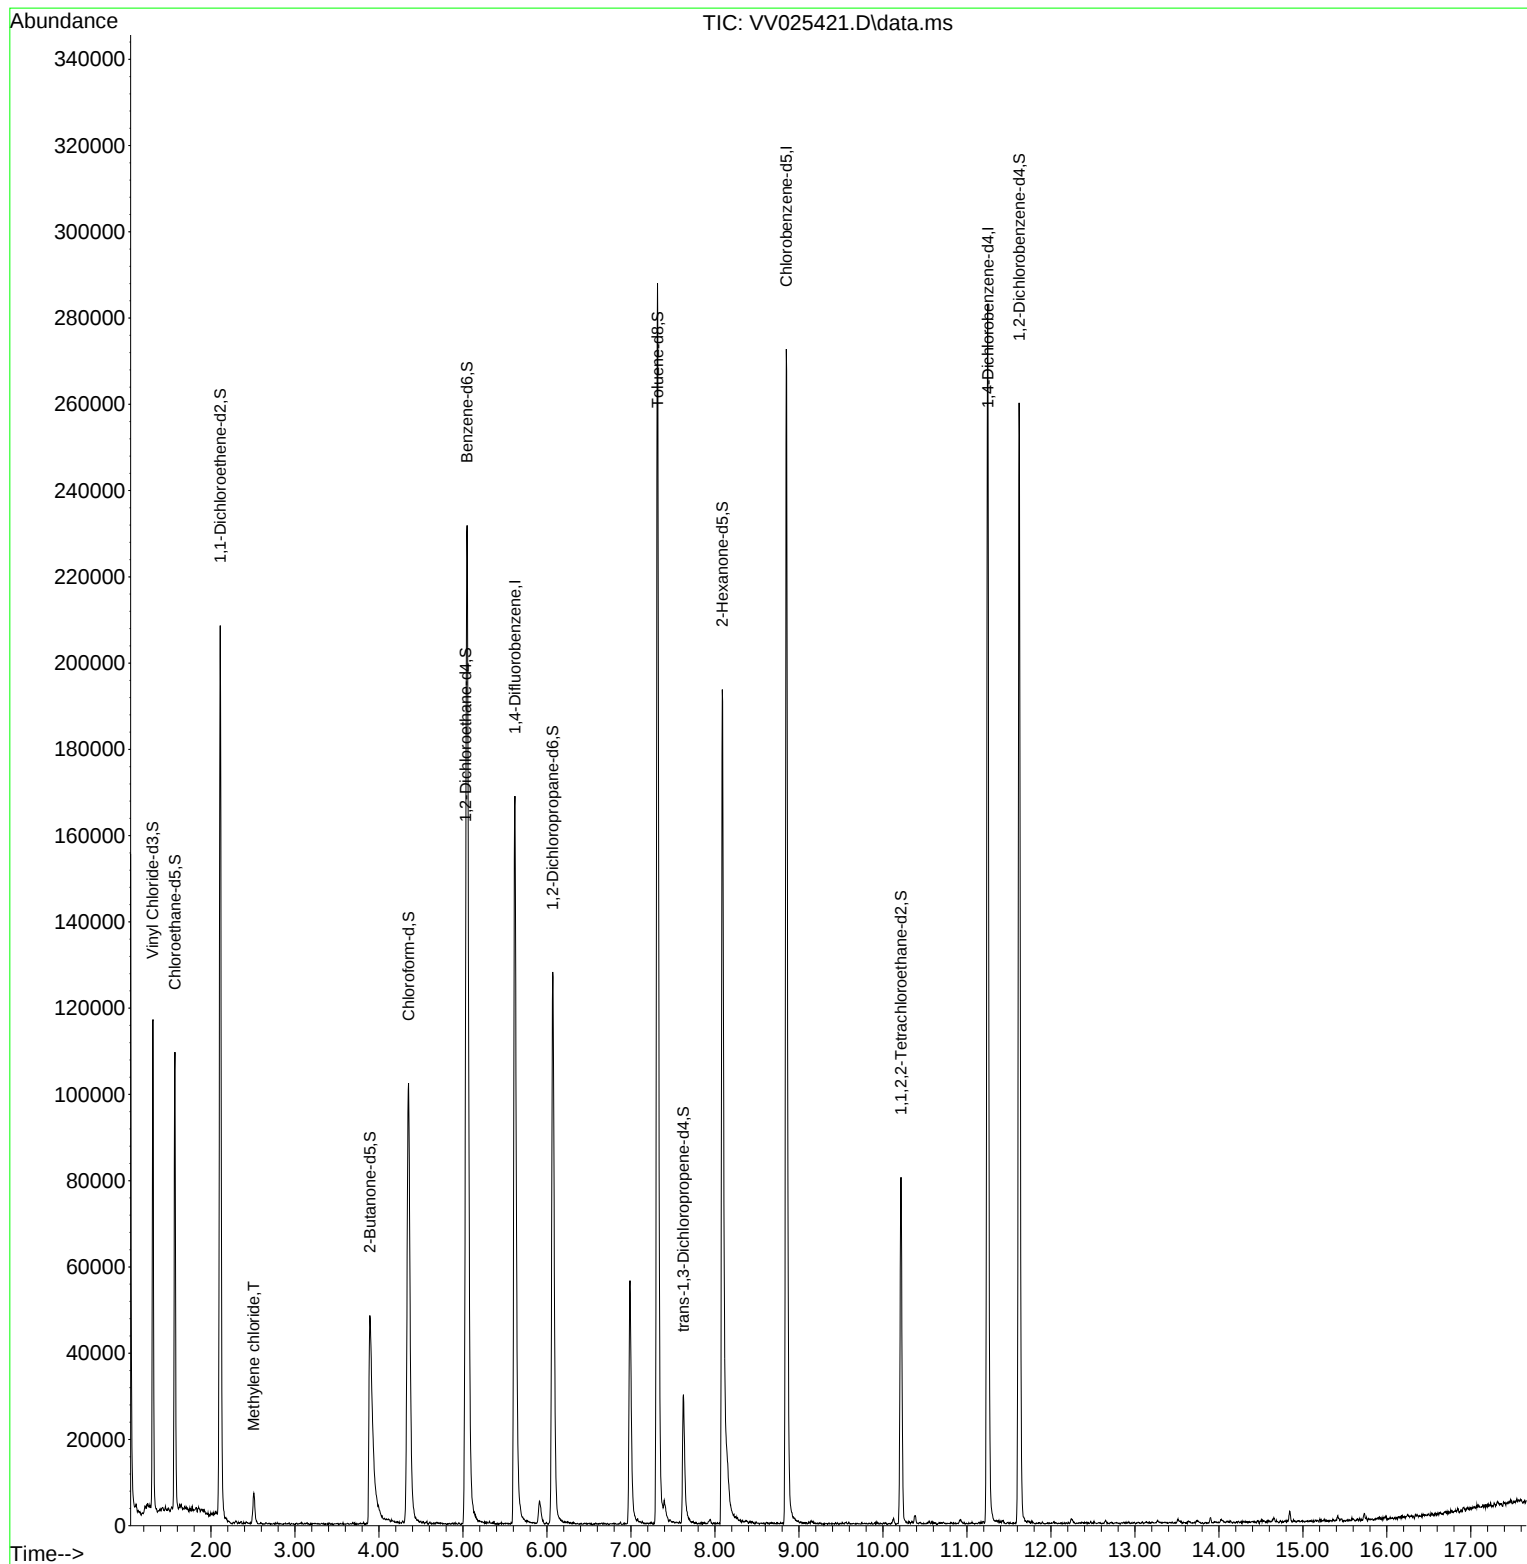

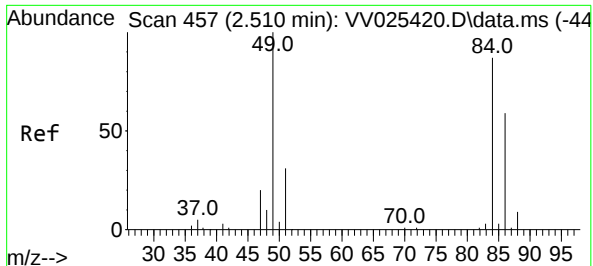

#16
Methylene chloride
Concen: 0.225 ug/L
RT: 2.510 min Scan# 41
Delta R.T. -0.000 min
Lab File: VV025421.D
Acq: 08 Apr 2022 19:54

Instrument :
MSVOA_V
ClientSampleId :
VBLK338

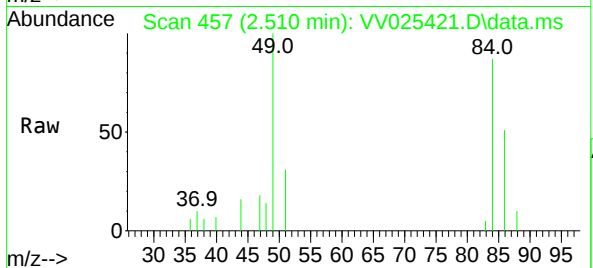

Tgt Ion: 84 Resp: 2953

Ion	Ratio	Lower	Upper
84	100		
86	58.3	45.9	85.3
49	114.7	76.6	142.3

