

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040822\
 Data File : VV025407.D
 Acq On : 08 Apr 2022 13:33
 Operator : SY/MD
 Sample : VIBLK243
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK243

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV025407.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	95	rBV	149878	152287	20.15%	2.304%
2	1.568	156	164	181	rVB	145766	166541	22.04%	2.520%
3	2.108	321	332	351	rVB	276499	403512	53.40%	6.106%
4	2.507	446	456	468	rBV2	20762	34689	4.59%	0.525%
5	3.044	612	623	634	rBV5	4151	8906	1.18%	0.135%
6	3.880	874	883	918	rBV	68163	196688	26.03%	2.976%
7	4.346	1011	1028	1050	rBV	131628	327173	43.30%	4.951%
8	5.044	1229	1245	1280	rBV2	300822	755655	100.00%	11.434%
9	5.613	1409	1422	1455	rBV	249833	513428	67.94%	7.769%
10	5.912	1505	1515	1532	rVB7	7664	17431	2.31%	0.264%
11	6.066	1550	1563	1591	rBV	167934	349706	46.28%	5.292%
12	6.986	1835	1849	1875	rBV	77361	149129	19.74%	2.257%
13	7.314	1939	1951	1970	rBV	382608	684885	90.63%	10.364%
14	7.397	1971	1977	1992	rVB3	9280	18239	2.41%	0.276%
15	7.622	2037	2047	2069	rBV	43509	80795	10.69%	1.223%
16	8.085	2180	2191	2228	rBV	254460	506206	66.99%	7.660%
17	8.850	2417	2429	2456	rBV	387149	654772	86.65%	9.908%
18	9.934	2756	2766	2778	rBV2	5494	8804	1.17%	0.133%
19	10.214	2839	2853	2870	rBV	99460	162715	21.53%	2.462%
20	10.918	3062	3072	3083	rVB4	6569	9681	1.28%	0.146%
21	11.185	3148	3155	3164	rBV4	8403	12417	1.64%	0.188%
22	11.246	3164	3174	3194	rVV	428865	678235	89.75%	10.263%
23	11.622	3279	3291	3311	rBV	353159	573363	75.88%	8.676%
24	12.648	3600	3610	3622	rBV4	15352	23335	3.09%	0.353%
25	13.262	3789	3801	3812	rBV	22056	33508	4.43%	0.507%
26	13.503	3866	3876	3893	rBV	23979	38303	5.07%	0.580%
27	13.744	3938	3951	3965	rBV2	24750	39178	5.18%	0.593%
28	14.844	4285	4293	4300	rBV6	6658	9036	1.20%	0.137%




Sum of corrected areas: 6608617

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040822\
Data File : VV025407.D
Acq On : 08 Apr 2022 13:33
Operator : SY/MD
Sample : VIBLK243
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK243

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

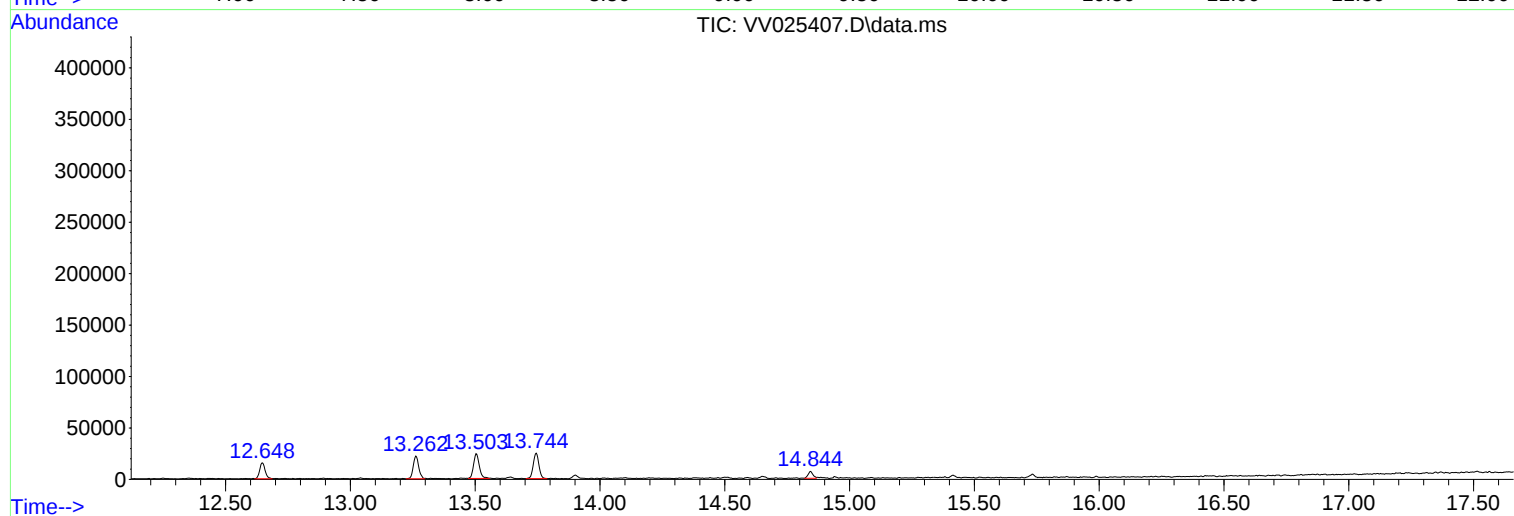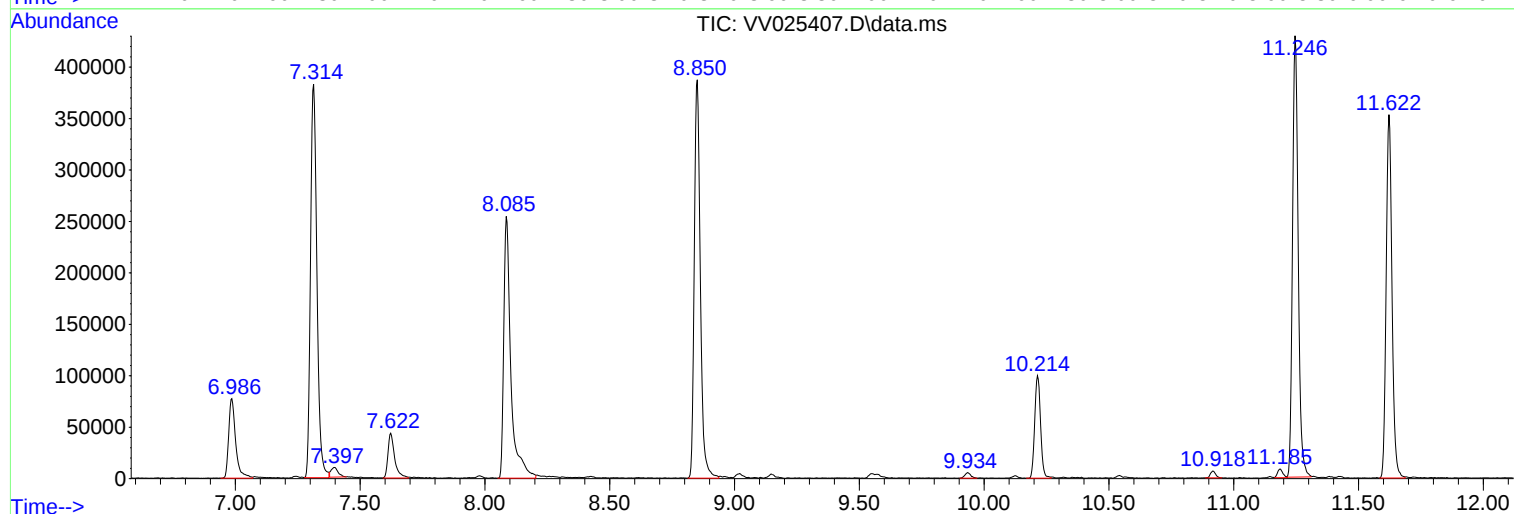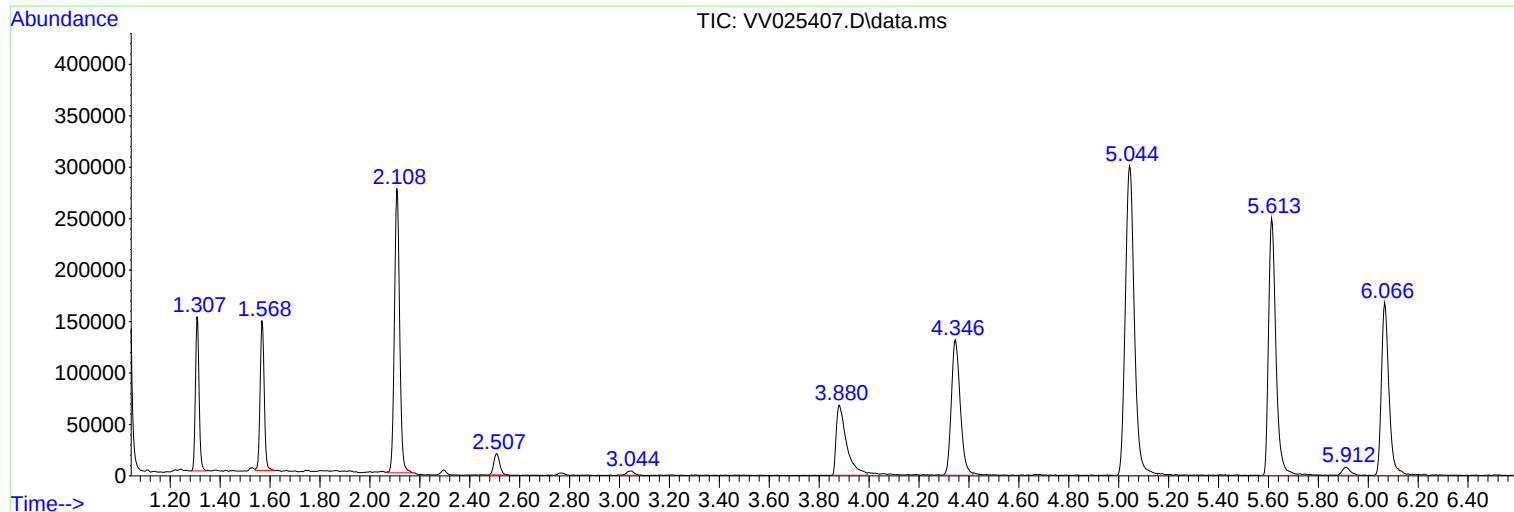

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040822\
Data File : VV025407.D
Acq On : 08 Apr 2022 13:33
Operator : SY/MD
Sample : VIBLK243
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK243

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040822\
Data File : VV025407.D
Acq On : 08 Apr 2022 13:33
Operator : SY/MD
Sample : VIBLK243
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK243

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
