

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040822\
 Data File : VV025414.D
 Acq On : 08 Apr 2022 16:47
 Operator : SY/MD
 Sample : N2291-02DL 10X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B29DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV025414.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.311	76	84	96	rVB	155466	157323	19.06%	2.119%
2	1.571	157	165	179	rBV	139169	157523	19.08%	2.121%
3	1.757	214	223	233	rVB	75162	99040	12.00%	1.334%
4	2.111	321	333	357	rVB	280611	410964	49.79%	5.535%
5	2.510	447	457	471	rVB2	6402	11058	1.34%	0.149%
6	3.899	878	889	927	rBV2	65816	239593	29.03%	3.227%
7	4.352	1013	1030	1058	rBV	142891	363565	44.05%	4.896%
8	5.050	1230	1247	1275	rBV2	332387	825408	100.00%	11.116%
9	5.616	1411	1423	1446	rBV	260762	528777	64.06%	7.121%
10	5.915	1504	1516	1534	rVB10	9340	23321	2.83%	0.314%
11	6.069	1550	1564	1594	rBV	185637	386318	46.80%	5.203%
12	6.989	1839	1850	1868	rBV	85347	157981	19.14%	2.128%
13	7.317	1940	1952	1971	rBV	410564	721448	87.41%	9.716%
14	7.404	1973	1979	1991	rVB2	6075	11756	1.42%	0.158%
15	7.622	2038	2047	2072	rBV2	45341	85868	10.40%	1.156%
16	7.976	2143	2157	2177	rBV	301968	512002	62.03%	6.895%
17	8.088	2182	2192	2231	rBV	298756	585821	70.97%	7.890%
18	8.850	2418	2429	2448	rBV	414748	673921	81.65%	9.076%
19	10.214	2837	2853	2875	rBV	118993	188934	22.89%	2.544%
20	11.246	3164	3174	3195	rBV	452562	696141	84.34%	9.375%
21	11.622	3279	3291	3311	rBV	376858	588489	71.30%	7.926%




Sum of corrected areas: 7425251

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040822\
Data File : VV025414.D
Acq On : 08 Apr 2022 16:47
Operator : SY/MD
Sample : N2291-02DL 10X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B29DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

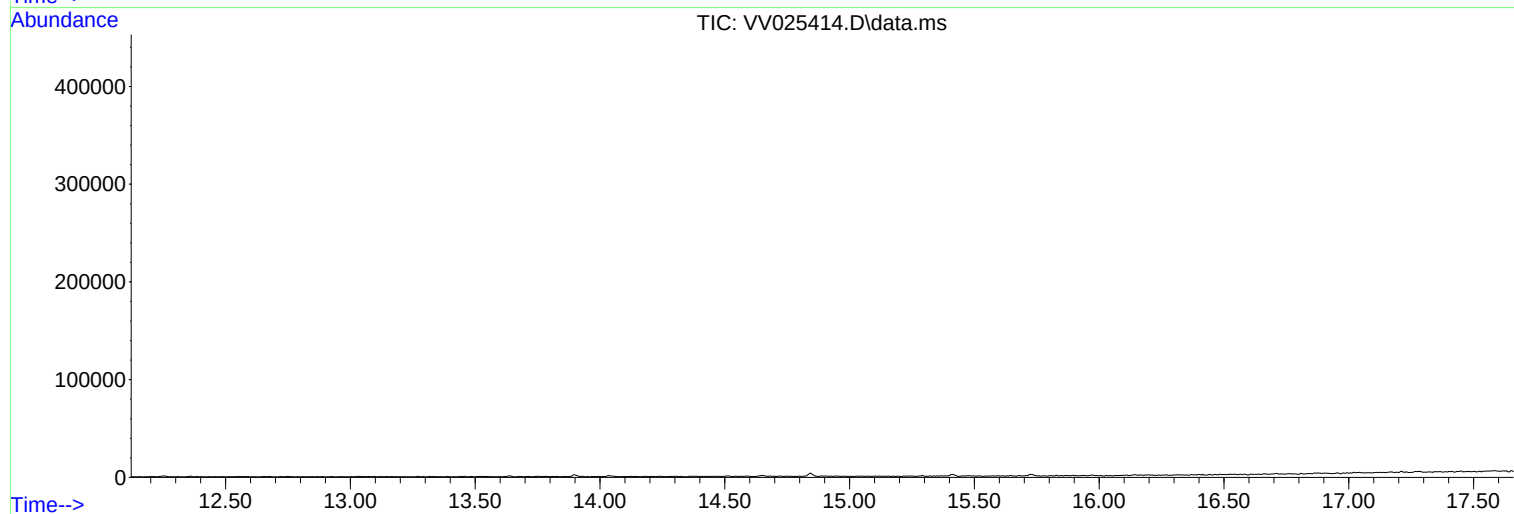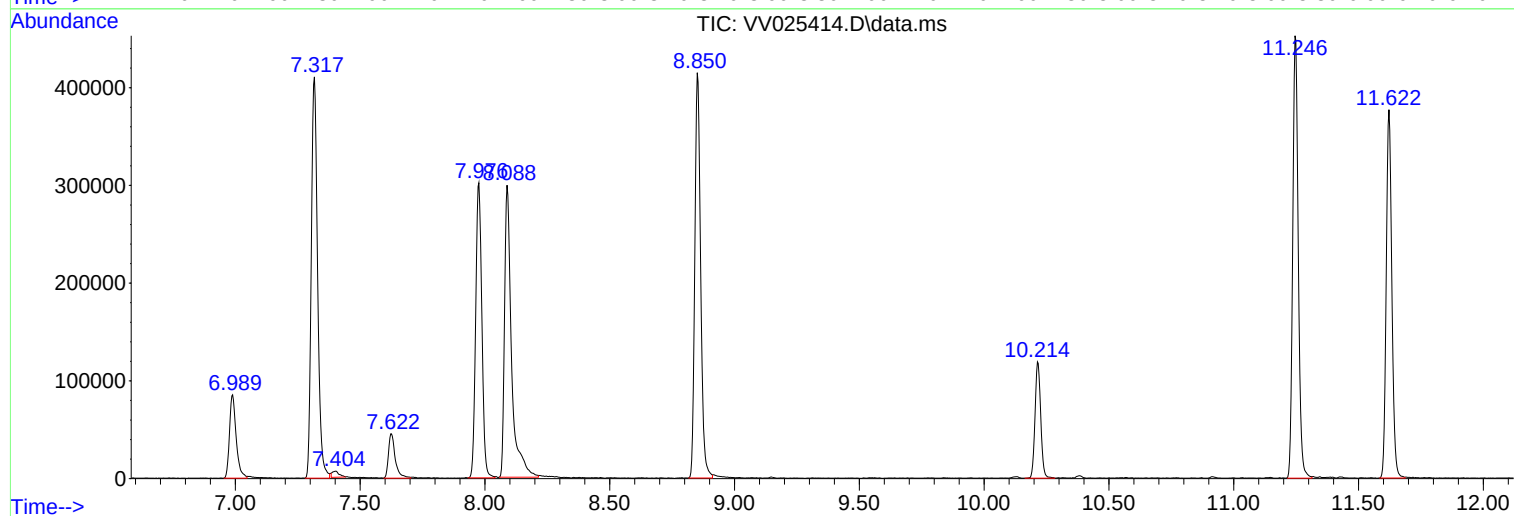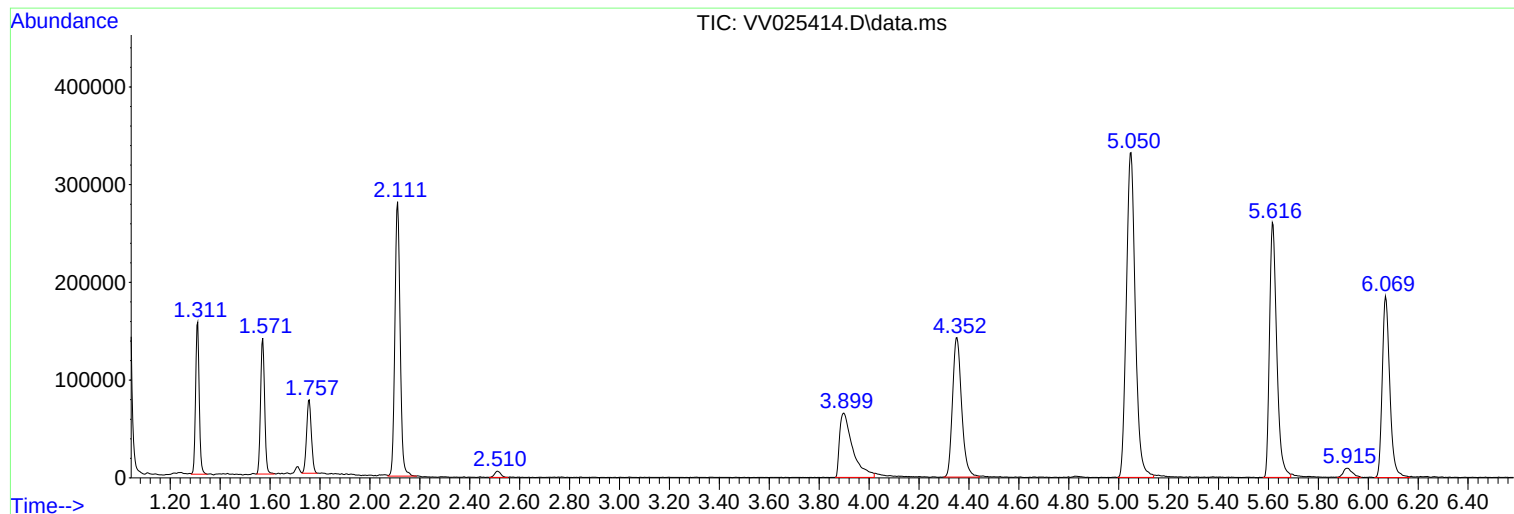

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040822\
Data File : VV025414.D
Acq On : 08 Apr 2022 16:47
Operator : SY/MD
Sample : N2291-02DL 10X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B29DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040822\
Data File : VV025414.D
Acq On : 08 Apr 2022 16:47
Operator : SY/MD
Sample : N2291-02DL 10X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B29DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
