

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040822\
 Data File : VV025417.D
 Acq On : 08 Apr 2022 17:57
 Operator : SY/MD
 Sample : N2320-04
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YB2P6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV025417.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.217	50	55	60	rBV	7553	7230	1.27%	0.161%
2	1.307	75	83	93	rBV	111421	115188	20.16%	2.565%
3	1.571	157	165	178	rBV	99930	114637	20.07%	2.553%
4	2.111	322	333	350	rBV	200750	292921	51.27%	6.523%
5	2.298	382	391	399	rBV	3707	6148	1.08%	0.137%
6	3.899	877	889	917	rBV2	44299	154328	27.01%	3.437%
7	4.352	1013	1030	1054	rBV	99999	250370	43.82%	5.576%
8	5.050	1230	1247	1276	rBV2	227891	571304	100.00%	12.723%
9	5.619	1413	1424	1447	rBV	142552	293307	51.34%	6.532%
10	5.915	1506	1516	1529	rBV8	5981	12957	2.27%	0.289%
11	6.069	1548	1564	1587	rBV	126568	265291	46.44%	5.908%
12	6.989	1838	1850	1871	rBV	55884	106404	18.62%	2.370%
13	7.317	1941	1952	1970	rBV	279610	491250	85.99%	10.940%
14	7.397	1972	1977	1993	rVB2	8337	15274	2.67%	0.340%
15	7.625	2037	2048	2066	rBV2	29651	57039	9.98%	1.270%
16	7.940	2135	2146	2161	rVB3	4553	8197	1.43%	0.183%
17	8.088	2182	2192	2235	rBV	184405	391974	68.61%	8.729%
18	8.850	2418	2429	2457	rBV	225491	377605	66.10%	8.409%
19	9.146	2511	2521	2530	rBV5	4560	7752	1.36%	0.173%
20	9.548	2637	2646	2659	rBV2	5424	9768	1.71%	0.218%
21	10.214	2842	2853	2867	rBV	78065	123593	21.63%	2.752%
22	10.381	2893	2905	2915	rBV	10765	17687	3.10%	0.394%
23	11.246	3162	3174	3201	rBV	223809	353878	61.94%	7.881%
24	11.532	3253	3263	3276	rBV4	8976	17975	3.15%	0.400%
25	11.622	3280	3291	3309	rVB	255812	403707	70.66%	8.990%
26	12.249	3477	3486	3496	rBV3	4029	6182	1.08%	0.138%
27	12.342	3507	3515	3534	rBV6	10599	18533	3.24%	0.413%




Sum of corrected areas: 4490499

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040822\
Data File : VV025417.D
Acq On : 08 Apr 2022 17:57
Operator : SY/MD
Sample : N2320-04
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YB2P6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

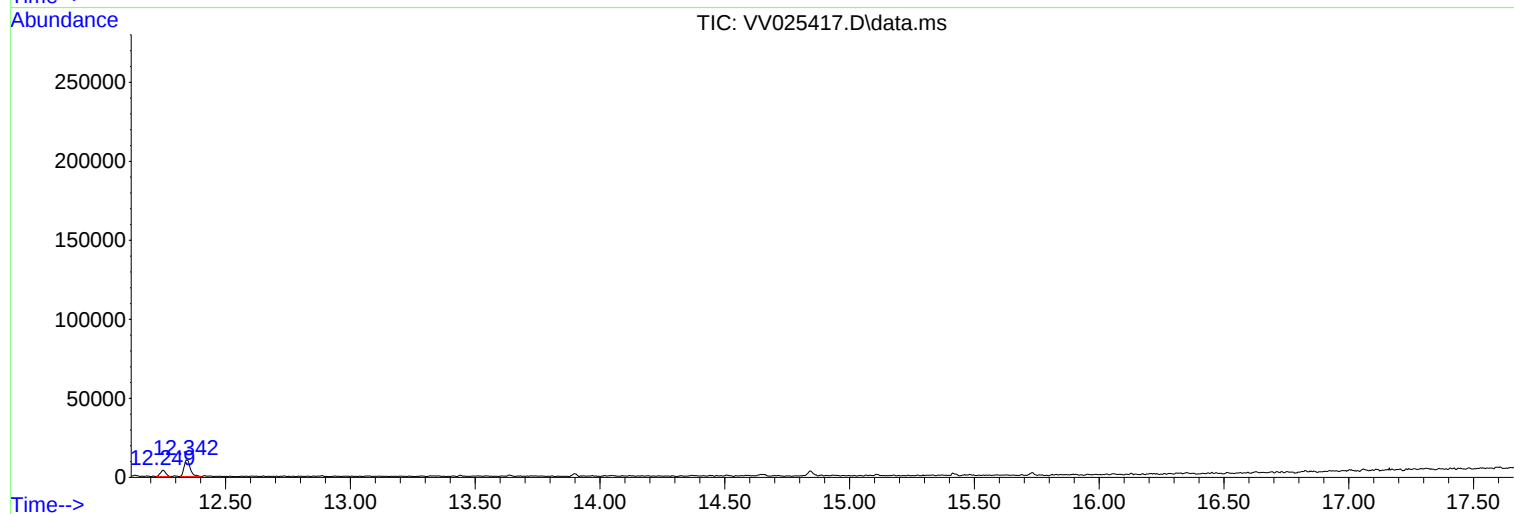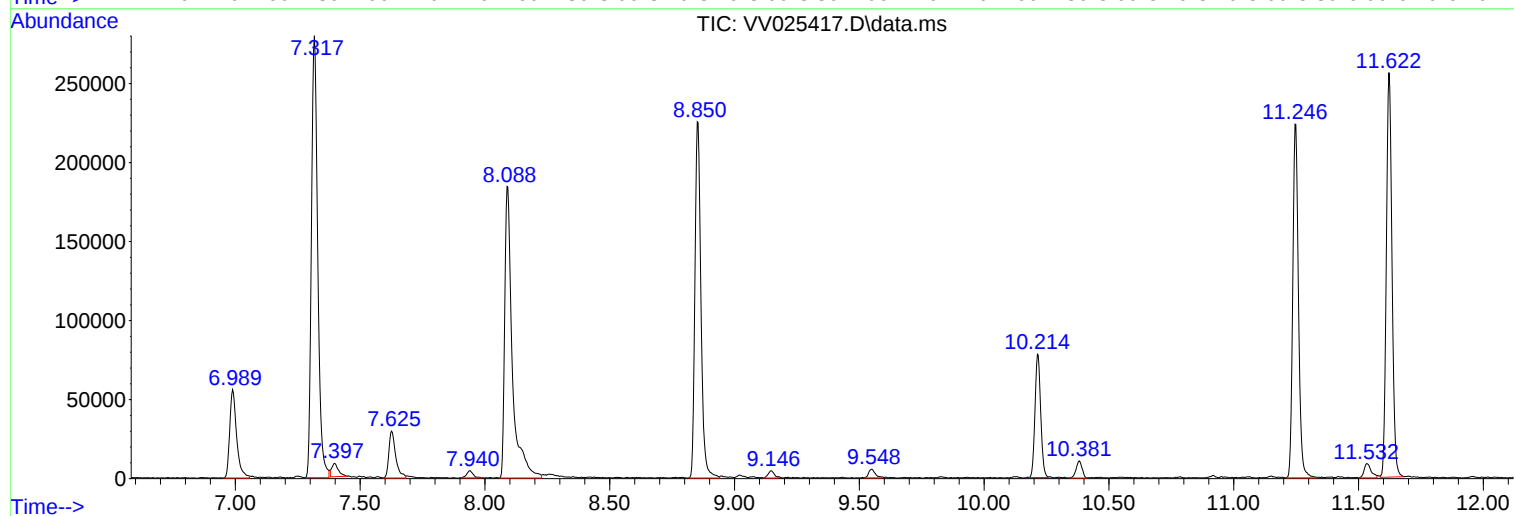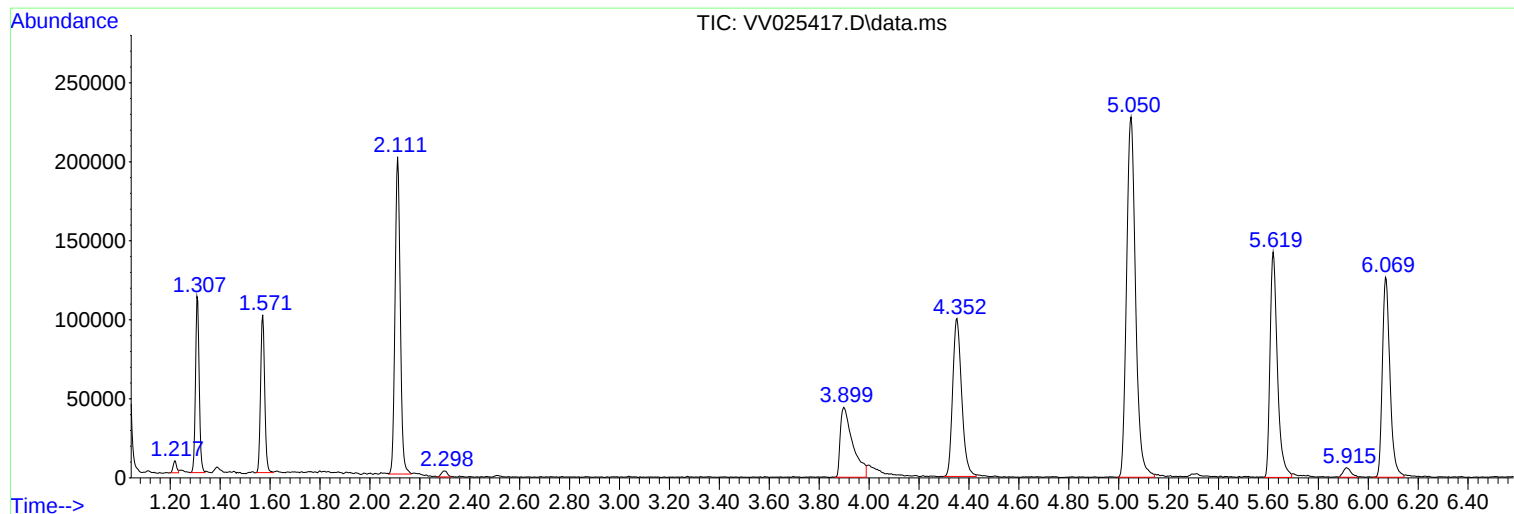

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040822\
Data File : VV025417.D
Acq On : 08 Apr 2022 17:57
Operator : SY/MD
Sample : N2320-04
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YB2P6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040822\
Data File : VV025417.D
Acq On : 08 Apr 2022 17:57
Operator : SY/MD
Sample : N2320-04
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YB2P6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc