

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040822\
 Data File : VV025421.D
 Acq On : 08 Apr 2022 19:54
 Operator : SY/MD
 Sample : VV0408WBL02
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK338

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV025421.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.311	76	84	96	rVB	113532	116069	20.13%	2.488%
2	1.571	157	165	178	rVB	105950	119564	20.74%	2.563%
3	2.111	322	333	350	rVB	206972	302918	52.54%	6.494%
4	2.510	446	457	467	rBV4	7093	12162	2.11%	0.261%
5	3.892	877	887	917	rBV	48323	150366	26.08%	3.223%
6	4.352	1013	1030	1056	rBV	101985	257208	44.61%	5.514%
7	5.050	1231	1247	1277	rBV2	231508	576538	100.00%	12.359%
8	5.619	1413	1424	1452	rBV	168584	350137	60.73%	7.506%
9	5.912	1503	1515	1535	rVB6	5364	12232	2.12%	0.262%
10	6.069	1548	1564	1588	rBV	128043	267404	46.38%	5.732%
11	6.989	1840	1850	1867	rBV	56308	105181	18.24%	2.255%
12	7.317	1939	1952	1973	rBV	287654	504958	87.58%	10.825%
13	7.397	1973	1977	1992	rVB4	4914	9275	1.61%	0.199%
14	7.625	2038	2048	2067	rBV2	29823	56449	9.79%	1.210%
15	8.088	2183	2192	2233	rBV	193457	392479	68.08%	8.414%
16	8.850	2419	2429	2454	rBV	272339	448009	77.71%	9.604%
17	10.217	2843	2854	2873	rBV	80312	128317	22.26%	2.751%
18	11.249	3164	3175	3198	rBV	282489	444052	77.02%	9.519%
19	11.622	3279	3291	3308	rBV	259836	411463	71.37%	8.821%




Sum of corrected areas: 4664781

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040822\
Data File : VV025421.D
Acq On : 08 Apr 2022 19:54
Operator : SY/MD
Sample : VV0408WBL02
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK338

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

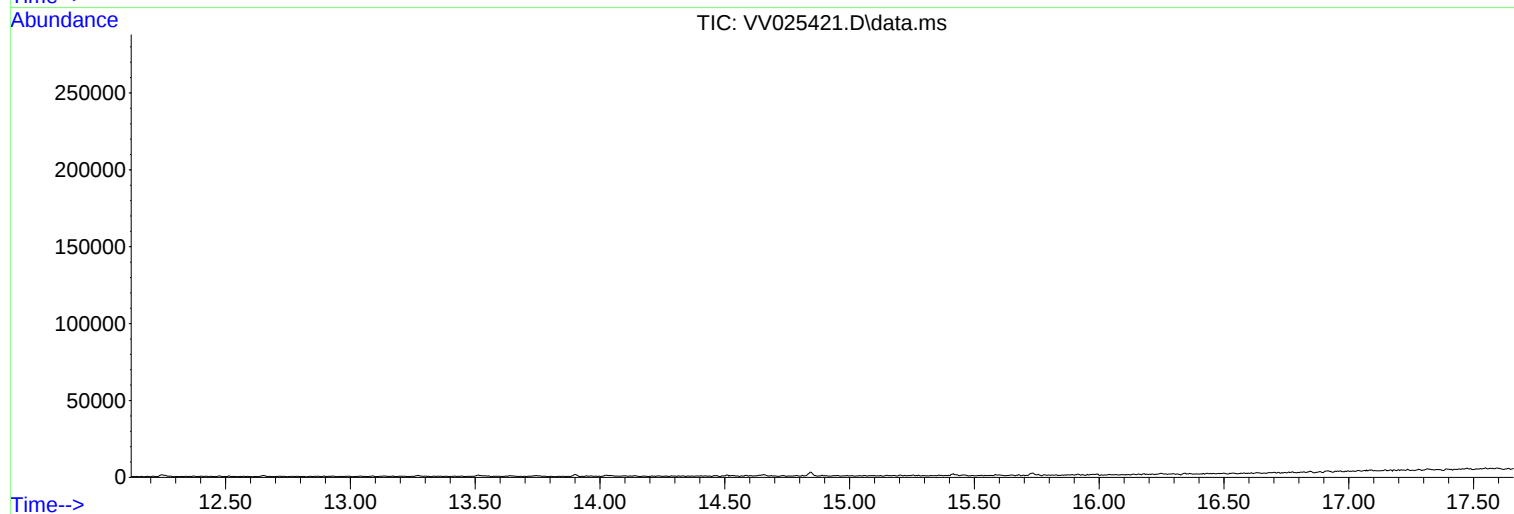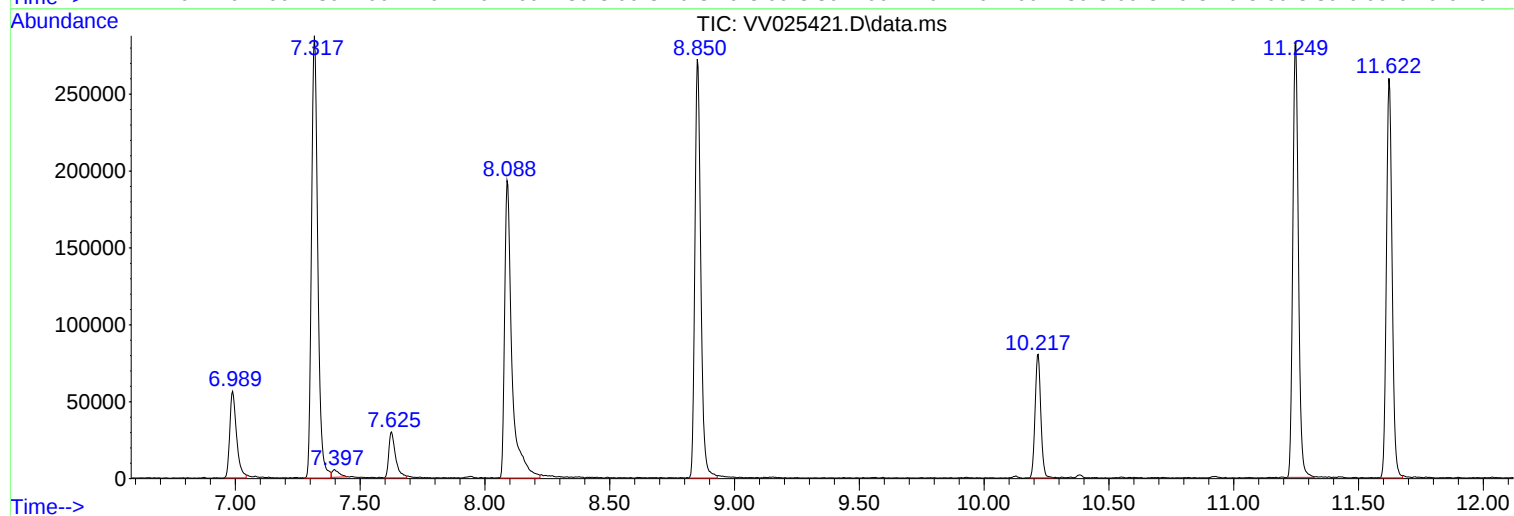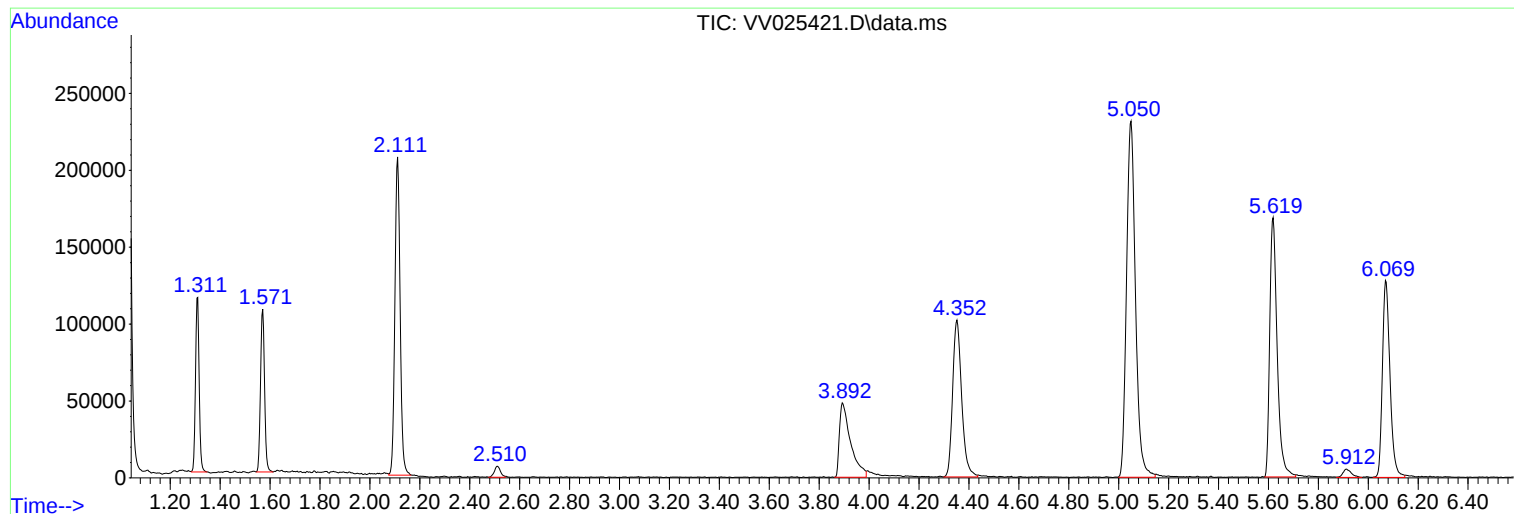

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040822\
Data File : VV025421.D
Acq On : 08 Apr 2022 19:54
Operator : SY/MD
Sample : VV0408WBL02
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK338

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040822\
Data File : VV025421.D
Acq On : 08 Apr 2022 19:54
Operator : SY/MD
Sample : VV0408WBL02
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK338

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc