

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040822\
 Data File : VV025422.D
 Acq On : 08 Apr 2022 20:17
 Operator : SY/MD
 Sample : N2319-02
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YB2G9

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV025422.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	96	rVB	105989	110207	2.76%	1.260%
2	1.571	157	165	180	rBV	96785	110640	2.77%	1.265%
3	2.114	322	334	355	rVB2	254885	426794	10.69%	4.880%
4	3.912	878	893	926	rBV2	76441	250941	6.29%	2.869%
5	4.355	1013	1031	1059	rBV2	89318	252667	6.33%	2.889%
6	5.050	1231	1247	1268	rBV3	197582	490139	12.28%	5.604%
7	5.619	1413	1424	1451	rBV	142608	294405	7.37%	3.366%
8	5.911	1501	1515	1538	rBV	2074294	3992475	100.00%	45.649%
9	6.072	1553	1565	1588	rVB	109042	227427	5.70%	2.600%
10	6.989	1841	1850	1877	rBV	44946	84981	2.13%	0.972%
11	7.317	1940	1952	1972	rBV	250469	436568	10.93%	4.992%
12	7.625	2041	2048	2069	rBV	24012	42689	1.07%	0.488%
13	7.976	2144	2157	2179	rBV	264105	438731	10.99%	5.016%
14	8.088	2183	2192	2224	rBV	161029	321187	8.04%	3.672%
15	8.853	2419	2430	2457	rBV	219373	367021	9.19%	4.196%
16	10.217	2843	2854	2869	rBV	69244	109184	2.73%	1.248%
17	11.249	3162	3175	3194	rBV	219881	346267	8.67%	3.959%
18	11.622	3278	3291	3311	rBV	218193	349149	8.75%	3.992%
19	12.342	3506	3515	3531	rBV2	60971	94609	2.37%	1.082%




Sum of corrected areas: 8746081

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040822\
Data File : VV025422.D
Acq On : 08 Apr 2022 20:17
Operator : SY/MD
Sample : N2319-02
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YB2G9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

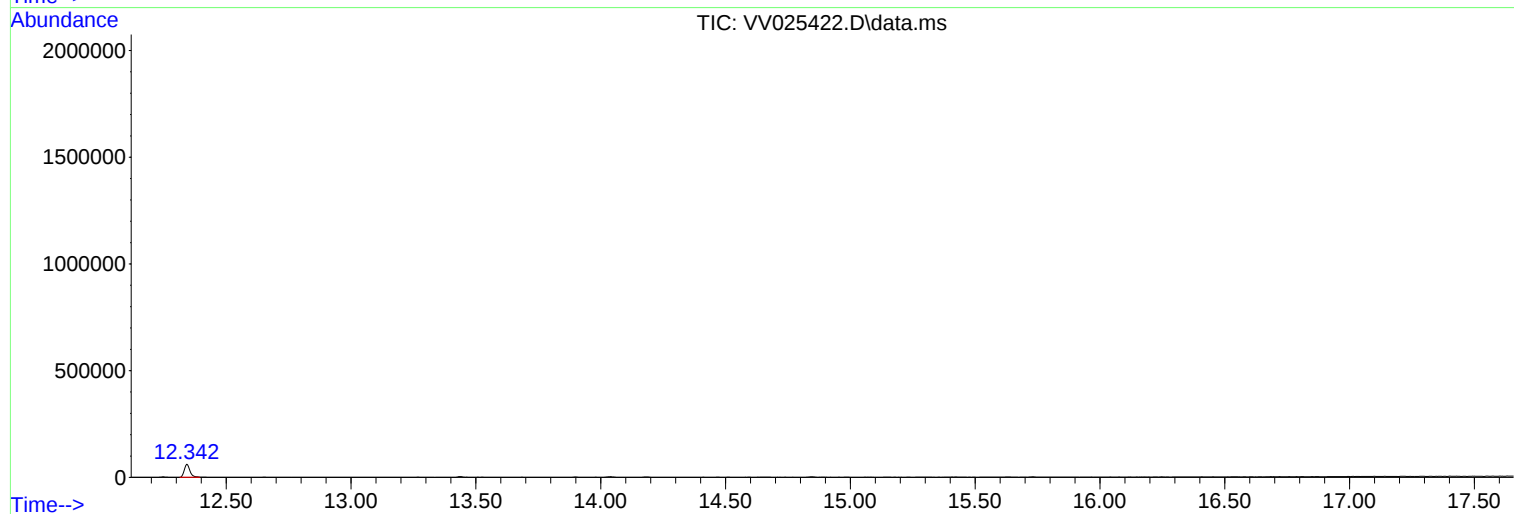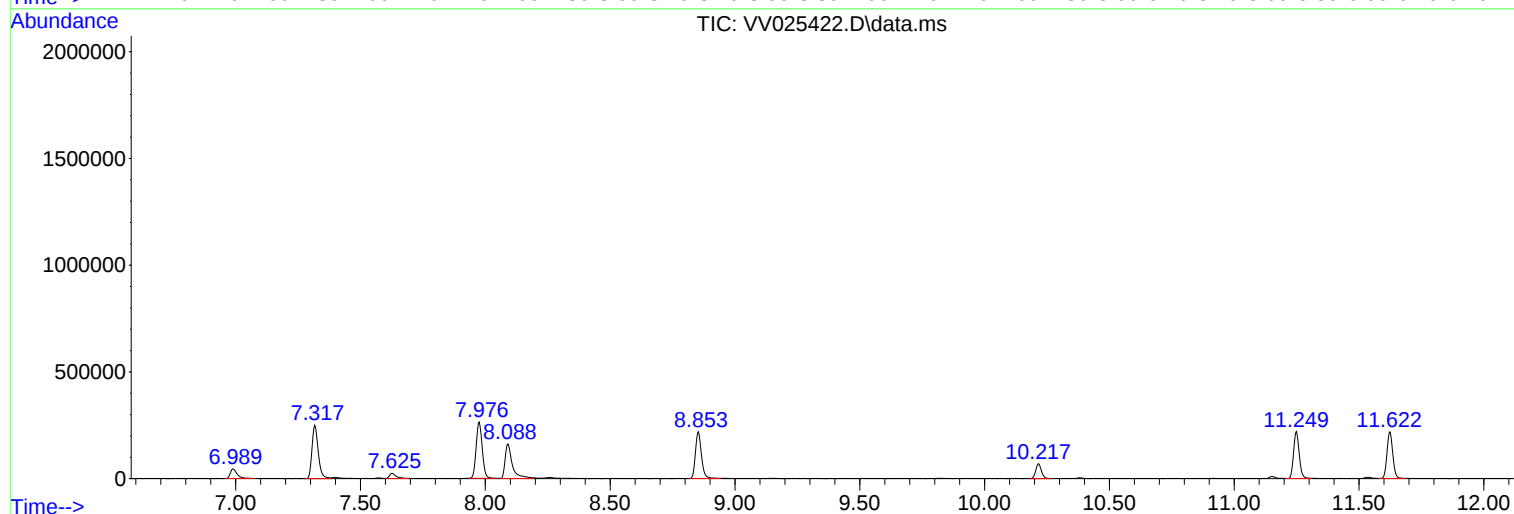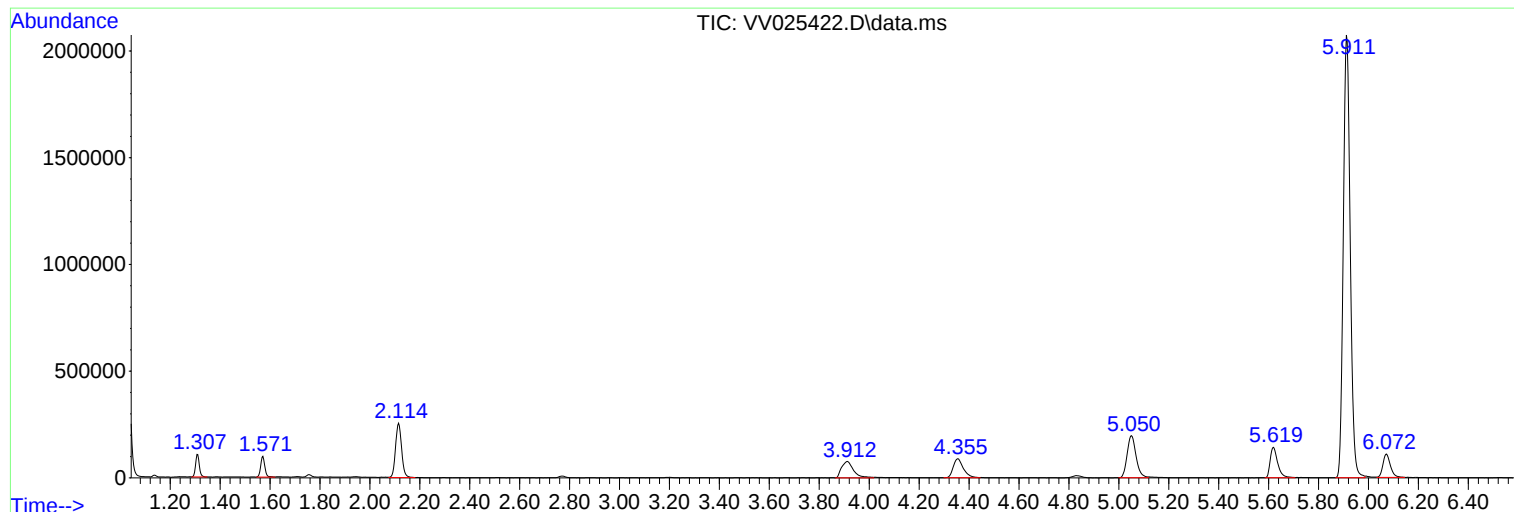

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040822\
Data File : VV025422.D
Acq On : 08 Apr 2022 20:17
Operator : SY/MD
Sample : N2319-02
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YB2G9










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Nonanal Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
12.342	1.37 ug/L	94609	1,4-Dichlorobenzene-d4	11.249

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Nonanal	142	C9H18O	000124-19-6	91
2			Nonanal	142	C9H18O	000124-19-6	91
3			Nonanal	142	C9H18O	000124-19-6	83
4			Nonanal	142	C9H18O	000124-19-6	64
5			Cyclohexanol, 4-methyl-	114	C7H14O	000589-91-3	30

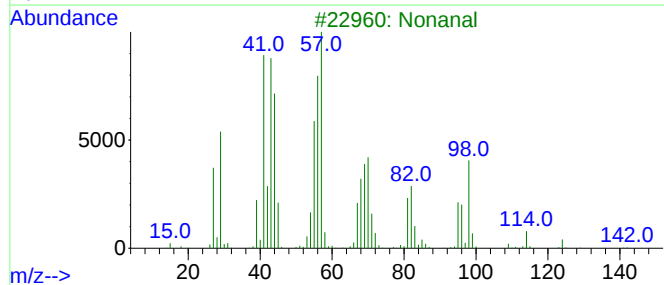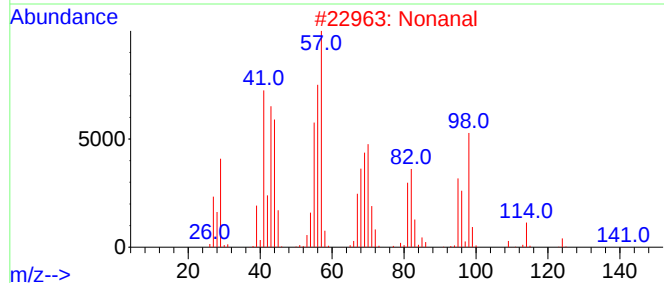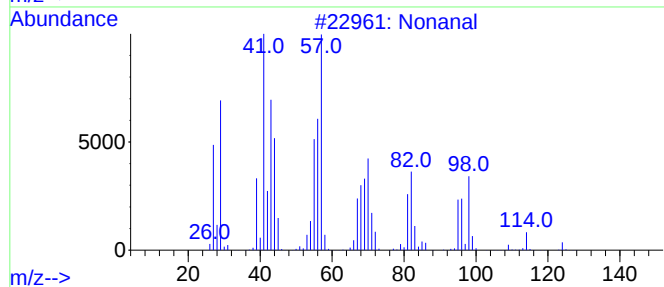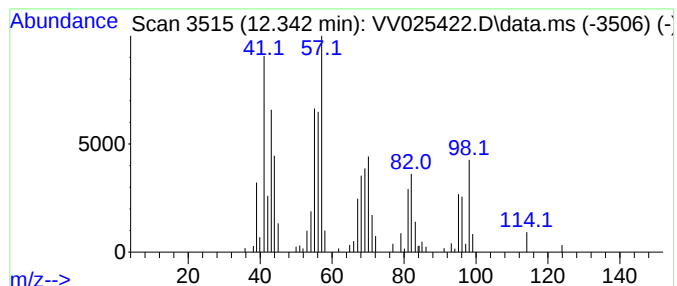

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040822\
Data File : VV025422.D
Acq On : 08 Apr 2022 20:17
Operator : SY/MD
Sample : N2319-02
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YB2G9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Nonanal	12.342	1.4	ug/L	94609	3	11.249	346267	5.0