

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040822\
 Data File : VV025432.D
 Acq On : 09 Apr 2022 00:12
 Operator : SY/MD
 Sample : N2319-16
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YB2J6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV025432.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.137	25	30	41	rVB	20980	20751	4.69%	0.497%
2	1.310	76	84	97	rVB	97728	99313	22.44%	2.377%
3	1.571	157	165	178	rBV	84863	98837	22.33%	2.365%
4	2.111	323	333	361	rVB	174782	264621	59.80%	6.333%
5	3.908	879	892	929	rBV3	50028	182389	41.21%	4.365%
6	4.352	1014	1030	1057	rBV	78164	210128	47.48%	5.029%
7	4.831	1168	1179	1190	rBV3	3241	6896	1.56%	0.165%
8	5.050	1233	1247	1274	rBV3	176637	442542	100.00%	10.591%
9	5.619	1411	1424	1446	rBV	125157	255728	57.79%	6.120%
10	5.915	1504	1516	1545	rBV	180395	363397	82.12%	8.697%
11	6.072	1553	1565	1584	rBV	98984	204117	46.12%	4.885%
12	6.989	1838	1850	1871	rBV2	39035	75219	17.00%	1.800%
13	7.317	1938	1952	1972	rBV	213424	375082	84.76%	8.976%
14	7.629	2039	2049	2062	rBV	21300	39001	8.81%	0.933%
15	7.937	2134	2145	2148	rBV2	5374	7555	1.71%	0.181%
16	7.976	2148	2157	2171	rVB	74079	123381	27.88%	2.953%
17	8.092	2181	2193	2219	rBV	156791	315148	71.21%	7.542%
18	8.854	2419	2430	2454	rBV	195921	327972	74.11%	7.849%
19	10.217	2842	2854	2866	rBV	65358	104589	23.63%	2.503%
20	10.381	2890	2905	2915	rVB5	8392	14234	3.22%	0.341%
21	11.249	3164	3175	3198	rBV	191456	294137	66.47%	7.039%
22	11.529	3255	3262	3271	rBV3	11028	18191	4.11%	0.435%
23	11.622	3280	3291	3306	rBV	198251	309118	69.85%	7.398%
24	12.249	3478	3486	3496	rVB2	5792	9354	2.11%	0.224%
25	12.349	3505	3517	3526	rBV7	4638	7449	1.68%	0.178%
26	14.043	4033	4044	4054	rVB2	5288	9365	2.12%	0.224%




Sum of corrected areas: 4178514

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040822\
Data File : VV025432.D
Acq On : 09 Apr 2022 00:12
Operator : SY/MD
Sample : N2319-16
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YB2J6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

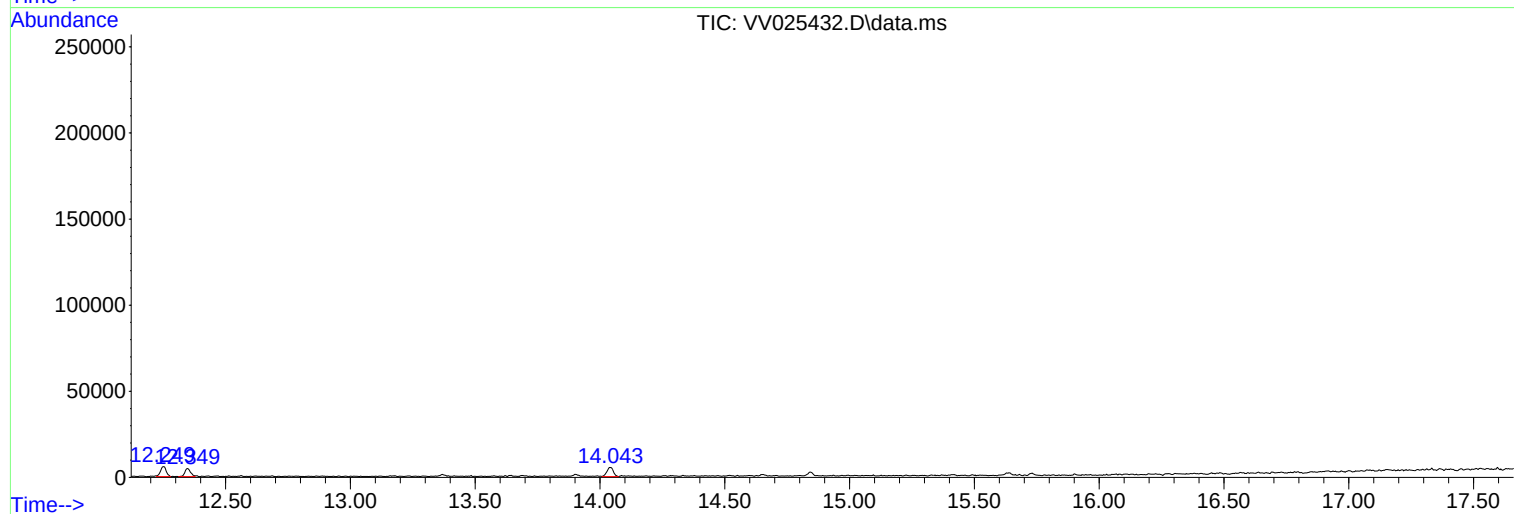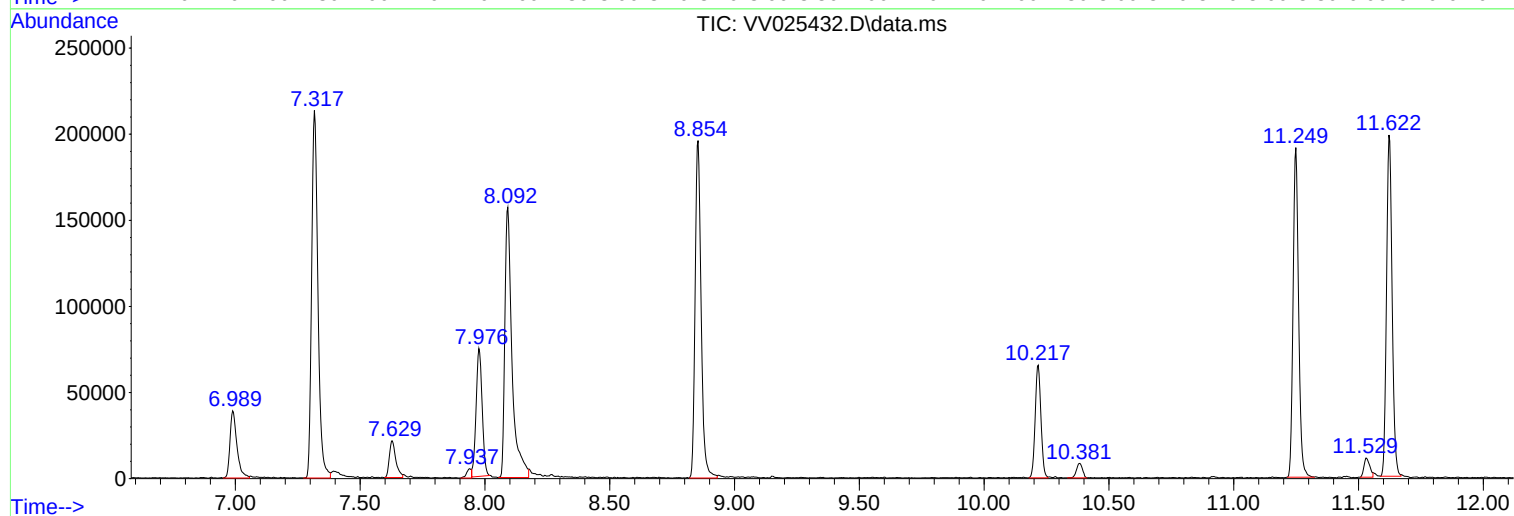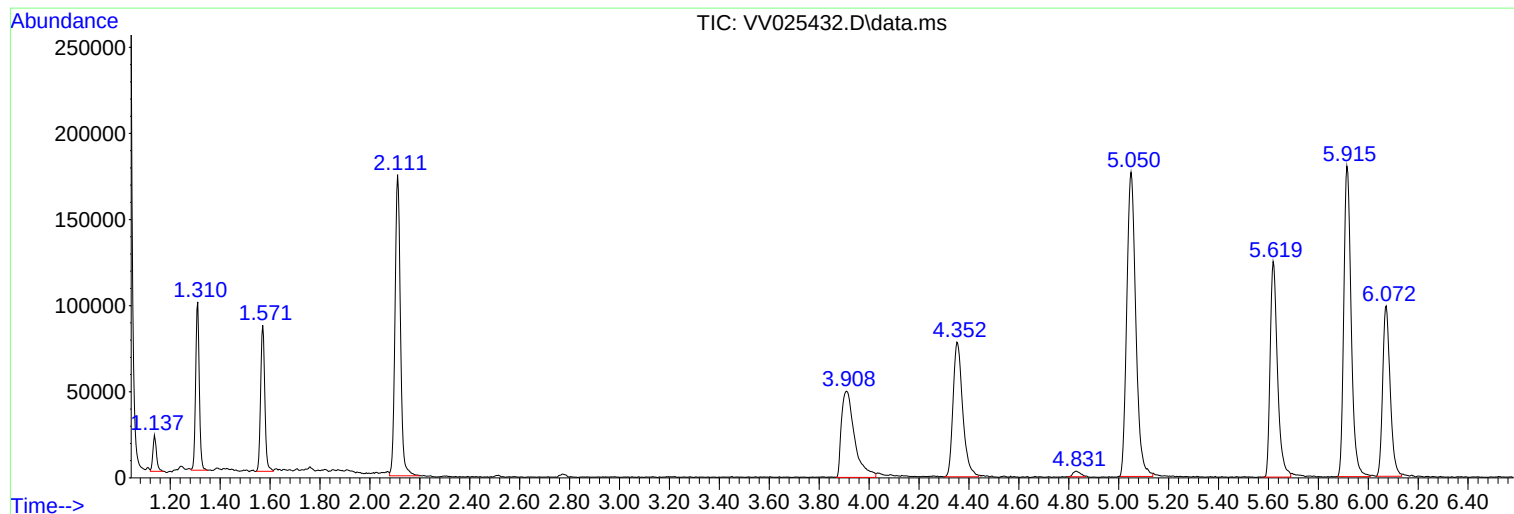

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040822\
Data File : VV025432.D
Acq On : 09 Apr 2022 00:12
Operator : SY/MD
Sample : N2319-16
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YB2J6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040822\
Data File : VV025432.D
Acq On : 09 Apr 2022 00:12
Operator : SY/MD
Sample : N2319-16
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YB2J6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------