
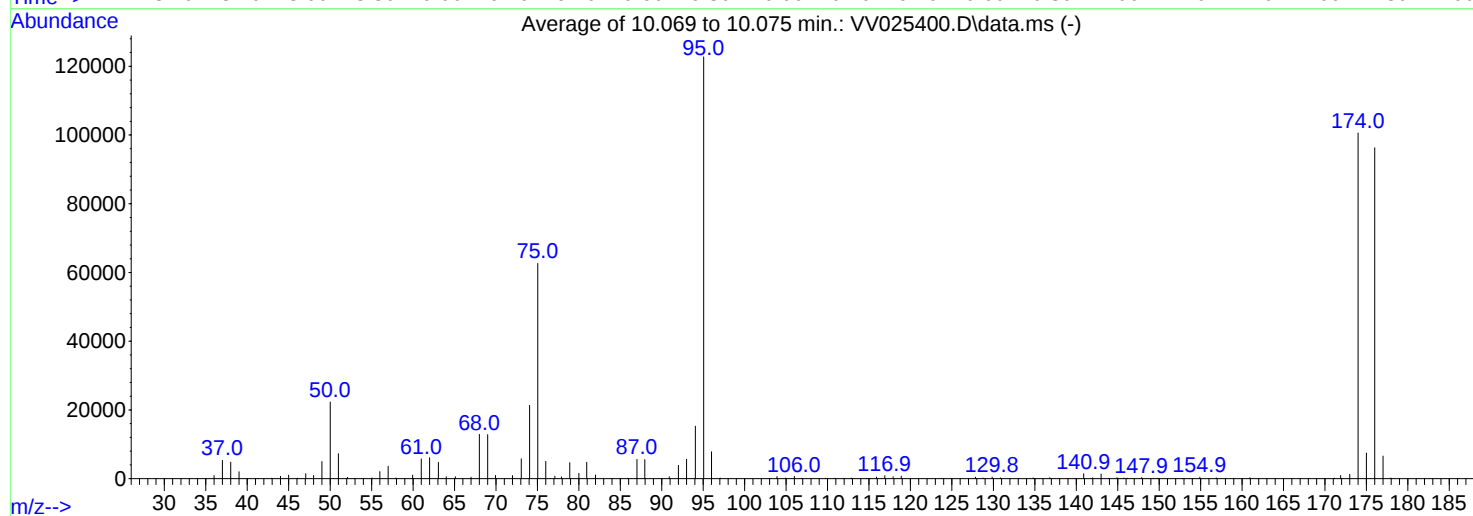


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040822\
 Data File : VV025400.D
 Acq On : 08 Apr 2022 08:55
 Operator : SY/MD
 Sample : BFB298
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB298

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Wed Apr 13 02:31:13 2022

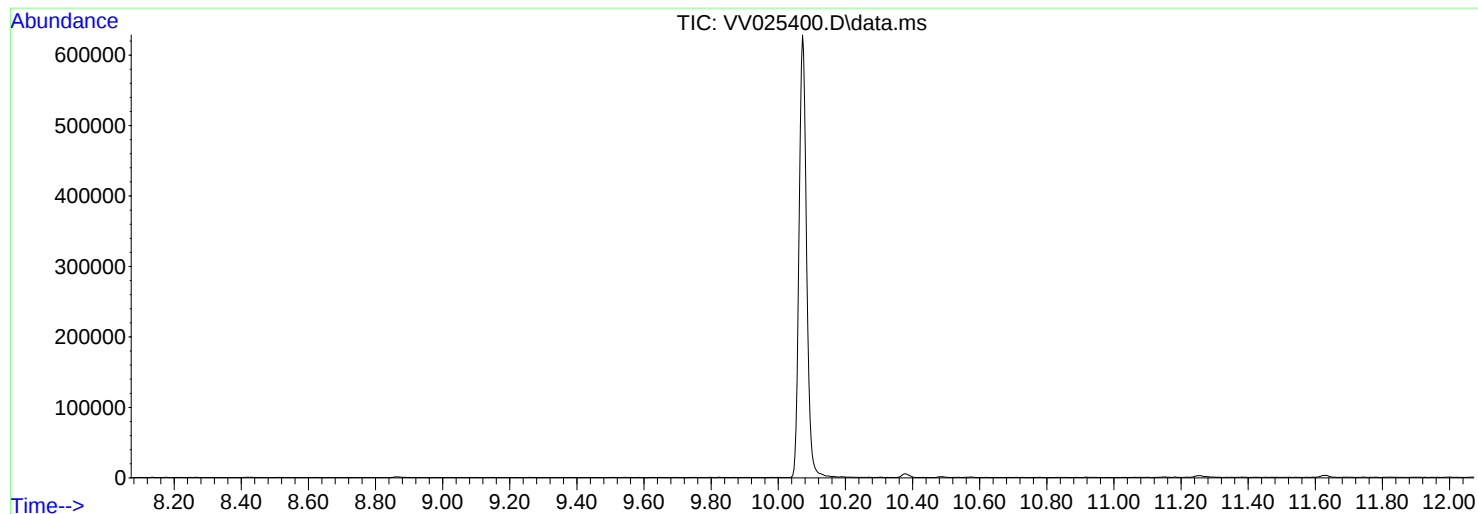

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.2	22296	PASS
75	95	30	80	51.0	62635	PASS
95	95	100	100	100.0	122757	PASS
96	95	5	9	6.4	7823	PASS
173	174	0.00	2	1.2	1253	PASS
174	95	50	120	82.0	100648	PASS
175	174	5	9	7.4	7456	PASS
176	174	95	105	95.7	96323	PASS
177	176	5	10	6.8	6547	PASS

m/z	Abundance
40.00	152.0
44.10	314.0

Instrument :
MSVOA_V
ClientSampleId :
BFB298

m/z	Abundance
36.00	877.0
37.00	5131.0
38.00	4924.0
39.00	1911.0
40.00	228.0
41.30	109.0
42.90	162.0
44.00	976.0
45.00	1102.0
46.00	175.0
47.10	1442.0
48.00	874.0
49.00	4750.0
50.00	22304.0
51.00	6904.0
52.10	398.0
55.00	208.0
56.00	1991.0
57.00	3639.0
58.00	182.0
60.00	983.0
61.00	5578.0
62.00	6227.0
63.00	4909.0
64.00	584.0
65.10	535.0
67.00	404.0
68.00	12338.0
69.00	12386.0
70.00	888.0
72.00	827.0
73.10	5678.0
74.10	20440.0
75.10	61520.0
76.00	5073.0
77.10	747.0
77.90	546.0
78.90	4647.0
80.00	1521.0
81.00	4614.0
82.00	1043.0
83.00	143.0
85.90	253.0
87.00	5391.0
87.90	5475.0
90.90	574.0
92.00	3725.0
93.00	5085.0
94.00	15138.0
95.10	119608.0
96.00	7747.0
97.00	230.0
103.90	561.0
105.00	182.0
106.00	640.0
106.80	163.0
109.70	109.0
110.90	159.0
111.90	106.0
112.80	178.0
114.70	168.0
115.90	452.0
116.90	807.0
117.90	563.0
118.90	708.0
123.70	130.0
127.90	404.0
128.80	200.0
129.90	459.0
131.00	218.0
134.80	209.0
136.80	303.0
140.90	1525.0
141.90	200.0
143.00	1305.0
144.90	266.0
145.80	229.0
146.20	154.0
147.90	276.0
149.80	110.0
152.80	120.0
154.90	364.0
156.90	229.0
159.00	158.0
161.00	192.0
171.10	113.0
171.90	803.0
173.00	1220.0
174.00	94592.0
175.00	7236.0
176.00	91592.0
177.00	6431.0

Instrument :
MSVOA_V
ClientSampleId :
BFB298

177.90

190.0

Instrument :
MSVOA_V
ClientSampleId :
BFB298

m/z	Abundance
36.00	905.0
37.00	5504.0
38.00	4961.0
39.00	2015.0
40.00	254.0
42.90	142.0
44.00	1036.0
45.00	1088.0
46.00	157.0
47.10	1504.0
48.00	978.0
49.00	5168.0
50.00	23120.0
51.00	7489.0
52.10	432.0
55.10	249.0
56.00	2079.0
57.00	3830.0
57.90	178.0
59.90	1079.0
61.00	5918.0
62.00	6386.0
63.10	4854.0
64.00	582.0
65.10	553.0
67.00	456.0
68.00	13390.0
69.00	13399.0
69.90	984.0
72.00	920.0
73.00	5931.0
74.00	22040.0
75.10	64800.0
76.00	5132.0
77.10	741.0
77.90	526.0
78.90	4842.0
80.00	1597.0
81.00	4883.0
82.00	1093.0
83.00	144.0
85.90	182.0
87.00	5802.0
88.00	5761.0
90.90	595.0
92.00	4038.0
93.00	5825.0
94.10	15774.0
95.10	126728.0
96.00	8038.0
97.10	203.0
103.90	658.0
104.90	167.0
106.00	655.0
106.90	163.0
109.70	146.0
110.90	182.0
112.90	185.0
114.70	138.0
115.20	119.0
115.90	475.0
116.90	923.0
117.90	602.0
118.90	741.0
123.70	115.0
127.90	475.0
128.80	206.0
129.90	485.0
130.80	216.0
134.80	220.0
136.80	313.0
140.90	1508.0
142.00	281.0
143.00	1406.0
144.00	120.0
144.90	293.0
145.70	210.0
146.20	155.0
147.90	330.0
149.30	113.0
149.90	133.0
152.80	108.0
153.70	100.0
154.90	439.0
156.90	228.0
159.00	175.0
161.00	320.0
171.20	166.0
171.90	915.0
173.00	1294.0
174.00	104400.0
175.00	7730.0

Instrument :
MSVOA_V
ClientSampleId :
BFB298

176.00	99672.0
177.00	6811.0
178.00	181.0

Instrument :
MSVOA_V
ClientSampleId :
BFB298

m/z	Abundance
36.00	845.0
37.00	5345.0
38.00	4557.0
39.00	2047.0
40.00	270.0
42.90	104.0
44.00	1047.0
45.00	956.0
46.10	127.0
47.00	1389.0
48.00	891.0
49.00	5061.0
50.00	21464.0
51.00	7347.0
52.10	359.0
52.90	116.0
53.80	101.0
55.00	281.0
56.00	2016.0
57.00	3473.0
57.90	170.0
59.90	1072.0
61.00	5689.0
62.00	5717.0
63.10	4502.0
64.00	489.0
65.10	556.0
67.00	426.0
68.00	12962.0
69.00	12702.0
69.90	963.0
72.00	891.0
73.00	5697.0
74.00	21480.0
75.00	61584.0
76.00	4820.0
77.10	648.0
77.90	483.0
78.90	4543.0
80.00	1564.0
80.90	4802.0
82.00	1054.0
83.00	127.0
87.00	5585.0
88.00	5445.0
90.90	516.0
92.00	3860.0
93.00	5994.0
94.10	14925.0
95.00	121936.0
96.00	7685.0
97.10	192.0
103.90	645.0
104.90	158.0
106.00	606.0
107.00	158.0
109.80	146.0
110.90	148.0
112.90	187.0
115.10	123.0
115.90	441.0
116.90	883.0
117.90	560.0
118.90	748.0
127.80	444.0
128.70	178.0
129.80	465.0
130.80	233.0
134.80	217.0
136.80	261.0
139.80	103.0
140.90	1356.0
142.00	293.0
143.00	1377.0
143.90	143.0
144.90	286.0
145.70	156.0
146.10	139.0
147.90	352.0
149.30	111.0
149.90	126.0
154.90	405.0
156.90	189.0
159.00	148.0
160.90	357.0
171.20	186.0
171.90	975.0
173.00	1245.0
174.00	102952.0
175.00	7401.0
176.00	97704.0
177.00	6398.0

Instrument :
MSVOA_V
ClientSampleId :
BFB298

178.00

169.0

Instrument :
MSVOA_V
ClientSampleId :
BFB298