

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV041119\
 Data File : VV010267.D
 Acq On : 12 Apr 2019 03:13
 Operator : SY/MD
 Sample : K2354-09
 Misc : 5.91G/10mL/MSVOA_V/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BF164

Quant Time: Apr 12 04:49:23 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM041019S.M
 Quant Title : VOC Analysis
 QLast Update : Fri Apr 12 04:45:26 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	241332	25.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	215775	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	96486	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.31	65	46476	16.73	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	66.92%
7) Chloroethane-d5	1.56	69	47788	20.02	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	80.08%
10) 1,1-Dichloroethene-d2	2.12	63	99224	14.03	ug/L	-0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	56.12%
20) 2-Butanone-d5	3.94	46	43211	61.47	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	122.94%
24) Chloroform-d	4.40	84	127411	23.12	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	92.48%
26) 1,2-Dichloroethane-d4	5.08	65	80086	25.51	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	102.04%
29) Benzene-d6	5.09	84	250313	24.06	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	96.24%
33) 1,2-Dichloropropane-d6	6.11	67	78441	25.35	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	101.40%
37) Toluene-d8	7.36	98	218563	21.54	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	86.16%
38) trans-1,3-Dichloropropene-	7.66	79	27848	21.58	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	86.32%
39) 2-Hexanone-d5	8.13	63	31538	59.00	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	118.00%
48) 1,1,2,2-Tetrachloroethane-	10.26	84	74923	26.97	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	107.88%
61) 1,2-Dichlorobenzene-d4	11.67	152	84273	23.65	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	94.60%


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
59) 1,2,3-Trichloropropane	11.30	75	11295	5.469	ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV041119\
Data File : VV010267.D
Acq On : 12 Apr 2019 03:13
Operator : SY/MD
Sample : K2354-09
Misc : 5.91G/10mL/MSVOA_V/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BF164

Quant Time: Apr 12 04:49:23 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM041019S.M
Quant Title : VOC Analysis
QLast Update : Fri Apr 12 04:45:26 2019
Response via : Initial Calibration

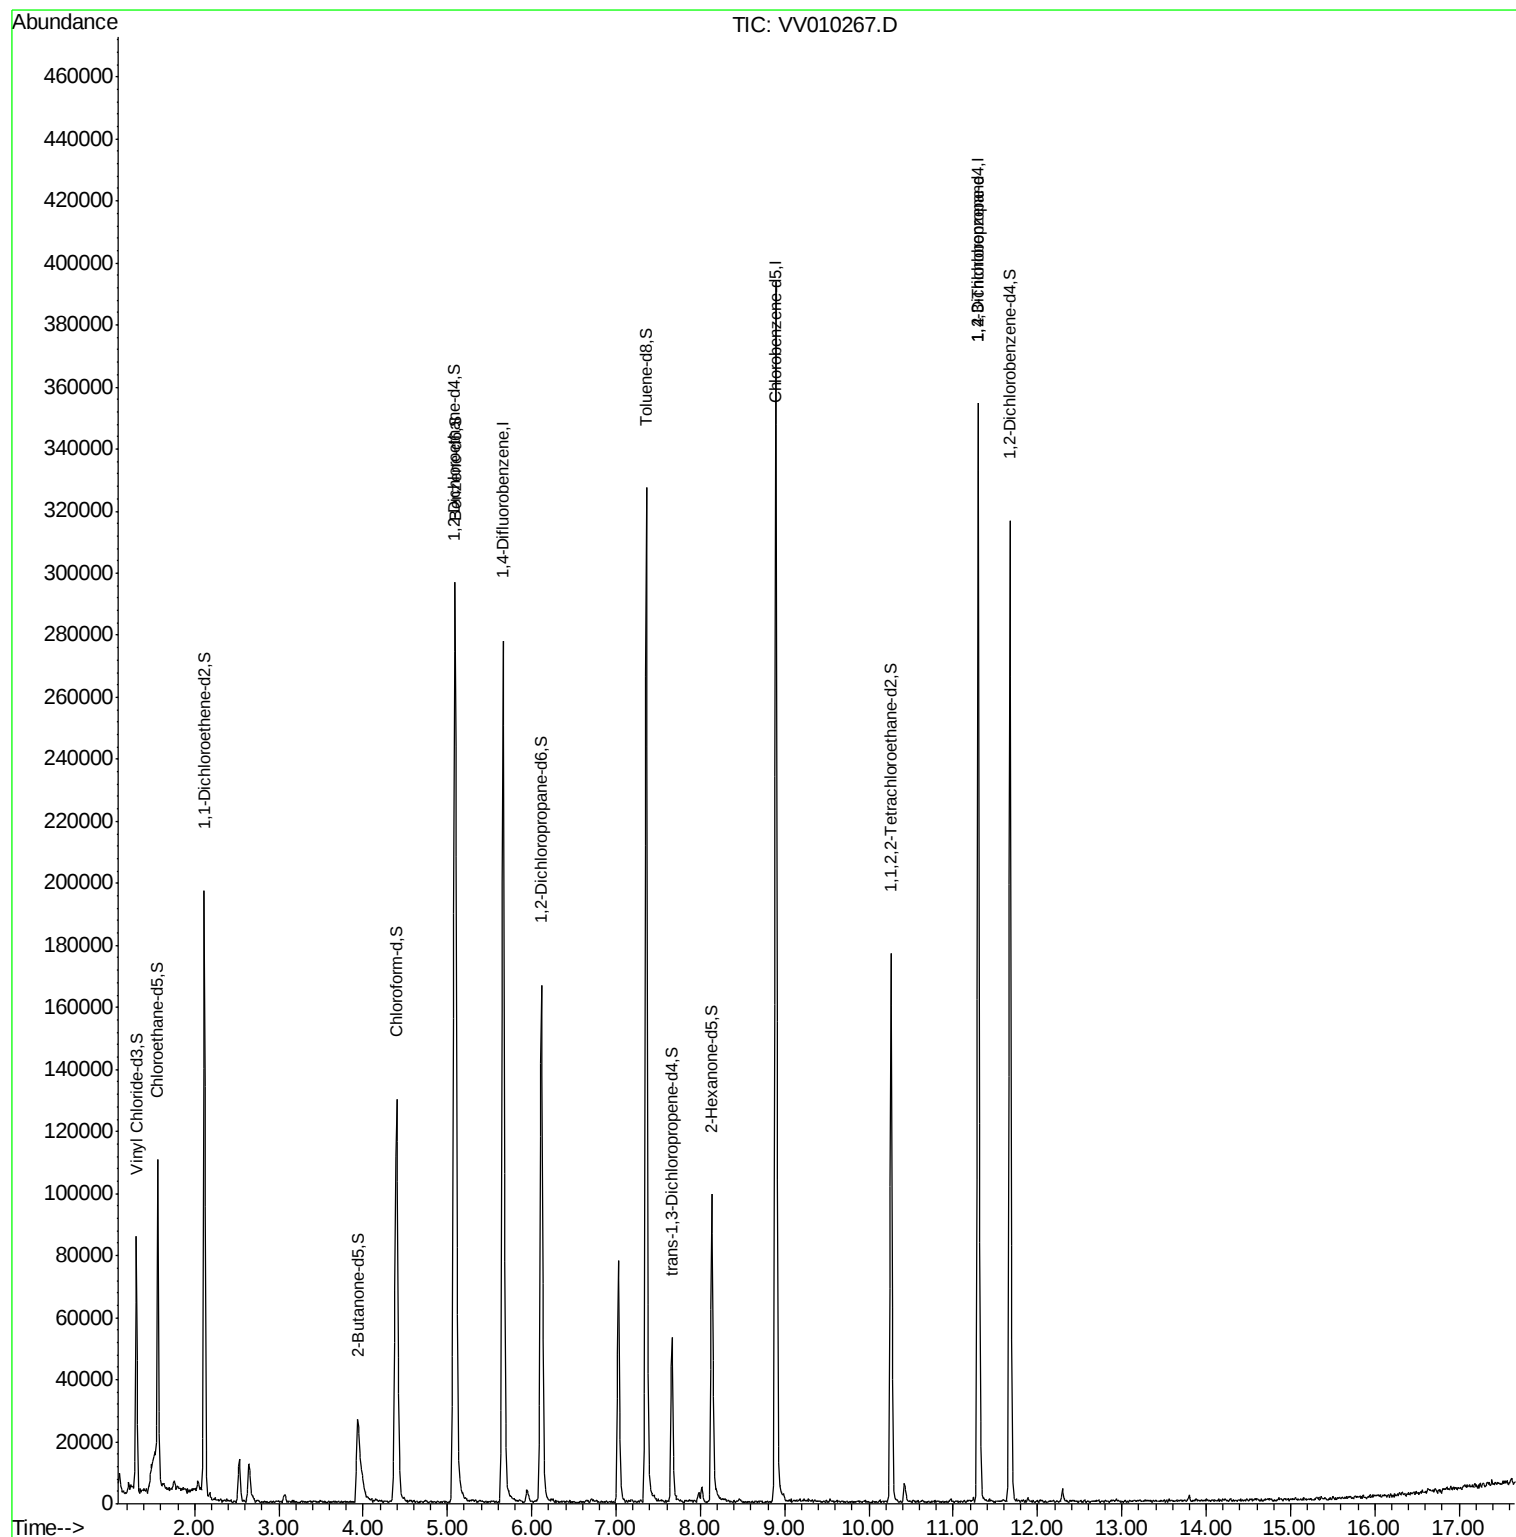

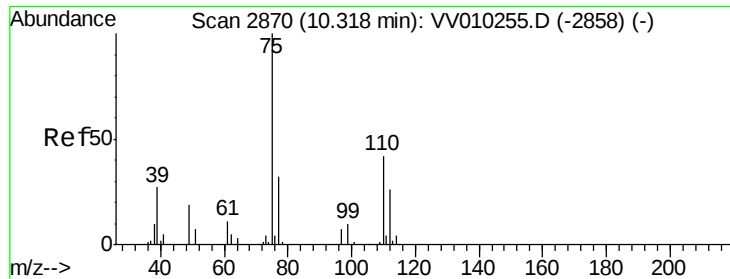

#59
 1,2,3-Trichloropropane
 Concen: 5.469 ug/L
 RT: 11.30 min Scan# 3174
 Delta R.T. 0.98 min
 Lab File: VV010267.D
 Acq: 12 Apr 2019 03:13

Instrument :
 MSVOA_V
 ClientSampleId :
 BF164

Tgt Ion: 75 Resp: 11295
 Ion Ratio Lower Upper
 75 100
 77 37.7 26.9 40.3

