


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV041119\
Data File : VV010238.D
Acq On : 11 Apr 2019 12:44
Operator : SY/MD
Sample : K2278-07
Misc : 5.42G/10mL/MSVOA_V/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DB6X4

Manual Integrations
APPROVED

MMDadoda
4/15/2019 12:29:36 AM

Quant Time: Apr 12 07:21:52 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM041019S.M
Quant Title : VOC Analysis
QLast Update : Fri Apr 12 04:45:26 2019
Response via : Initial Calibration

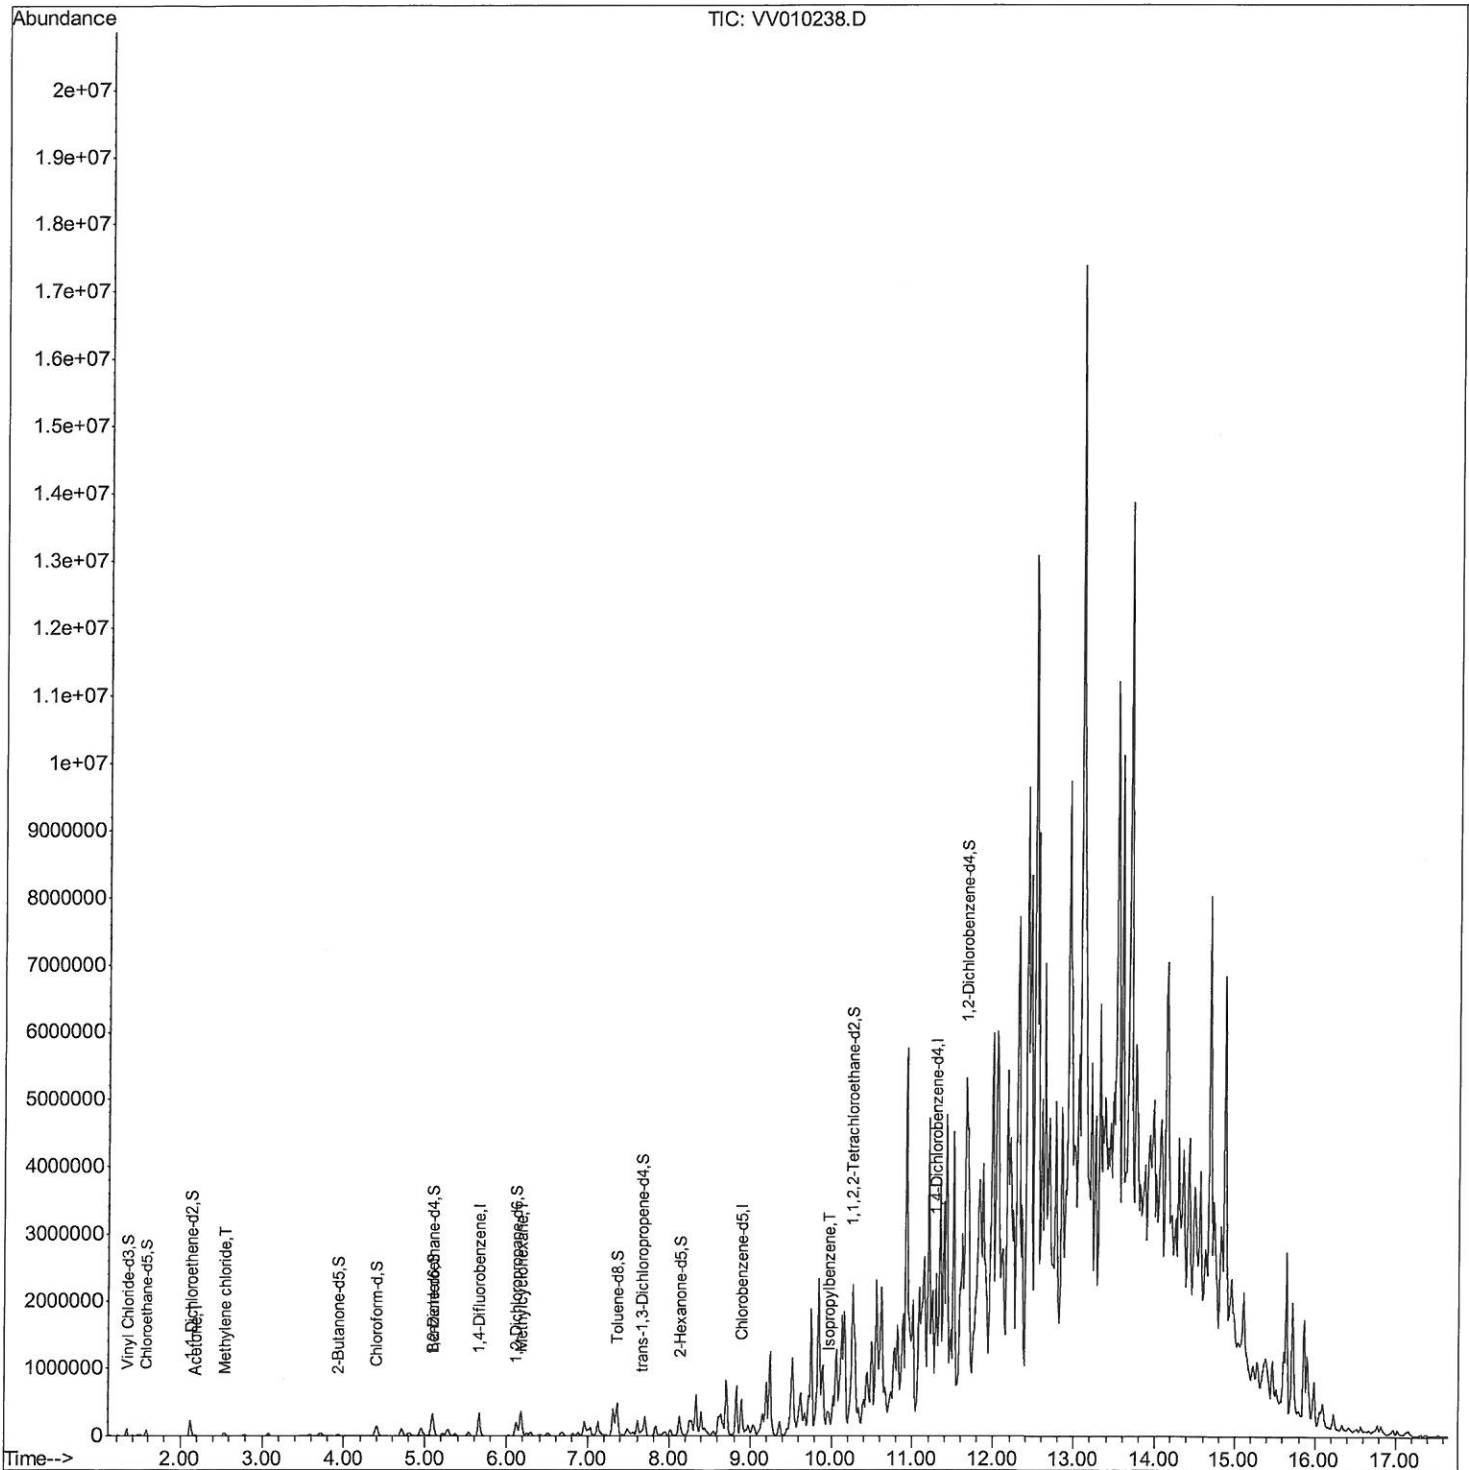

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV041119\
 Data File : VV010238.D
 Acq On : 11 Apr 2019 12:44
 Operator : SY/MD
 Sample : K2278-07
 Misc : 5.42G/10mL/MSVOA_V/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DB6X4

Manual Integrations
 APPROVED

MMDadoda
 4/15/2019 12:29:36 AM

Quant Time: Apr 12 07:19:17 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM041019S.M
 Quant Title : VOC Analysis
 QLast Update : Fri Apr 12 04:45:26 2019
 Response via : Initial Calibration

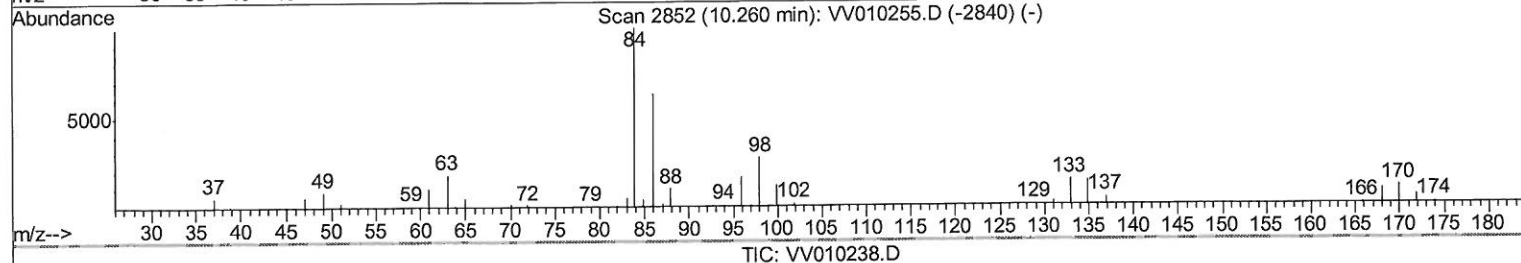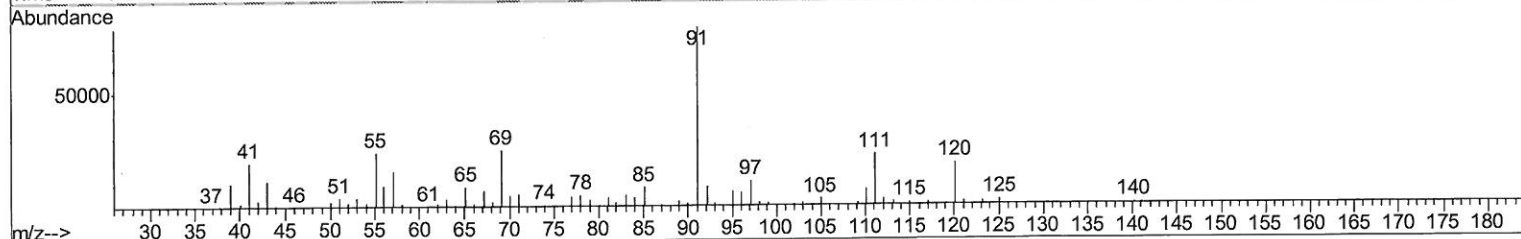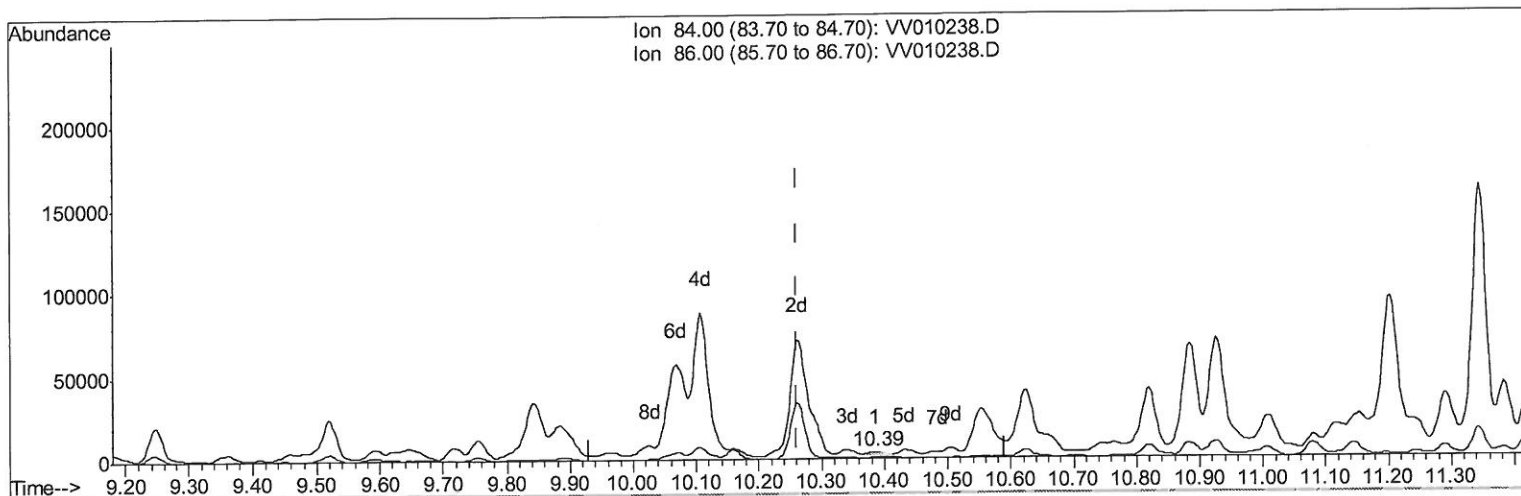

(48) 1,1,2,2-Tetrachloroethane-d2 (S)

10.386min (+0.126) 0.63ug/L

response 2396

Ion	Exp%	Act%
84.00	100	100
86.00	62.40	43.86
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV041119\
 Data File : VV010238.D
 Acq On : 11 Apr 2019 12:44
 Operator : SY/MD
 Sample : K2278-07
 Misc : 5.42G/10mL/MSVOA_V/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DB6X4

Manual Integrations
 APPROVED

MMDadoda
 4/15/2019 12:29:36 AM

Quant Time: Apr 12 07:19:17 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM041019S.M
 Quant Title : VOC Analysis
 QLast Update : Fri Apr 12 04:45:26 2019
 Response via : Initial Calibration

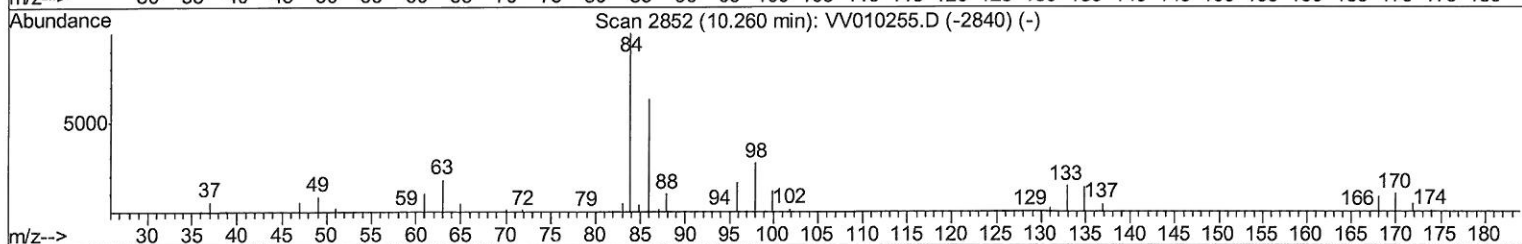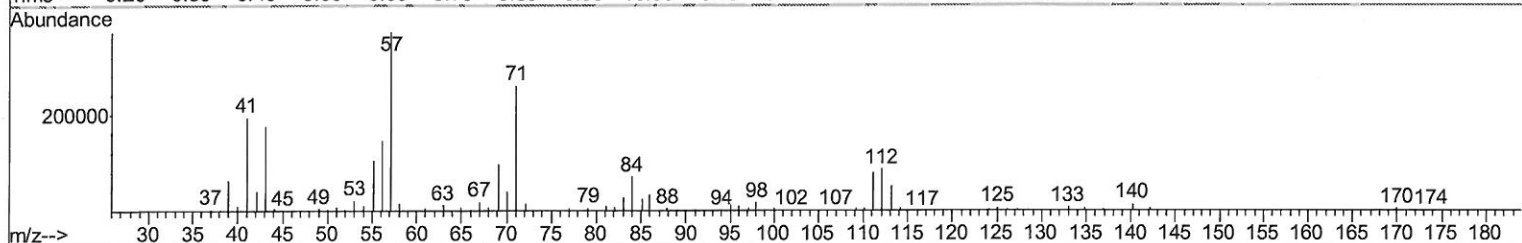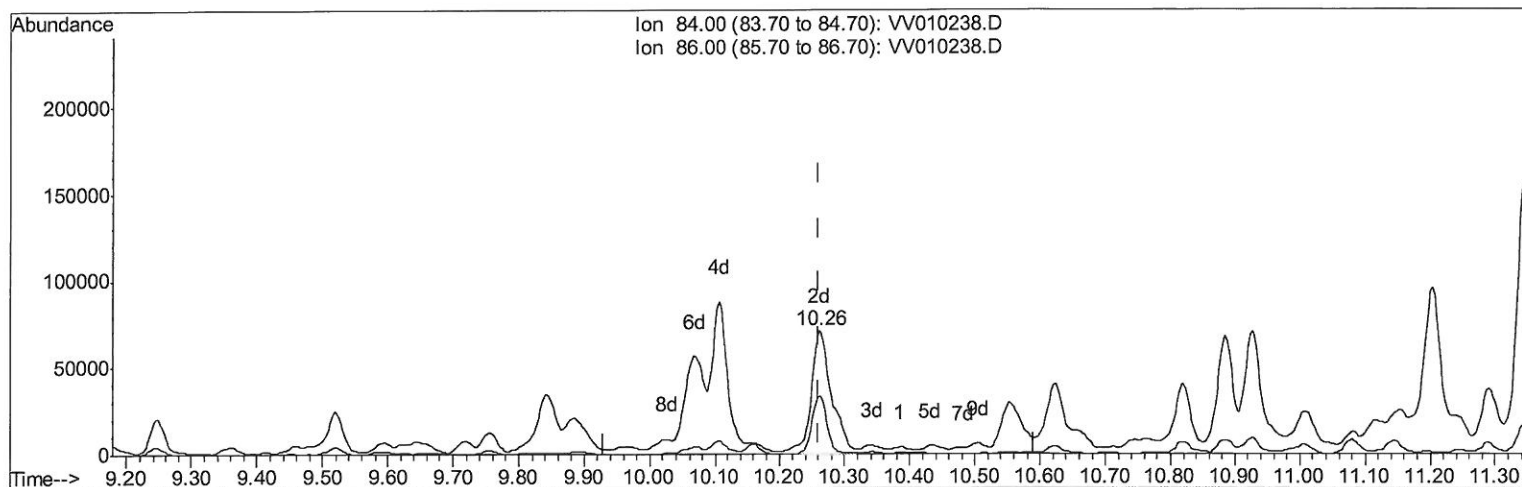

TIC: VV010238.D

(48) 1,1,2,2-Tetrachloroethane-d2 (S)

10.260min (+0.000) 41.11ug/L m

response 155240

Ion	Exp%	Act%
84.00	100	100
86.00	62.40	0.68#
0.00	0.00	0.00
0.00	0.00	0.00

MD
 4/16/19

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV041119\
 Data File : VV010238.D
 Acq On : 11 Apr 2019 12:44
 Operator : SY/MD
 Sample : K2278-07
 Misc : 5.42G/10mL/MSVOA_V/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DB6X4

Manual Integrations
 APPROVED

MMDadoda
 4/15/2019 12:29:36 AM

Quant Time: Apr 12 07:21:52 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM041019S.M
 Quant Title : VOC Analysis
 QLast Update : Fri Apr 12 04:45:26 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	305364	25.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	293366	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	166429	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	56492	16.07	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	64.28%		
7) Chloroethane-d5	1.57	69	60173	19.92	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	79.68%		
10) 1,1-Dichloroethene-d2	2.13	63	121816	13.61	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	54.44%		
20) 2-Butanone-d5	3.93	46	36591	41.13	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	82.26%		
24) Chloroform-d	4.40	84	144158	20.67	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	82.68%		
26) 1,2-Dichloroethane-d4	5.08	65	83318	20.98	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	83.92%		
29) Benzene-d6	5.10	84	296027	20.93	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	83.72%		
33) 1,2-Dichloropropane-d6	6.12	67	88686	21.08	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	84.32%		
37) Toluene-d8	7.36	98	299513	21.71	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	86.84%		
38) trans-1,3-Dichloropropene-	7.66	79	34519	19.68	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	78.72%		
39) 2-Hexanone-d5	8.13	63	28227	38.84	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	77.68%		
48) 1,1,2,2-Tetrachloroethane-	10.26	84	155240m	41.11	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	164.44%#		
61) 1,2-Dichlorobenzene-d4	11.67	152	158434	25.78	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	103.12%		

MD
 4/16/19

Target Compounds

					Qvalue
13) Acetone	2.19	43	7322	7.704	ug/L 94
16) Methylene chloride	2.54	84	11077	1.852	ug/L 89
36) Methylcyclohexane	6.18	83	151112	23.536	ug/L 97
57) Isopropylbenzene	9.97	105	83712	4.548	ug/L 96

(#) = qualifier out of range (m) = manual integration (+) = signals summed