

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW041122\
 Data File : VW025442.D
 Acq On : 11 Apr 2022 12:05
 Operator : SY/MD
 Sample : N2320-07
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Apr 12 07:04:51 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Apr 12 07:03:45 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	179048	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	180171	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	84515	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	74049	4.448	ug/L	0.00
Spiked Amount	5.000	Range				

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041122\
Data File : VV025442.D
Acq On : 11 Apr 2022 12:05
Operator : SY/MD
Sample : N2320-07
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Apr 12 07:04:51 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Apr 12 07:03:45 2022
Response via : Initial Calibration

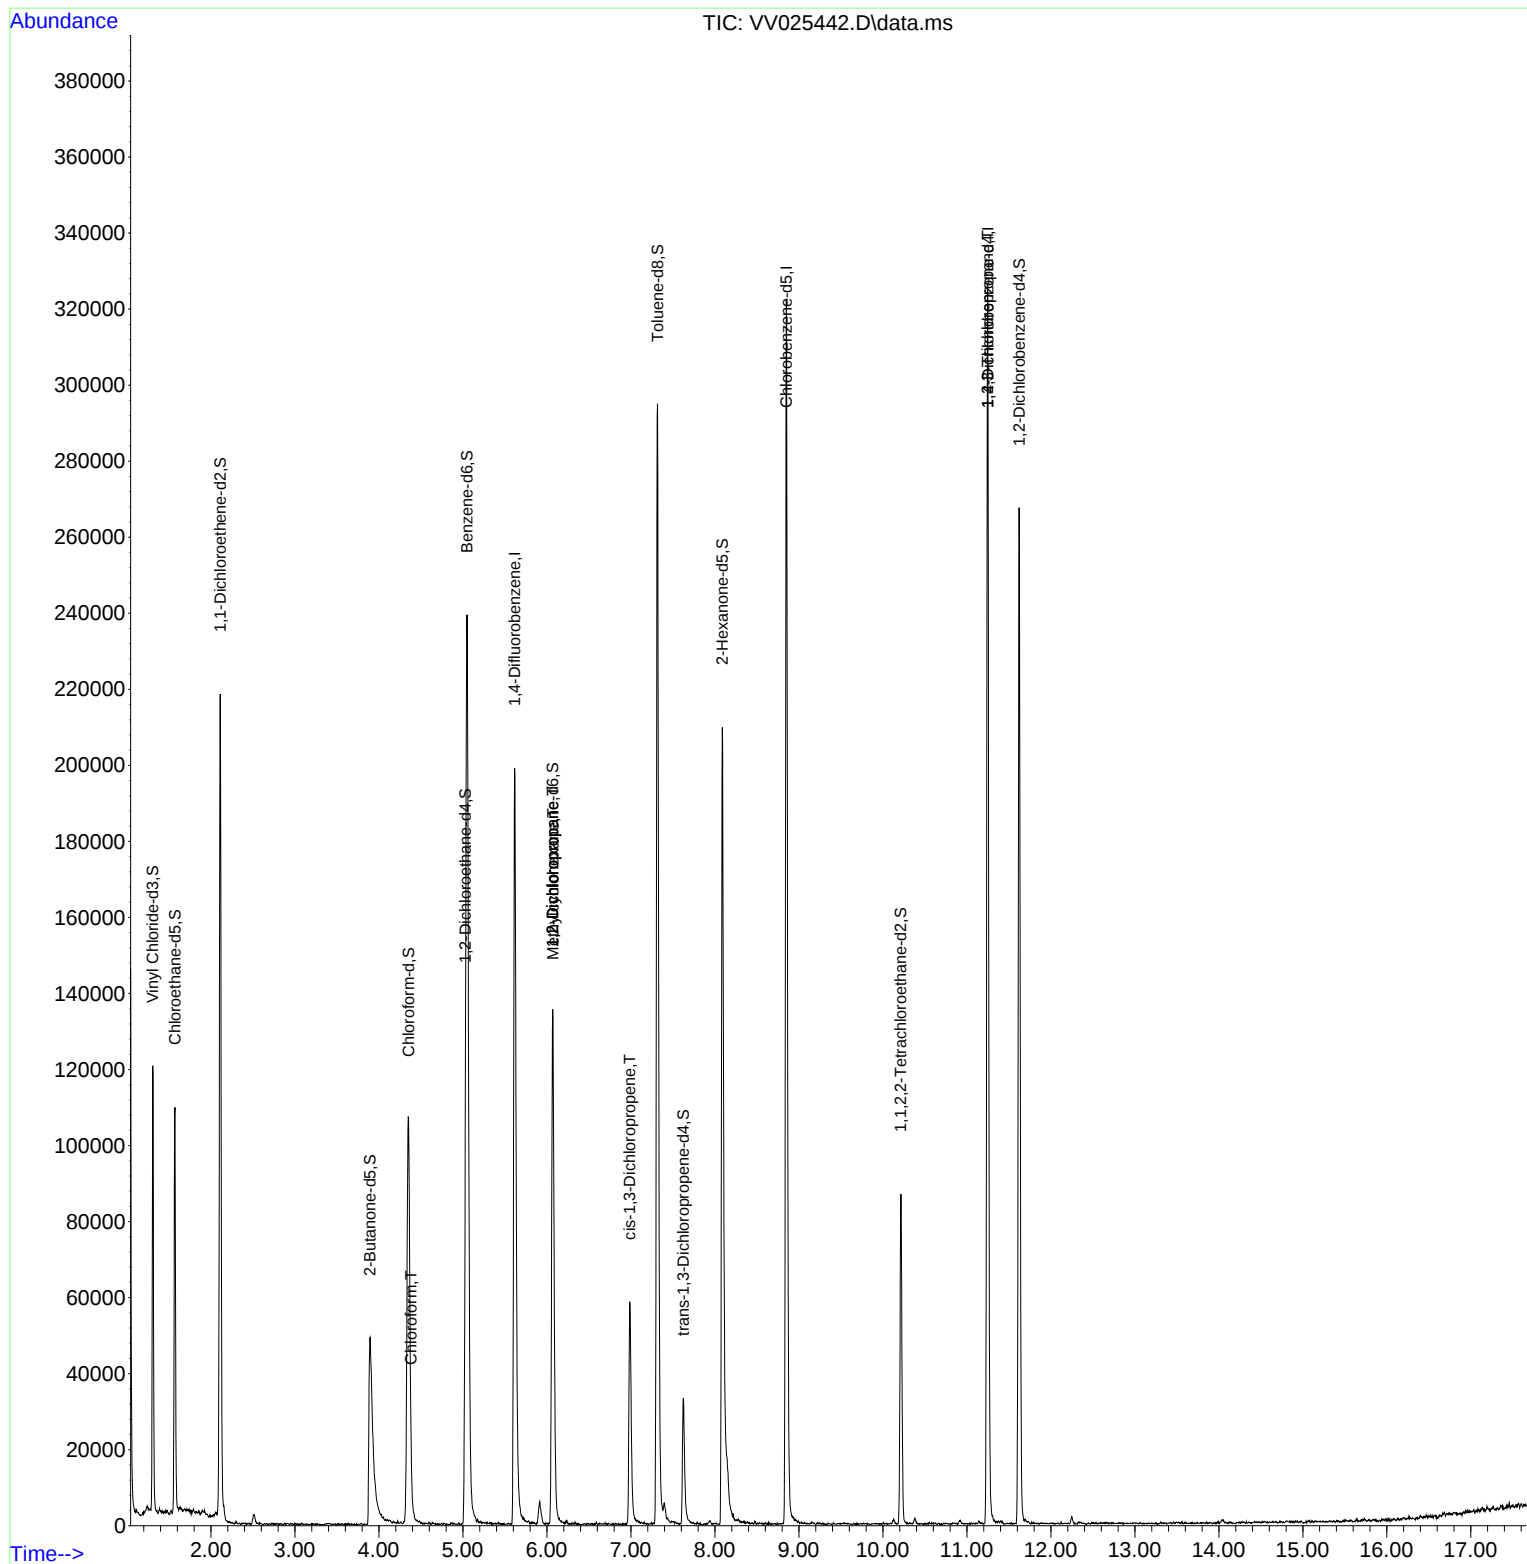

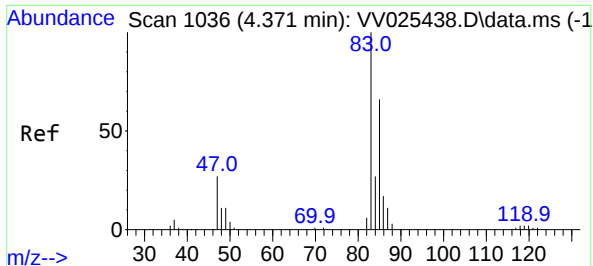

#25

Chloroform

Concen: 0.092 ug/L

RT: 4.381 min Scan# 10

Delta R.T. 0.010 min

Lab File: VV025442.D

Acq: 11 Apr 2022 12:05

Instrument :

MSVOA_V




ClientSampleId :


Tgt Ion: 83 Resp: 2141

Ion Ratio Lower Upper

83 100

85 62.1 43.5 80.7


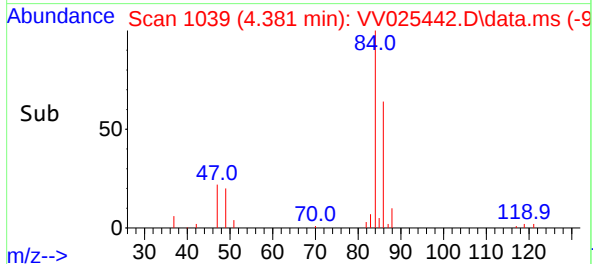
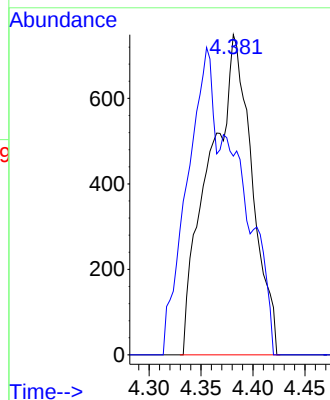
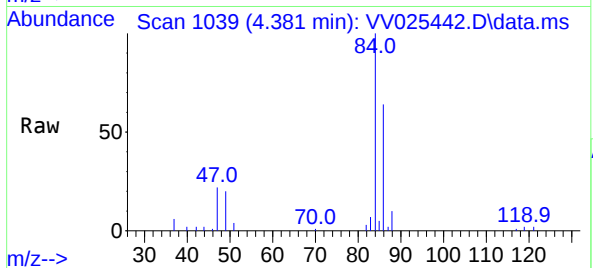


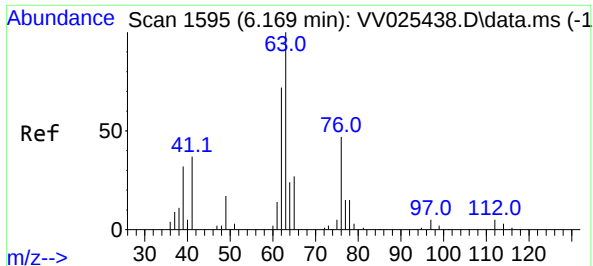

#37
1,2-Dichloropropane
Concen: 0.578 ug/L
RT: 6.069 min Scan# 11
Delta R.T. -0.100 min
Lab File: VV025442.D
Acq: 11 Apr 2022 12:05


Instrument :
MSVOA_V
ClientSampleId :

Tgt Ion: 63 Resp: 7122
Ion Ratio Lower Upper
63 100
112 0.0 3.8 5.8#

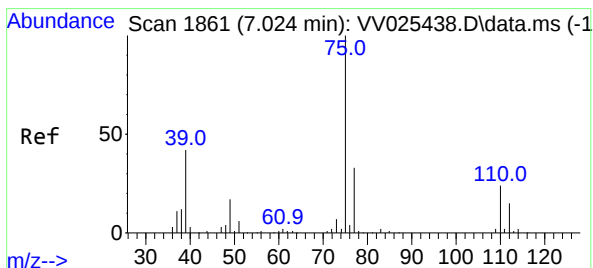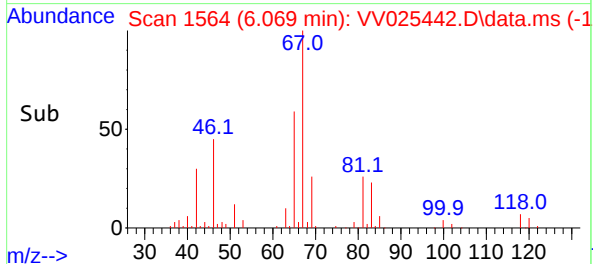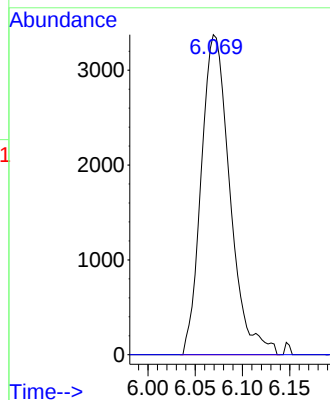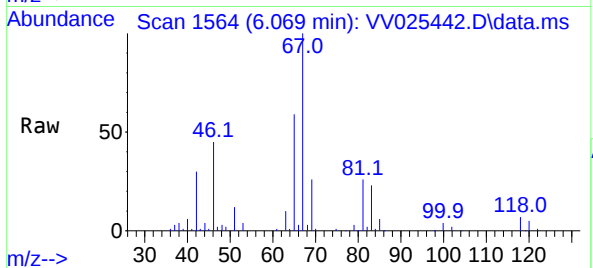


#39
cis-1,3-Dichloropropene
Concen: 0.099 ug/L
RT: 6.985 min Scan# 1849
Delta R.T. -0.038 min
Lab File: VV025442.D
Acq: 11 Apr 2022 12:05

Tgt Ion: 75 Resp: 15

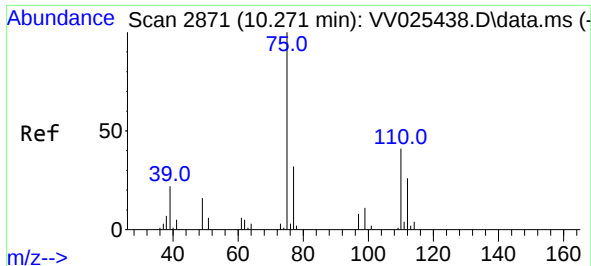

#61
1,2,3-Trichloropropane
Concen: 1.837 ug/L
RT: 11.246 min Scan# 31
Delta R.T. 0.974 min
Lab File: VV025442.D
Acq: 11 Apr 2022 12:05

Instrument :
MSVOA_V
ClientSampleId :

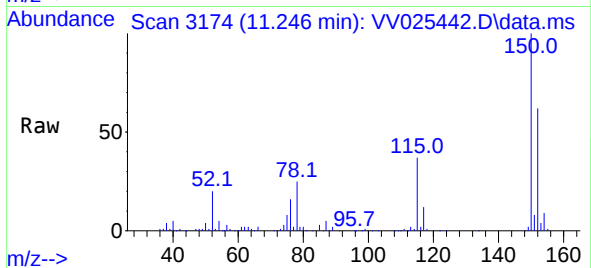

Tgt Ion:	75	Resp:	10225
Ion	Ratio	Lower	Upper
75	100		
77	33.6	25.6	38.4
110	3.3	34.7	52.1#

