

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041122\
 Data File : VV025449.D
 Acq On : 11 Apr 2022 14:49
 Operator : SY/MD
 Sample : N2319-17DL 5X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YB2K4DL

Manual IntegrationsAPPROVED

Quant Time: Apr 12 07:06:16 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Apr 12 07:03:45 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 04/12/2022
 Supervised By :Mahesh Dadoda 04/15/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	134132	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	131817	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	64062	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	61540	4.935	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130	Recovery	=	98.600%	
7) Chloroethane-d5	1.568	69	56178	4.235	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130	Recovery	=	84.600%	
11) 1,1-Dichloroethene-d2	2.105	63	98245	3.933	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125	Recovery	=	78.600%	
20) 2-Butanone-d5	3.905	46	80501	53.070	ug/L	0.02
Spiked Amount 50.000	Range 40	- 130	Recovery	=	106.140%	
24) Chloroform-d	4.349	84	92185	4.892	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	97.800%	
26) 1,2-Dichloroethane-d4	5.030	65	41772	5.145	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	102.800%	
32) Benzene-d6	5.050	84	184158	4.829	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	96.600%	
36) 1,2-Dichloropropane-d6	6.069	67	54202	5.096	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140	Recovery	=	102.000%	
41) Toluene-d8	7.317	98	159957	4.519	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	90.400%	
43) trans-1,3-Dichloroprop...	7.625	79	16131	4.512	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130	Recovery	=	90.200%	
46) 2-Hexanone-d5	8.091	63	62280	49.635	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130	Recovery	=	99.260%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	34092	5.073	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120	Recovery	=	101.400%	
66) 1,2-Dichlorobenzene-d4	11.622	152	54408	5.066	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120	Recovery	=	101.400%	
Target Compounds						
					Qvalue	
22) cis-1,2-Dichloroethene	3.921	96	1781m	0.174	ug/L	
25) Chloroform	4.381	83	5532	0.317	ug/L	86
34) Trichloroethene	5.911	95	59826	5.786	ug/L	99
47) Tetrachloroethene	7.976	164	20140	2.488	ug/L	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041122\
Data File : VV025449.D
Acq On : 11 Apr 2022 14:49
Operator : SY/MD
Sample : N2319-17DL 5X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YB2K4DL

Manual IntegrationsAPPROVED

Quant Time: Apr 12 07:06:16 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Apr 12 07:03:45 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 04/12/2022
Supervised By :Mahesh Dadoda 04/15/2022

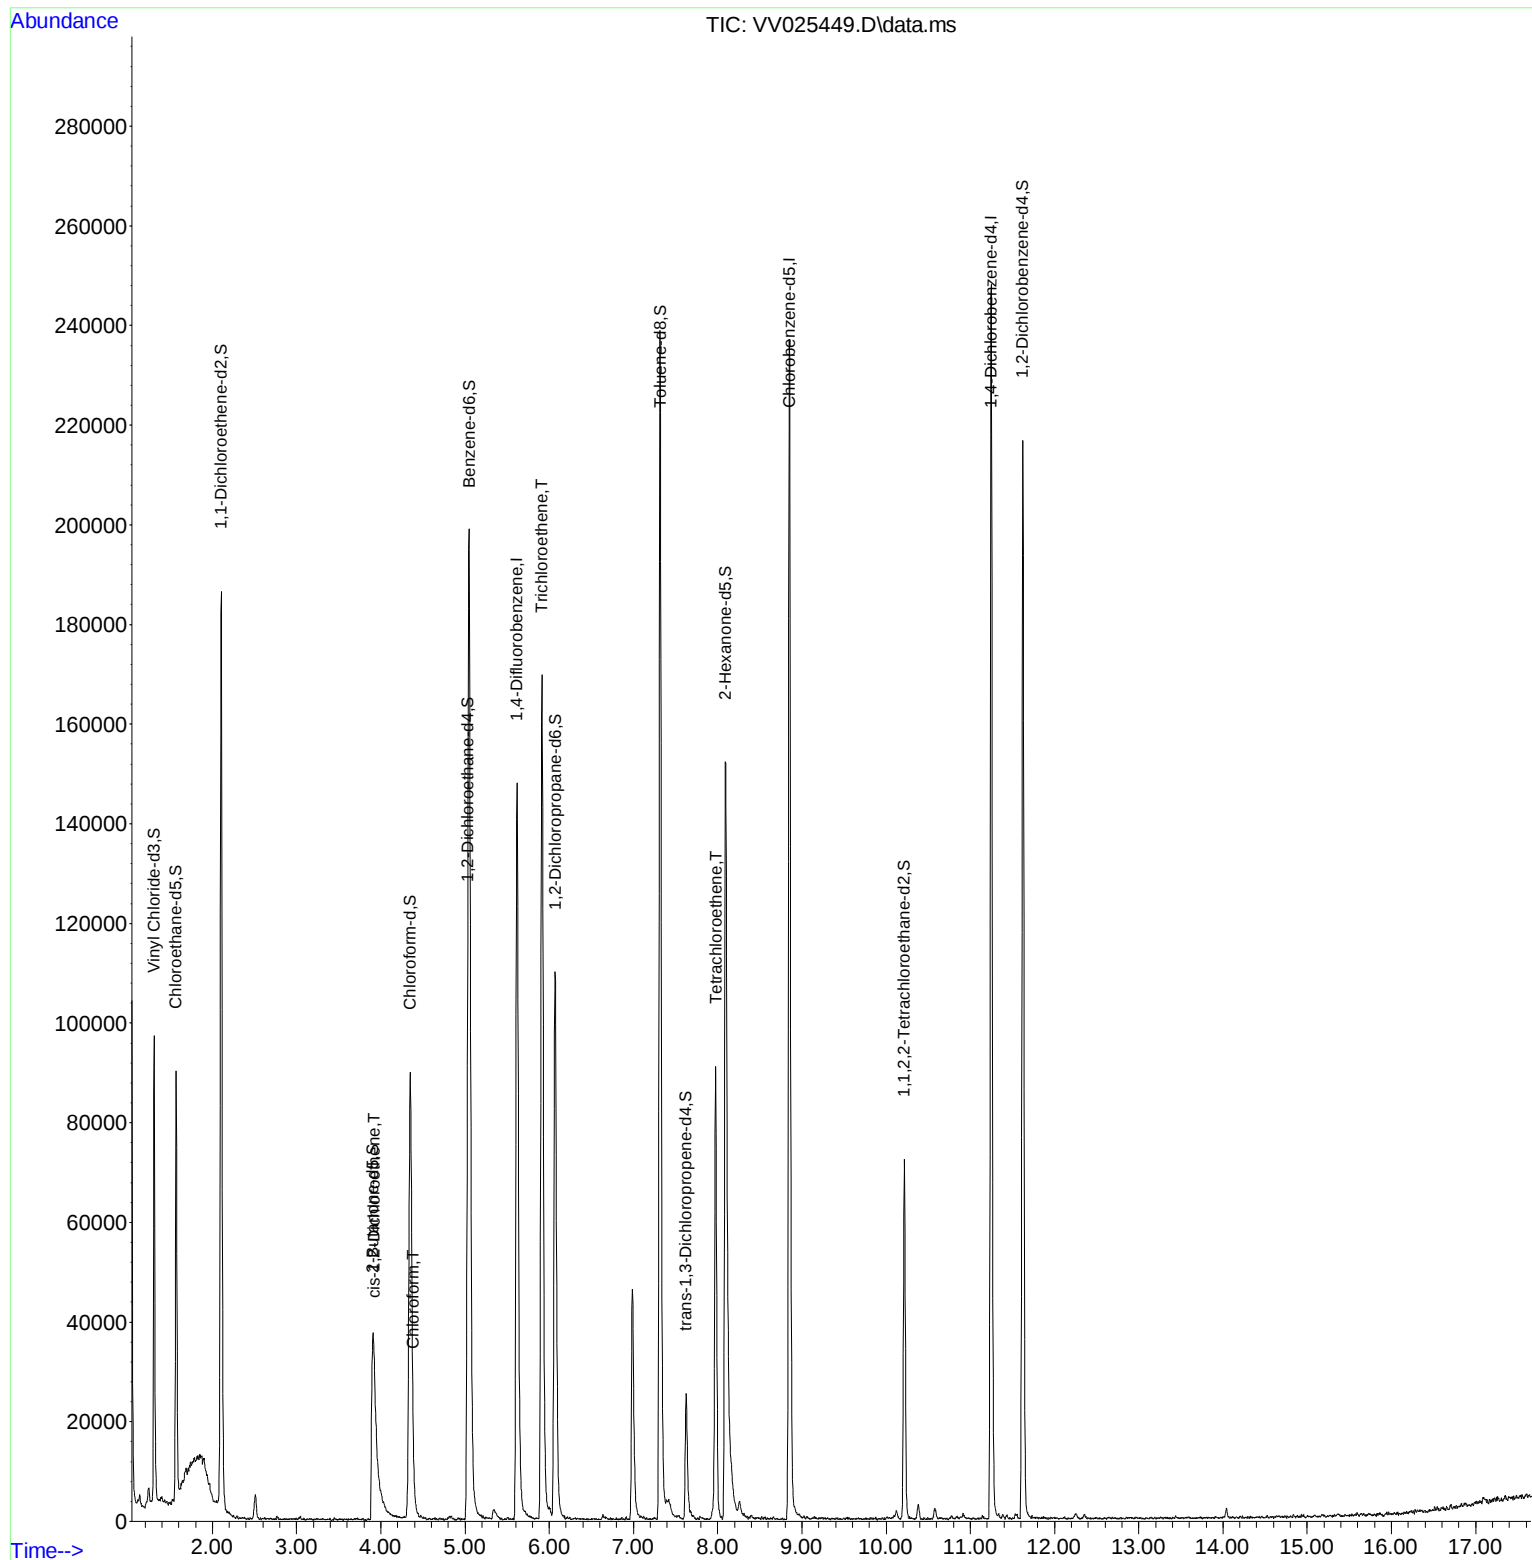




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041122\
 Data File : VV025449.D
 Acq On : 11 Apr 2022 14:49
 Operator : SY/MD
 Sample : N2319-17DL 5X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YB2K4DL

Manual IntegrationsAPPROVED

Quant Time: Apr 12 07:06:16 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Apr 12 07:03:45 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 04/12/2022
 Supervised By :Mahesh Dadoda 04/15/2022

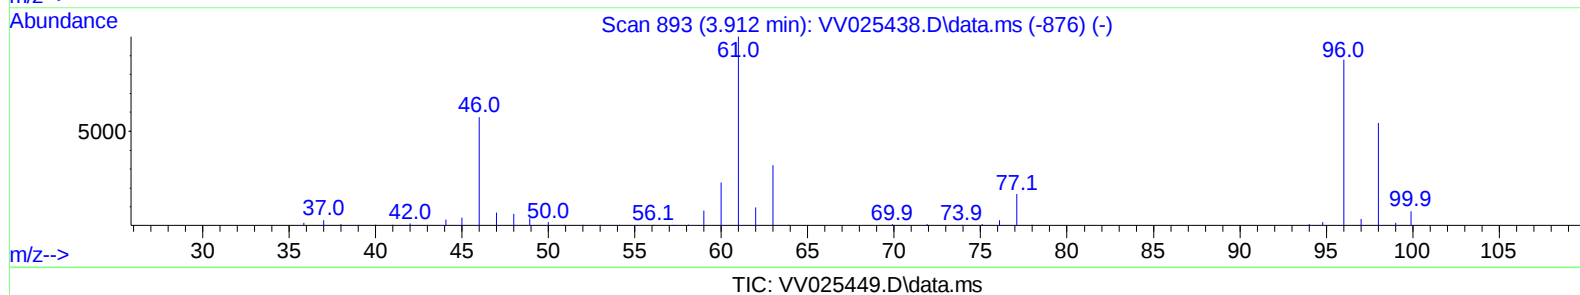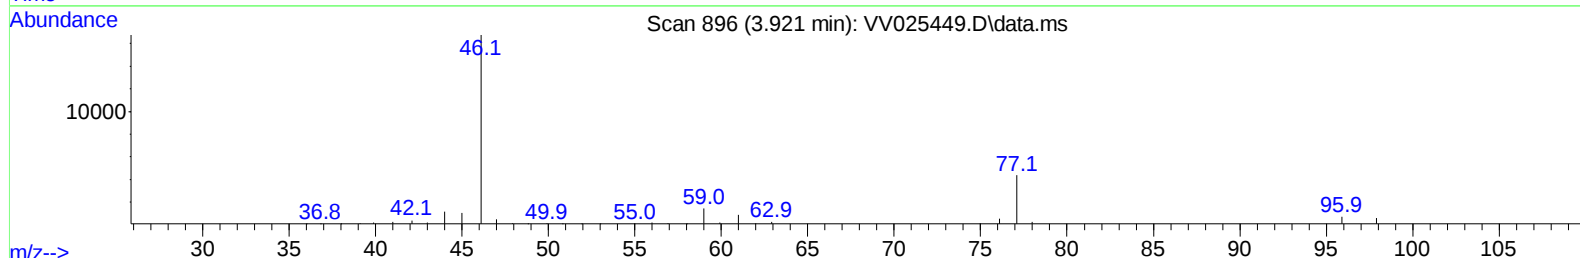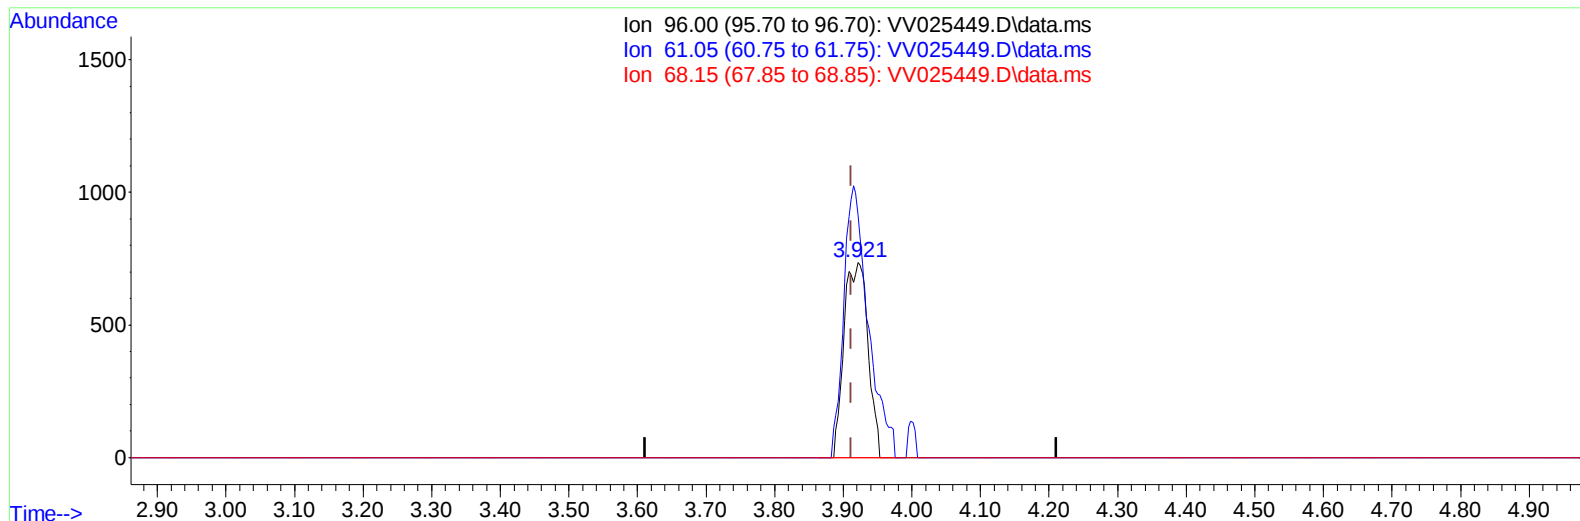

(22) cis-1,2-Dichloroethene (T)

3.921min (+ 0.010) 0.17 ug/L m

response 1781

Ion	Exp%	Act%
96.00	100.00	100.00
61.05	114.30	124.32
68.15	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041122\
 Data File : VV025449.D
 Acq On : 11 Apr 2022 14:49
 Operator : SY/MD
 Sample : N2319-17DL 5X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YB2K4DL

Manual IntegrationsAPPROVED

Quant Time: Apr 12 07:06:16 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Apr 12 07:03:45 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 04/12/2022
 Supervised By :Mahesh Dadoda 04/15/2022

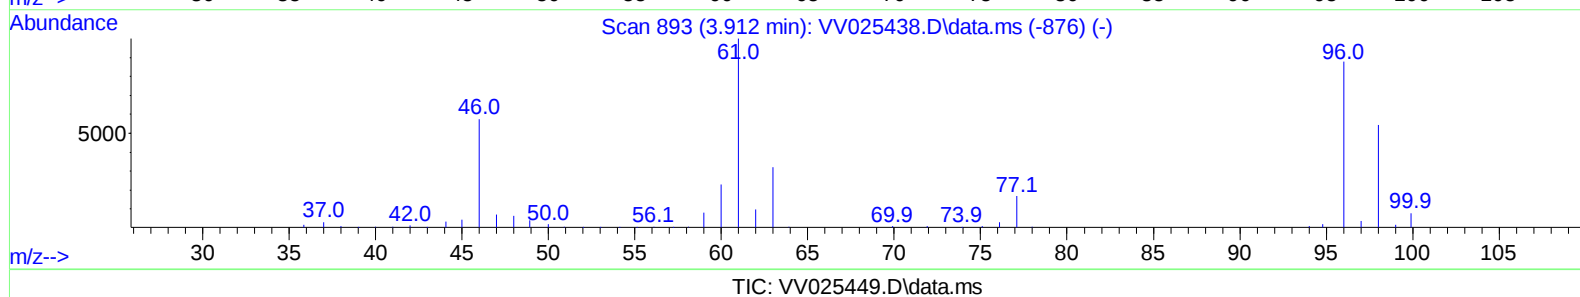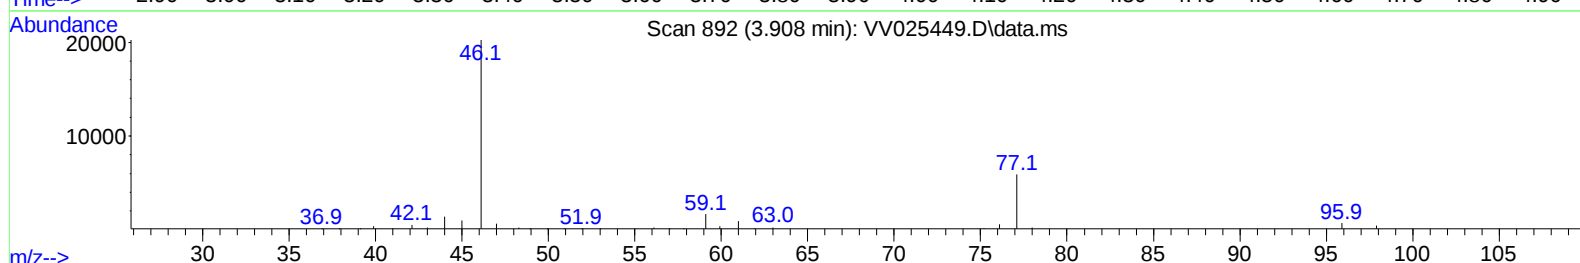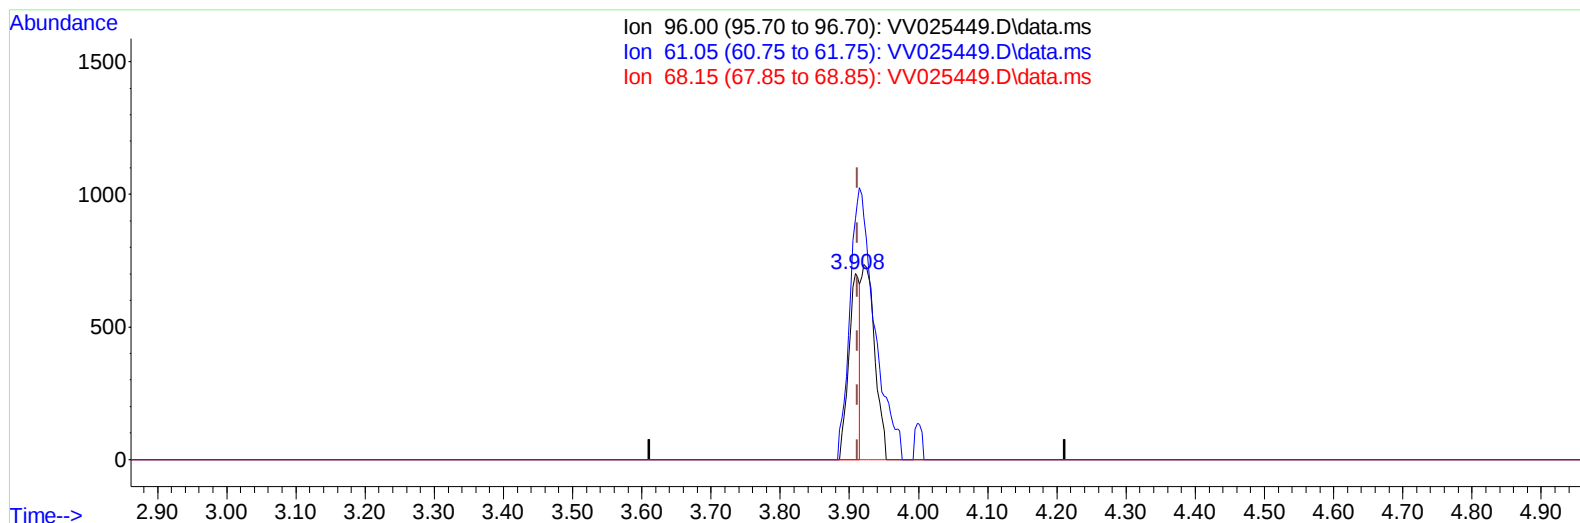

(22) cis-1,2-Dichloroethene (T)

3.908min (-0.003) 0.08 ug/L

response 790

Ion	Exp%	Act%
96.00	100.00	100.00
61.05	114.30	129.81
68.15	0.00	0.00
0.00	0.00	0.00