

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041122\
 Data File : VV025456.D
 Acq On : 11 Apr 2022 17:33
 Operator : SY/MD
 Sample : N2357-01
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 Y0AA0

Manual IntegrationsAPPROVED

Quant Time: Apr 12 07:07:50 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Apr 12 07:03:45 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 04/15/2022
 Supervised By :Mahesh Dadoda 04/15/2022

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)
-----04/15/2022							
Supervised By :Mahesh Dadoda							
Internal Standards							
1) 1,4-Difluorobenzene	5.619	114		125609	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117		127776	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152		60126	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.310	65		58540	5.013	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	100.200%	
7) Chloroethane-d5	1.571	69		54318	4.372	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	87.400%	
11) 1,1-Dichloroethene-d2	2.111	63		88277	3.774	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	75.400%	
20) 2-Butanone-d5	3.899	46		74137	52.190	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	104.380%	
24) Chloroform-d	4.349	84		88022	4.988	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.800%	
26) 1,2-Dichloroethane-d4	5.034	65		42645	5.609	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	112.200%	
32) Benzene-d6	5.053	84		175319	4.742	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.800%	
36) 1,2-Dichloropropane-d6	6.069	67		52509	5.093	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	101.800%	
41) Toluene-d8	7.316	98		150117	4.375	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	87.600%	
43) trans-1,3-Dichloroprop...	7.625	79		15127	4.365	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	87.200%	
46) 2-Hexanone-d5	8.088	63		53349	43.862	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	87.720%	
56) 1,1,2,2-Tetrachloroeth...	10.213	84		30262	4.646	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	93.000%	
66) 1,2-Dichlorobenzene-d4	11.622	152		50605	5.020	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	100.400%	
Target Compounds							
25) Chloroform	4.374	83		2010m	0.123	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041122\
Data File : VV025456.D
Acq On : 11 Apr 2022 17:33
Operator : SY/MD
Sample : N2357-01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
Y0AA0

Manual IntegrationsAPPROVED

Quant Time: Apr 12 07:07:50 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Apr 12 07:03:45 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 04/15/2022
Supervised By :Mahesh Dadoda 04/15/2022

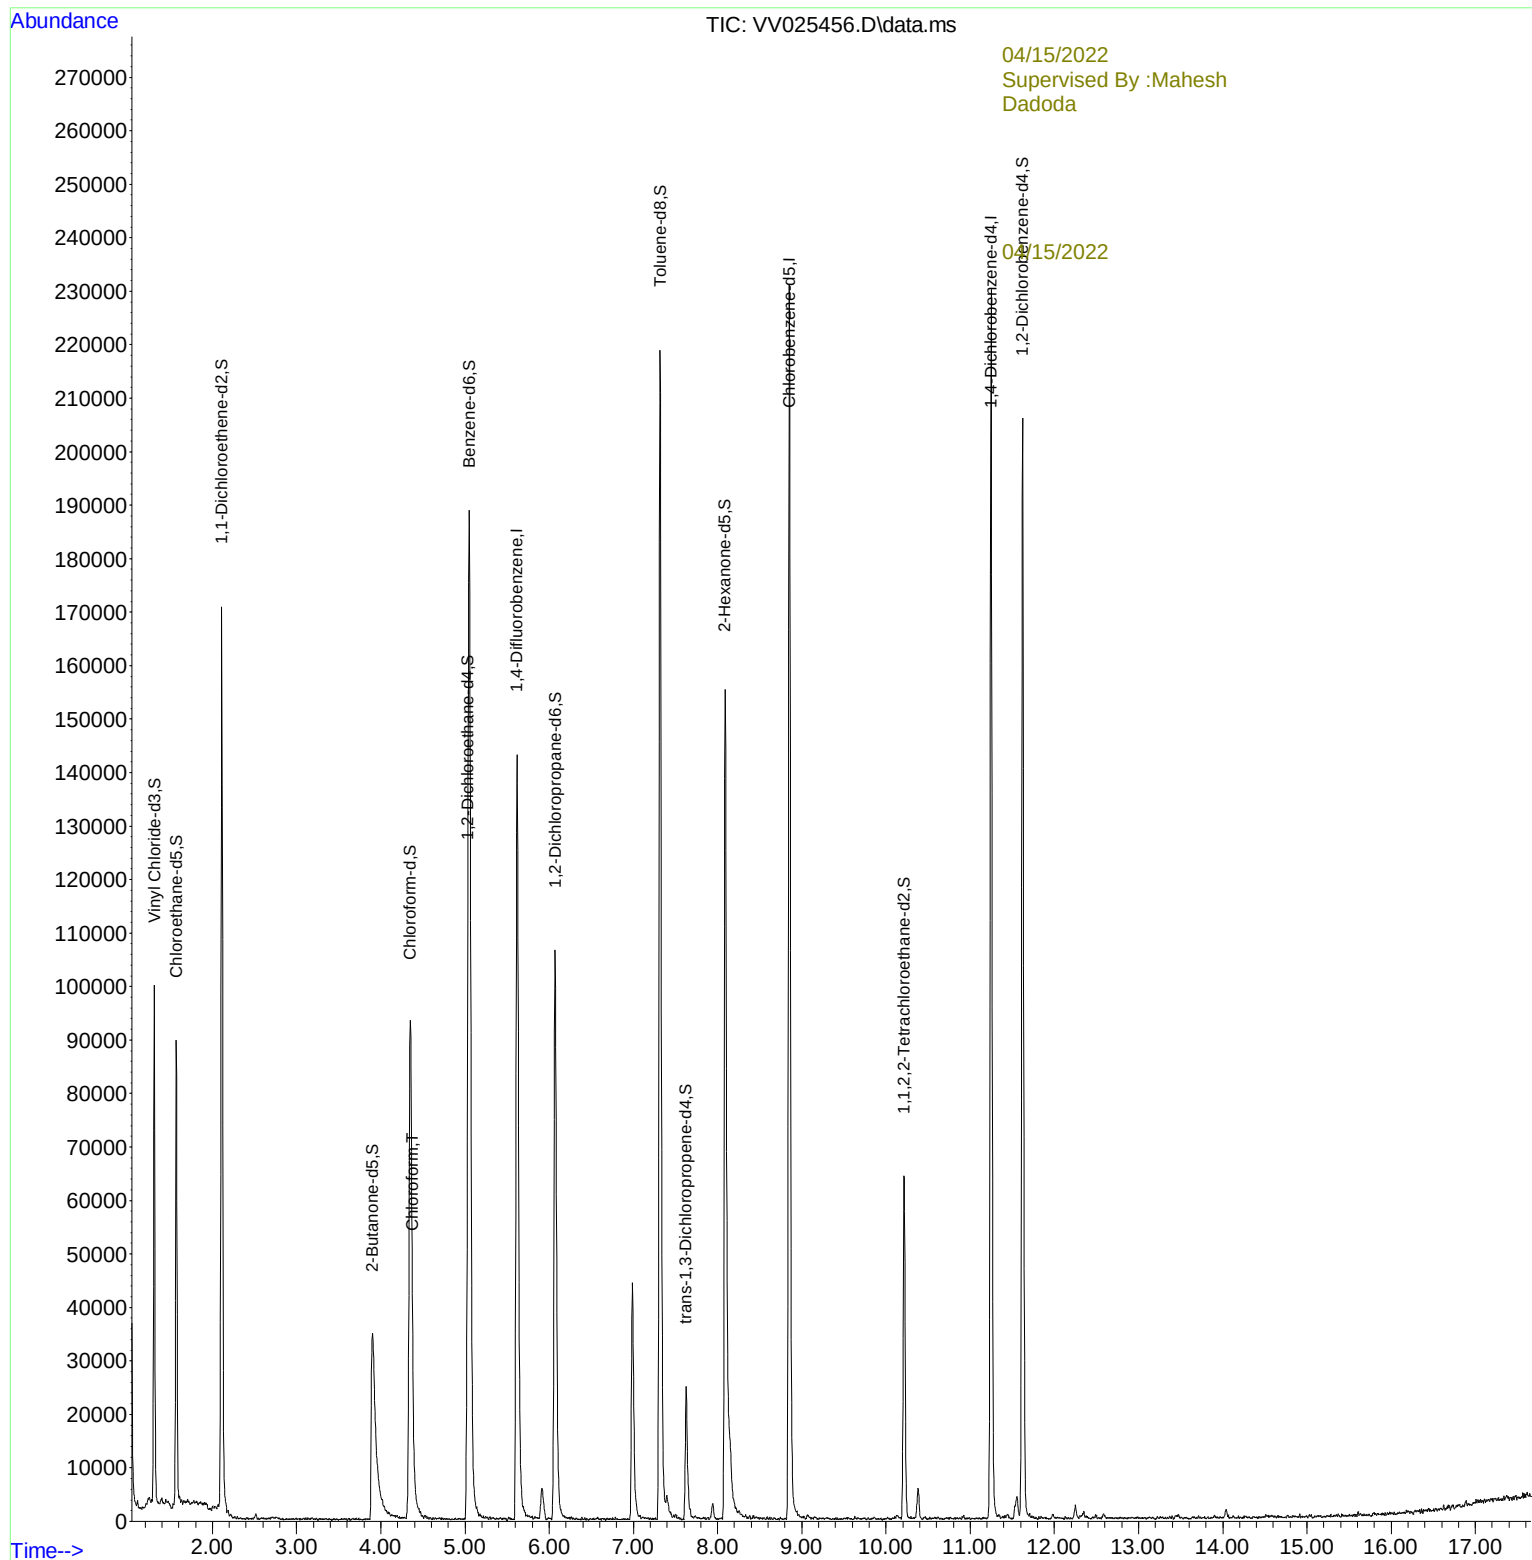




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041122\
 Data File : VV025456.D
 Acq On : 11 Apr 2022 17:33
 Operator : SY/MD
 Sample : N2357-01
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 Y0AA0

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 04/15/2022
 Supervised By :Mahesh Dadoda 04/15/2022

Quant Time: Apr 12 07:07:50 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Apr 12 07:03:45 2022
 Response via : Initial Calibration

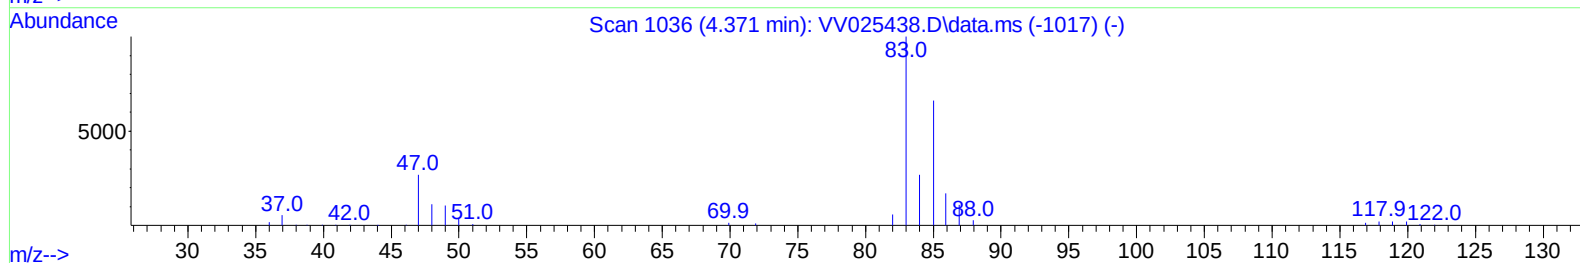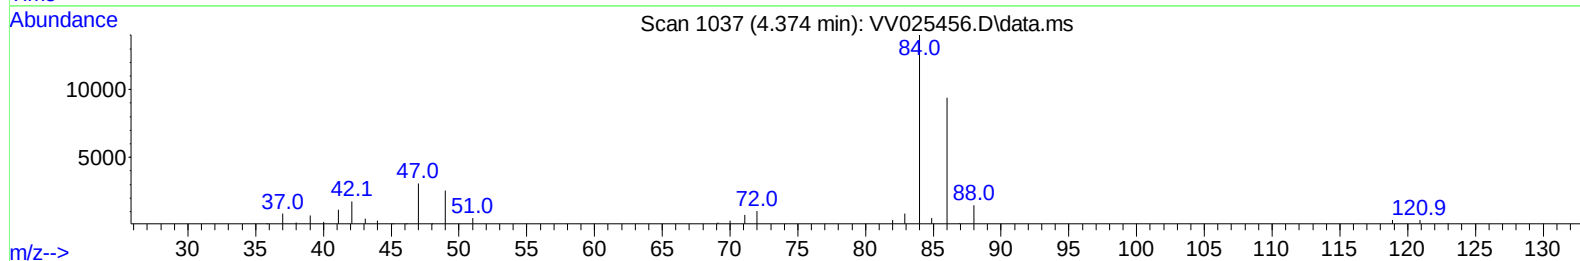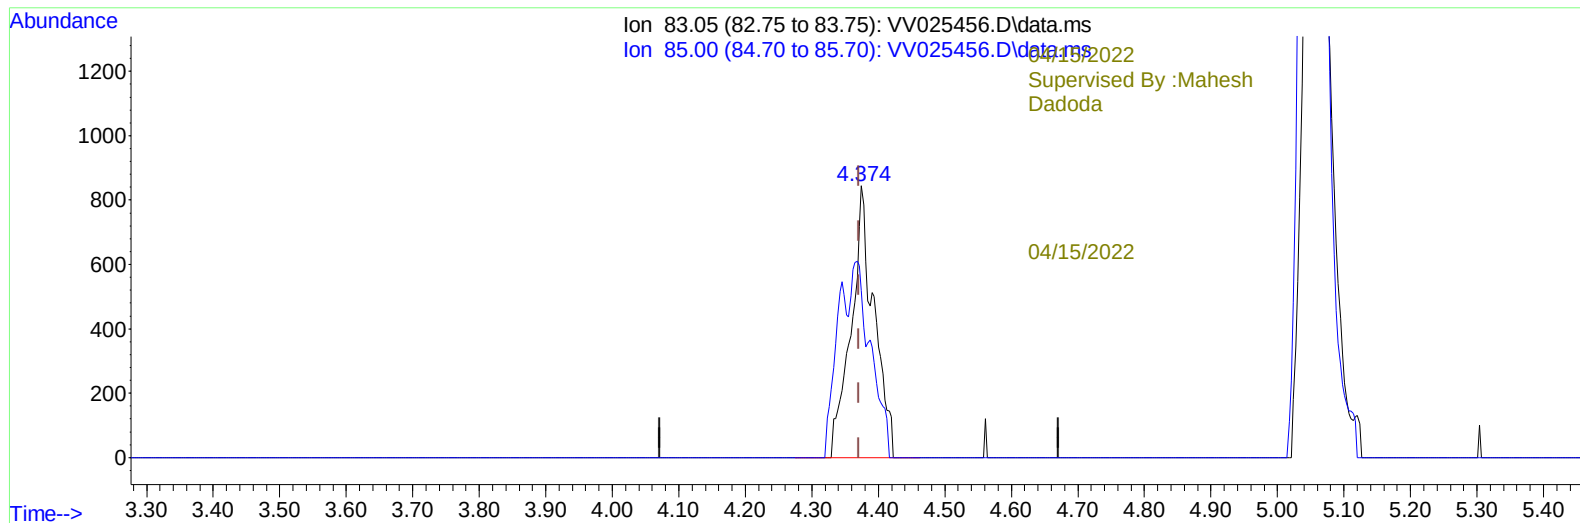

TIC: VV025456.D\data.ms

(25) Chloroform (T)

4.374min (+ 0.003) 0.12 ug/L m

response 2010

Ion	Exp%	Act%
83.05	100.00	100.00
85.00	62.10	61.49
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041122\
 Data File : VV025456.D
 Acq On : 11 Apr 2022 17:33
 Operator : SY/MD
 Sample : N2357-01
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 Y0AA0

Manual IntegrationsAPPROVED

Quant Time: Apr 12 07:07:50 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Apr 12 07:03:45 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 04/15/2022
 Supervised By :Mahesh Dadoda 04/15/2022

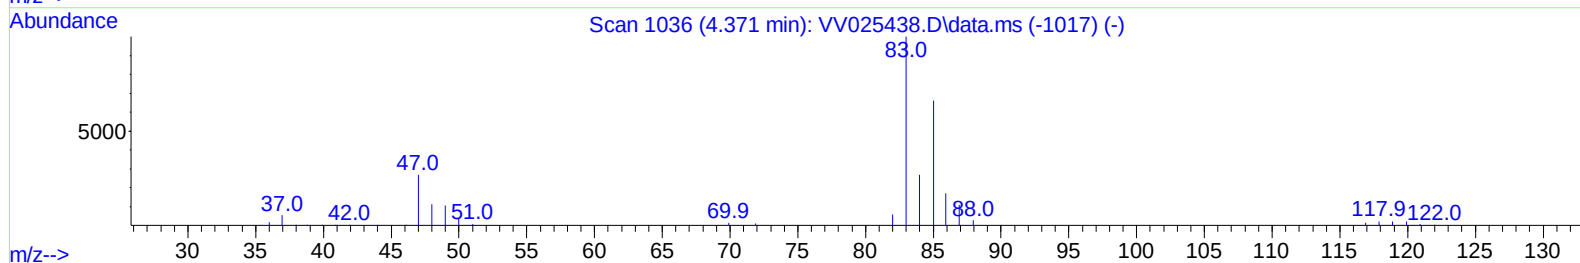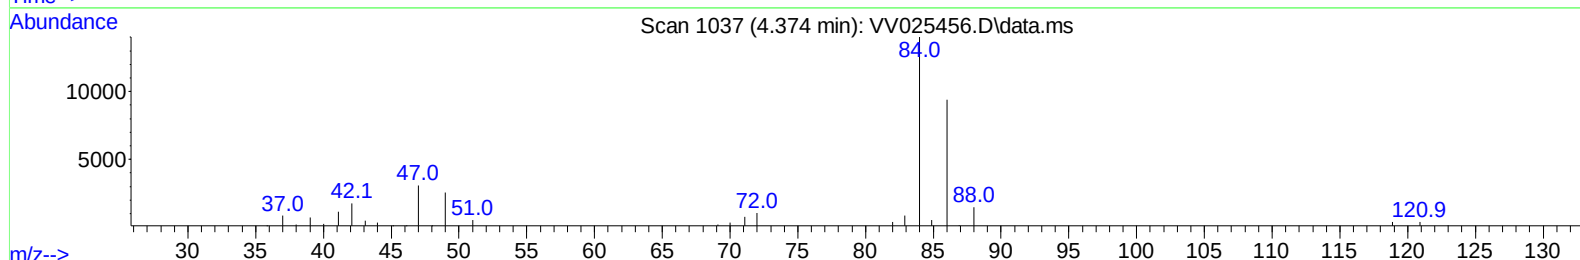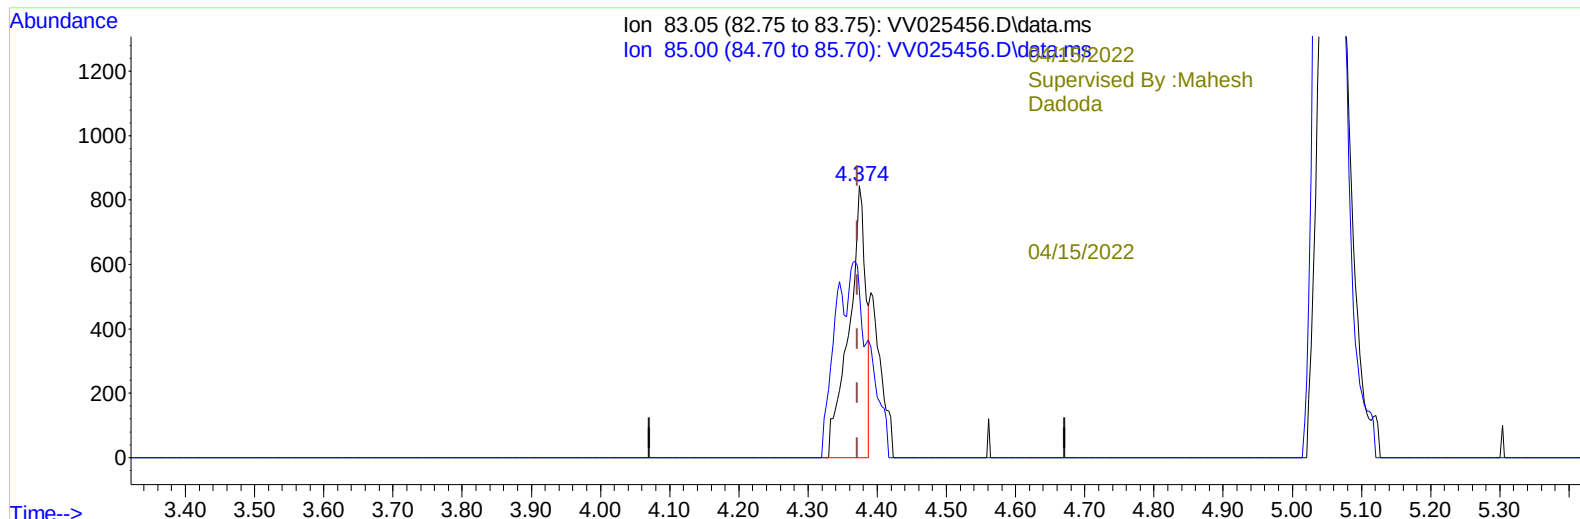

TIC: VV025456.D\data.ms

(25) Chloroform (T)

4.374min (+ 0.003) 0.09 ug/L

response 1442

Ion	Exp%	Act%
83.05	100.00	100.00
85.00	62.10	61.49
0.00	0.00	0.00
0.00	0.00	0.00