

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW041122\
 Data File : VW025460.D
 Acq On : 11 Apr 2022 19:06
 Operator : SY/MD
 Sample : N2357-04
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YAYW6

Quant Time: Apr 12 07:08:40 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Apr 12 07:03:45 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	122404	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	125689	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	56366	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	56015	4.922	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	98.400%
7) Chloroethane-d5	1.571	69	53303	4.403	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	88.000%
11) 1,1-Dichloroethene-d2	2.111	63	87499	3.838	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	76.800%
20) 2-Butanone-d5	3.899	46	73516	53.108	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	106.220%
24) Chloroform-d	4.352	84	87787	5.105	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	102.000%
26) 1,2-Dichloroethane-d4	5.037	65	40711	5.494	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	109.800%
32) Benzene-d6	5.053	84	171398	4.713	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.200%
36) 1,2-Dichloropropane-d6	6.069	67	51246	5.053	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	101.000%
41) Toluene-d8	7.317	98	143729	4.259	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	85.200%
43) trans-1,3-Dichloroprop...	7.625	79	13854	4.064	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	81.200%
46) 2-Hexanone-d5	8.088	63	56486	47.212	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	94.420%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	32368	5.052	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	101.000%
66) 1,2-Dichlorobenzene-d4	11.625	152	50186	5.310	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	106.200%
Target Compounds					Qvalue	
25) Chloroform	4.375	83	1495	0.094	ug/L	# 73


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041122\
Data File : VV025460.D
Acq On : 11 Apr 2022 19:06
Operator : SY/MD
Sample : N2357-04
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YAYW6

Quant Time: Apr 12 07:08:40 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Apr 12 07:03:45 2022
Response via : Initial Calibration

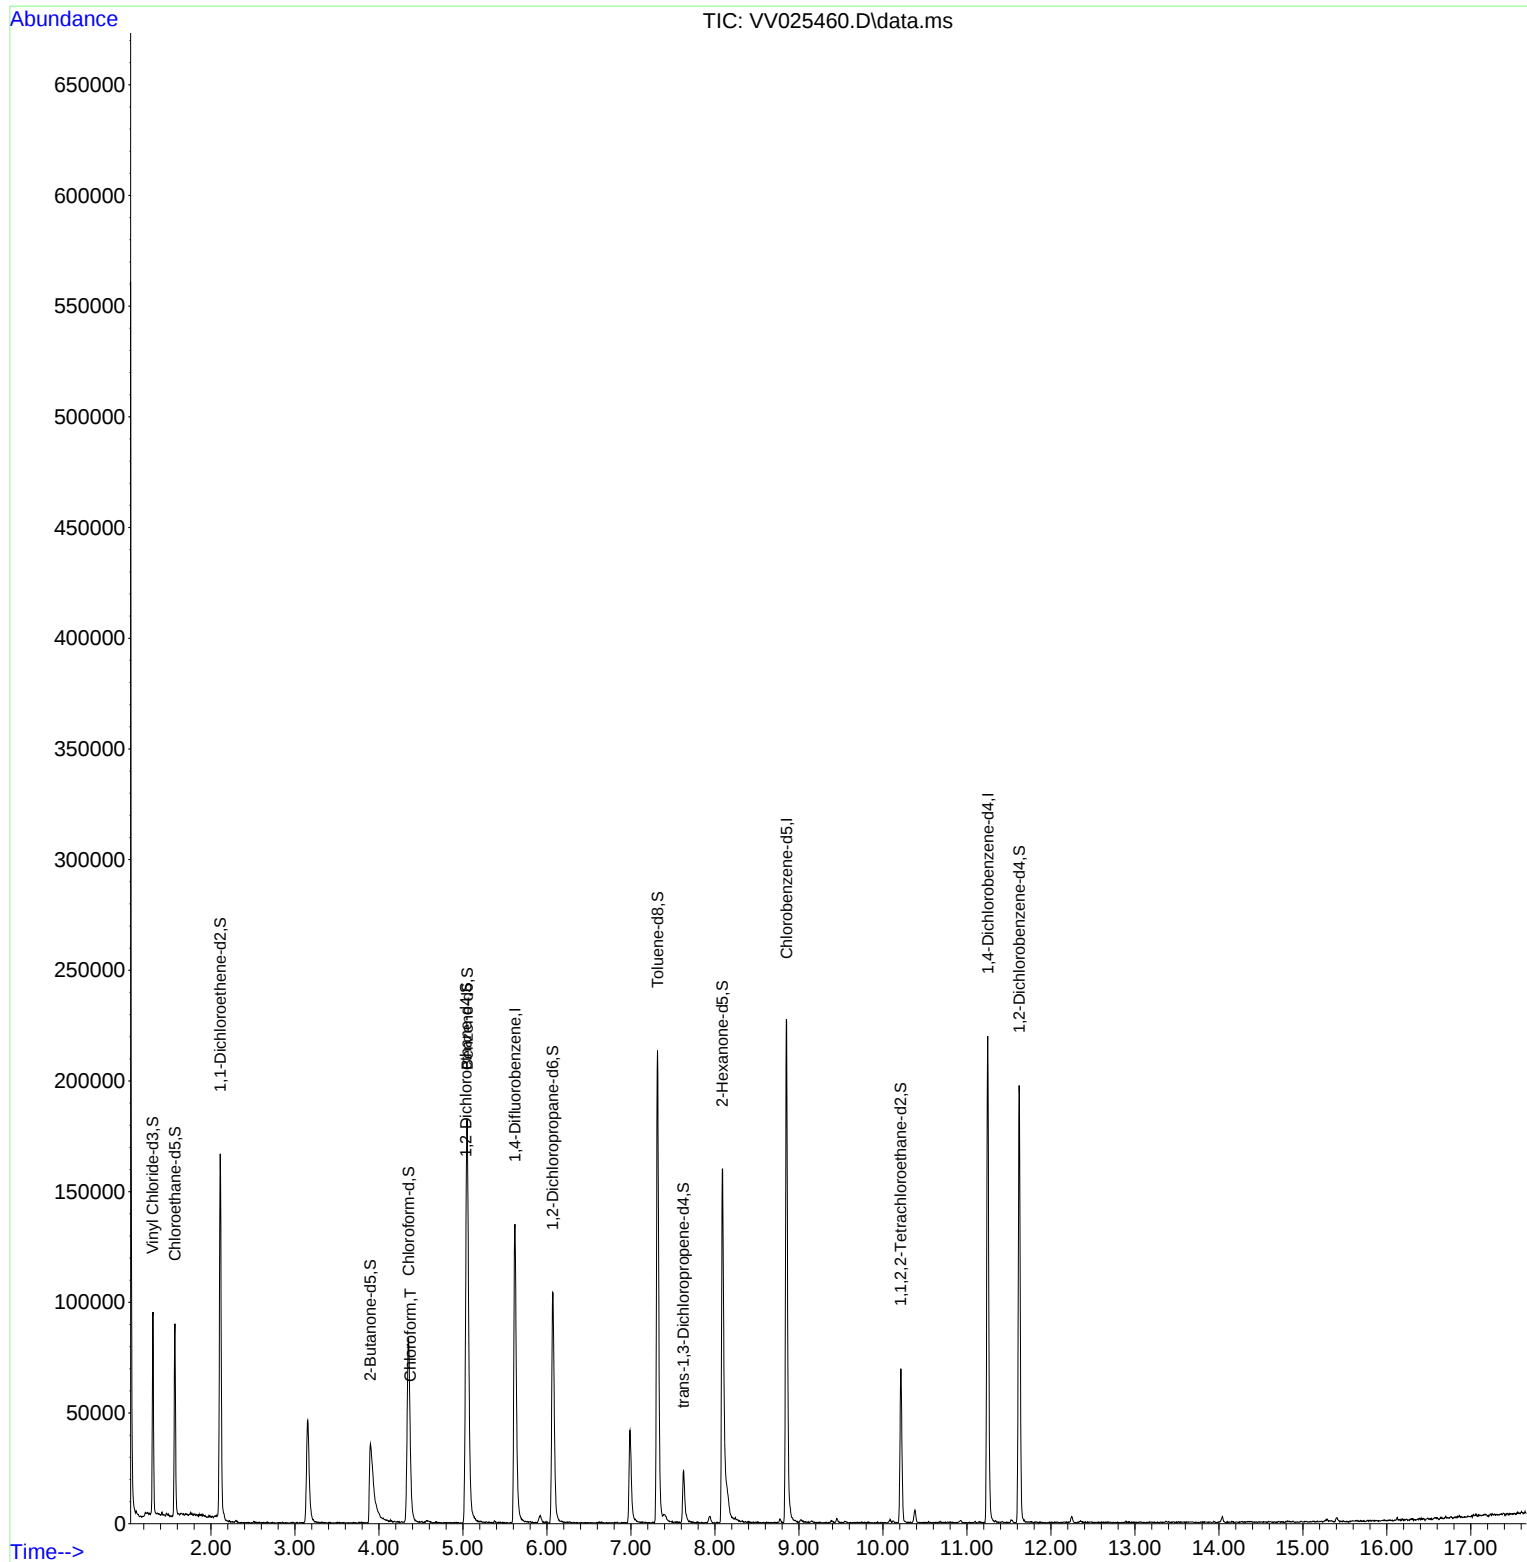

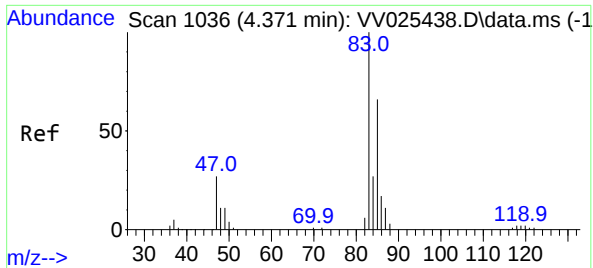

#25
Chloroform
Concen: 0.094 ug/L
RT: 4.375 min Scan# 10
Delta R.T. 0.003 min
Lab File: VV025460.D
Acq: 11 Apr 2022 19:06

Instrument :
MSVOA_V
ClientSampleId :
YAYW6

Tgt Ion: 83 Resp: 1495
Ion Ratio Lower Upper
83 100
85 83.0 43.5 80.7#

