

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041122\
 Data File : VV025441.D
 Acq On : 11 Apr 2022 11:41
 Operator : SY/MD
 Sample : N2319-02DL 10X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YB2G9DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV025441.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	100	rVB	116740	117796	20.28%	2.302%
2	1.571	157	165	179	rVB	104961	118815	20.46%	2.322%
3	2.111	322	333	348	rVB	210796	312951	53.88%	6.117%
4	3.896	877	888	917	rBV	46889	162667	28.00%	3.179%
5	4.352	1014	1030	1062	rBV	104816	265881	45.77%	5.197%
6	5.050	1229	1247	1271	rBV2	233681	580852	100.00%	11.353%
7	5.616	1412	1423	1446	rBV	178565	368167	63.38%	7.196%
8	5.915	1504	1516	1534	rBV2	169126	337306	58.07%	6.593%
9	6.069	1552	1564	1594	rVB	128096	266803	45.93%	5.215%
10	6.989	1840	1850	1871	rBV	57099	108517	18.68%	2.121%
11	7.317	1938	1952	1971	rBV	278077	494393	85.12%	9.663%
12	7.625	2038	2048	2067	rBV	32560	59434	10.23%	1.162%
13	7.979	2149	2158	2173	rVB3	20388	36536	6.29%	0.714%
14	8.088	2178	2192	2228	rBV	198512	398695	68.64%	7.793%
15	8.850	2418	2429	2457	rBV	292775	481259	82.85%	9.406%
16	10.214	2841	2853	2868	rBV2	82390	131418	22.63%	2.569%
17	10.381	2897	2905	2914	rVB2	5107	6945	1.20%	0.136%
18	11.246	3163	3174	3196	rBV	301376	460992	79.36%	9.010%
19	11.622	3279	3291	3314	rBV	254284	399438	68.77%	7.807%
20	12.345	3509	3516	3525	rBV7	5181	7415	1.28%	0.145%




Sum of corrected areas: 5116280

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041122\
Data File : VV025441.D
Acq On : 11 Apr 2022 11:41
Operator : SY/MD
Sample : N2319-02DL 10X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YB2G9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

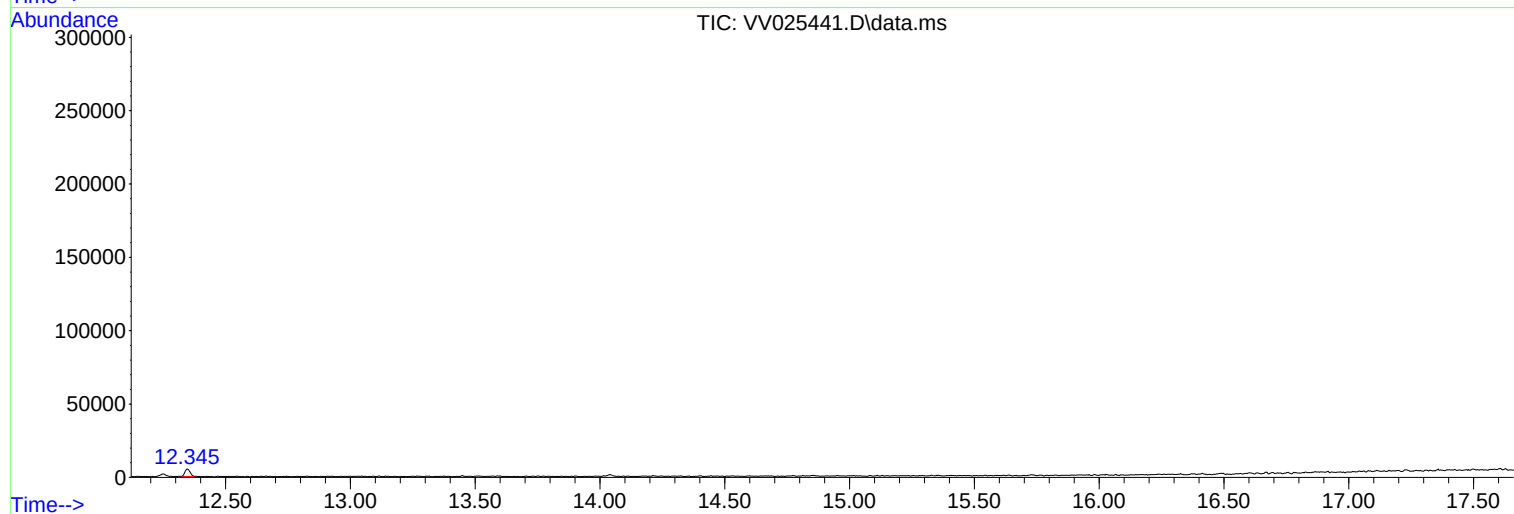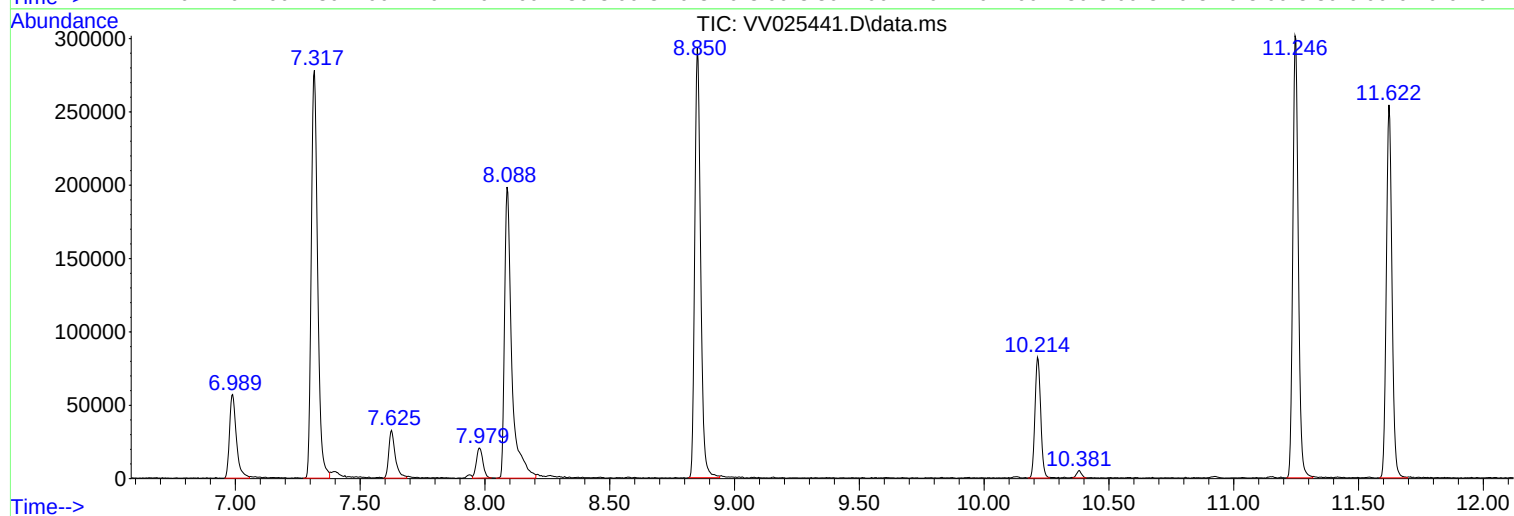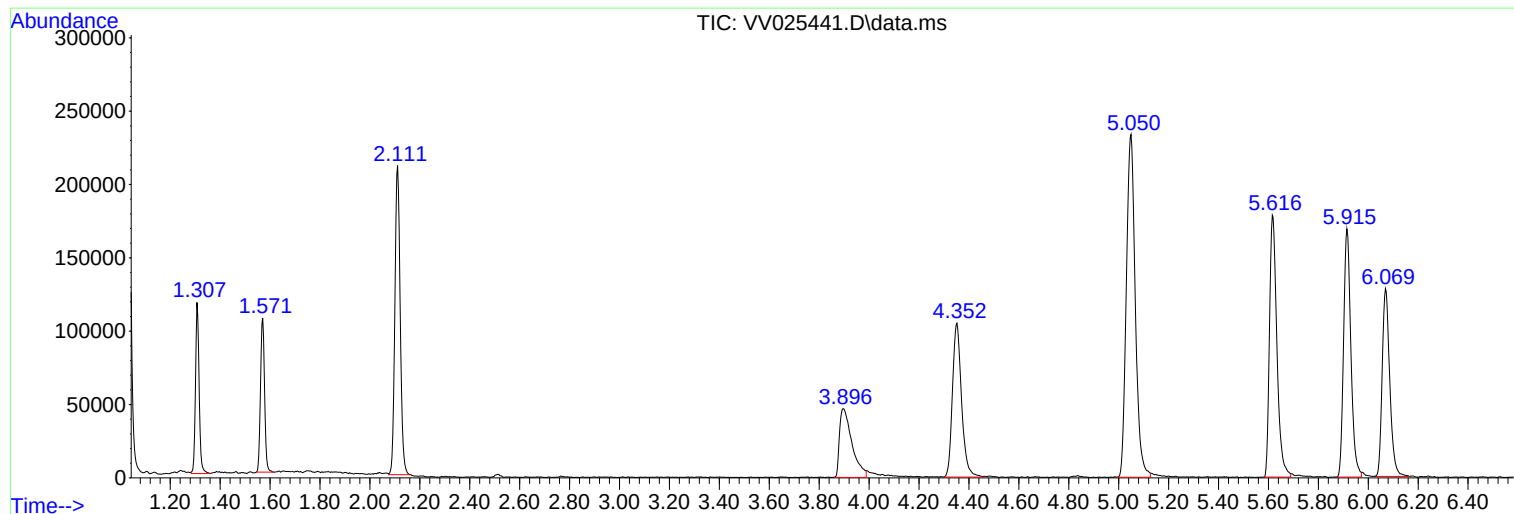

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041122\
Data File : VV025441.D
Acq On : 11 Apr 2022 11:41
Operator : SY/MD
Sample : N2319-02DL 10X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YB2G9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041122\
Data File : VV025441.D
Acq On : 11 Apr 2022 11:41
Operator : SY/MD
Sample : N2319-02DL 10X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YB2G9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc