

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041122\
 Data File : VV025443.D
 Acq On : 11 Apr 2022 12:28
 Operator : SY/MD
 Sample : N2319-03DL 10X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YB2H0DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV025443.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	102	rVB	103450	105749	19.79%	2.244%
2	1.568	156	164	176	rBV	97355	114020	21.33%	2.420%
3	2.111	322	333	359	rVB	194901	297069	55.58%	6.304%
4	3.899	875	889	927	rBV	43028	157556	29.48%	3.344%
5	4.349	1014	1029	1057	rBV	93548	239065	44.73%	5.073%
6	5.050	1229	1247	1280	rBV2	213541	534443	100.00%	11.342%
7	5.619	1412	1424	1451	rBV	163611	341200	63.84%	7.241%
8	5.915	1504	1516	1540	rBV	158812	323221	60.48%	6.859%
9	6.069	1551	1564	1591	rBV	116881	246267	46.08%	5.226%
10	6.989	1840	1850	1871	rBV2	49757	98166	18.37%	2.083%
11	7.317	1939	1952	1969	rBV	257874	448132	83.85%	9.510%
12	7.625	2032	2048	2066	rBV	28907	53367	9.99%	1.133%
13	7.976	2148	2157	2172	rVB2	19428	34505	6.46%	0.732%
14	8.088	2183	2192	2231	rBV	181014	370171	69.26%	7.855%
15	8.850	2418	2429	2446	rBV	265910	434565	81.31%	9.222%
16	10.214	2840	2853	2871	rBV2	76475	122356	22.89%	2.597%
17	11.249	3163	3175	3195	rBV	266750	418502	78.31%	8.881%
18	11.622	3280	3291	3315	rBV	234757	367807	68.82%	7.805%
19	12.348	3509	3517	3525	rBV5	4472	6103	1.14%	0.130%




Sum of corrected areas: 4712264

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041122\
Data File : VV025443.D
Acq On : 11 Apr 2022 12:28
Operator : SY/MD
Sample : N2319-03DL 10X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YB2H0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

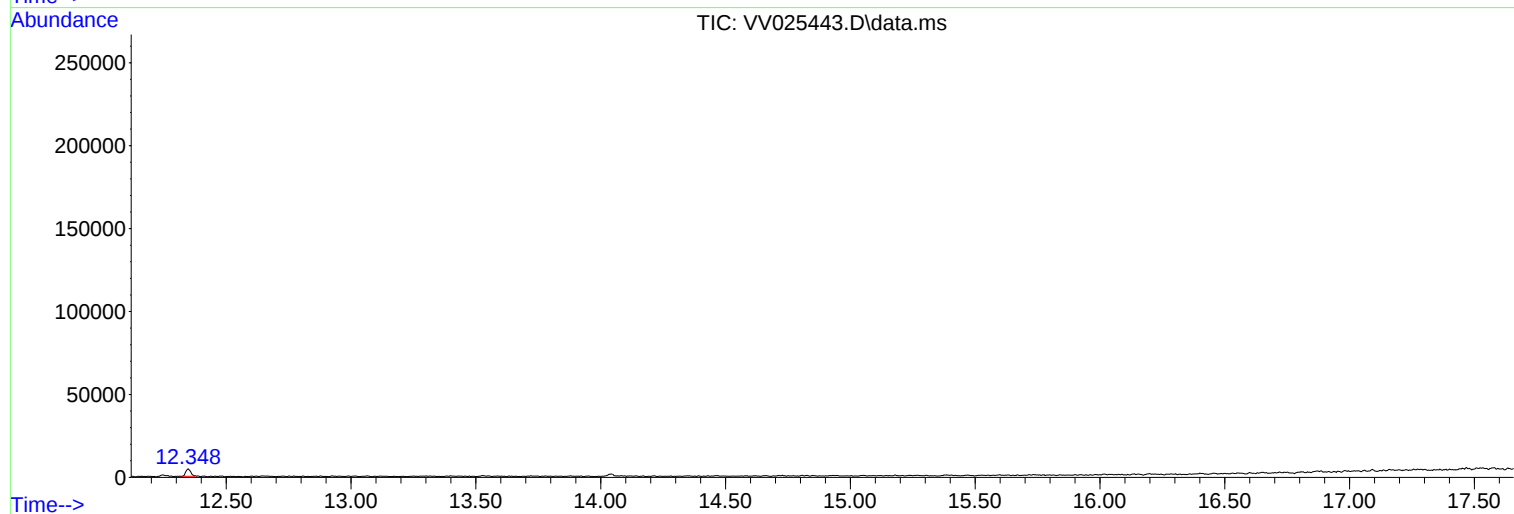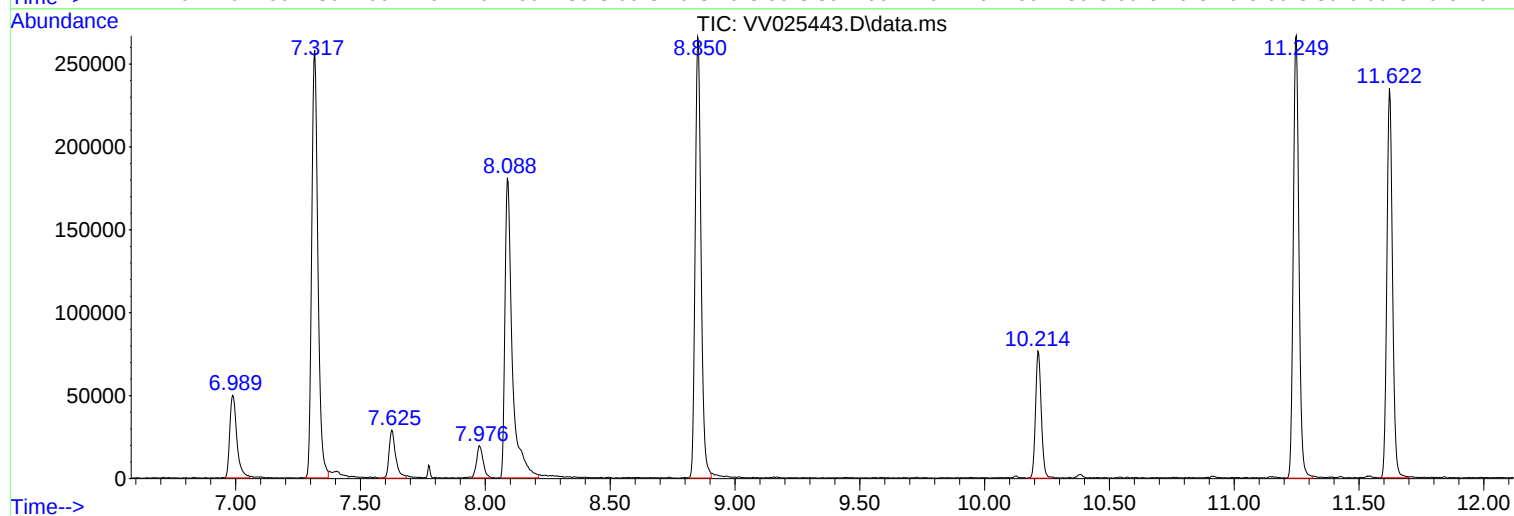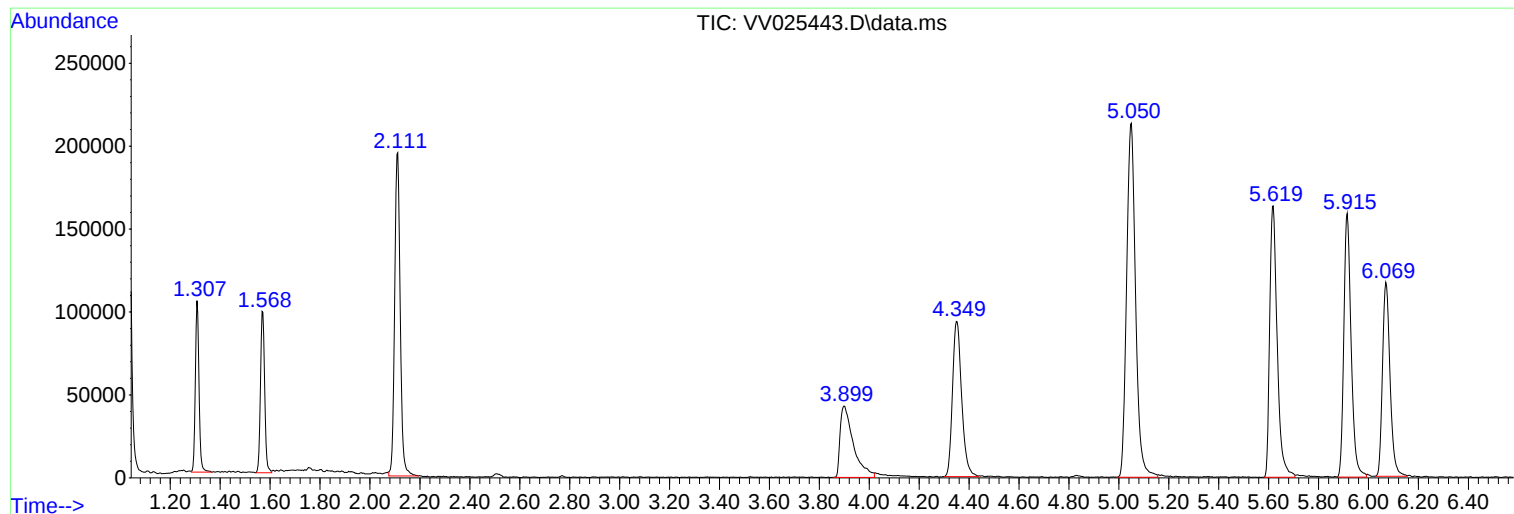

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041122\
Data File : VV025443.D
Acq On : 11 Apr 2022 12:28
Operator : SY/MD
Sample : N2319-03DL 10X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YB2H0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041122\
Data File : VV025443.D
Acq On : 11 Apr 2022 12:28
Operator : SY/MD
Sample : N2319-03DL 10X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YB2H0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc