

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041122\
 Data File : VV025445.D
 Acq On : 11 Apr 2022 13:15
 Operator : SY/MD
 Sample : N2319-06DL 10X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YB2H3DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV025445.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	94	rBV	106940	111558	19.73%	2.164%
2	1.571	156	165	175	rBV	100126	117075	20.71%	2.271%
3	2.108	316	332	353	rVB2	219245	334727	59.21%	6.493%
4	2.510	446	457	465	rBV5	3496	5980	1.06%	0.116%
5	3.905	879	891	931	rBV	42513	159354	28.19%	3.091%
6	4.349	1014	1029	1063	rVB	100332	255614	45.22%	4.959%
7	5.047	1229	1246	1277	rBV2	228520	565304	100.00%	10.966%
8	5.616	1411	1423	1451	rBV	170864	348276	61.61%	6.756%
9	5.915	1503	1516	1548	rBV	208614	426477	75.44%	8.273%
10	6.069	1551	1564	1592	rVB2	126511	264132	46.72%	5.124%
11	6.989	1840	1850	1873	rBV	54514	103694	18.34%	2.012%
12	7.317	1940	1952	1974	rBV	269914	480633	85.02%	9.324%
13	7.625	2038	2048	2064	rBV	30620	55095	9.75%	1.069%
14	7.976	2146	2157	2172	rBV	73472	123789	21.90%	2.401%
15	8.091	2182	2193	2232	rBV	195668	403627	71.40%	7.830%
16	8.850	2419	2429	2456	rBV	272277	449719	79.55%	8.724%
17	10.214	2841	2853	2868	rBV	80980	128172	22.67%	2.486%
18	11.246	3163	3174	3205	rBV	276549	434088	76.79%	8.421%
19	11.622	3277	3291	3314	rBV	246352	387628	68.57%	7.520%




Sum of corrected areas: 5154942

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041122\
Data File : VV025445.D
Acq On : 11 Apr 2022 13:15
Operator : SY/MD
Sample : N2319-06DL 10X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YB2H3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

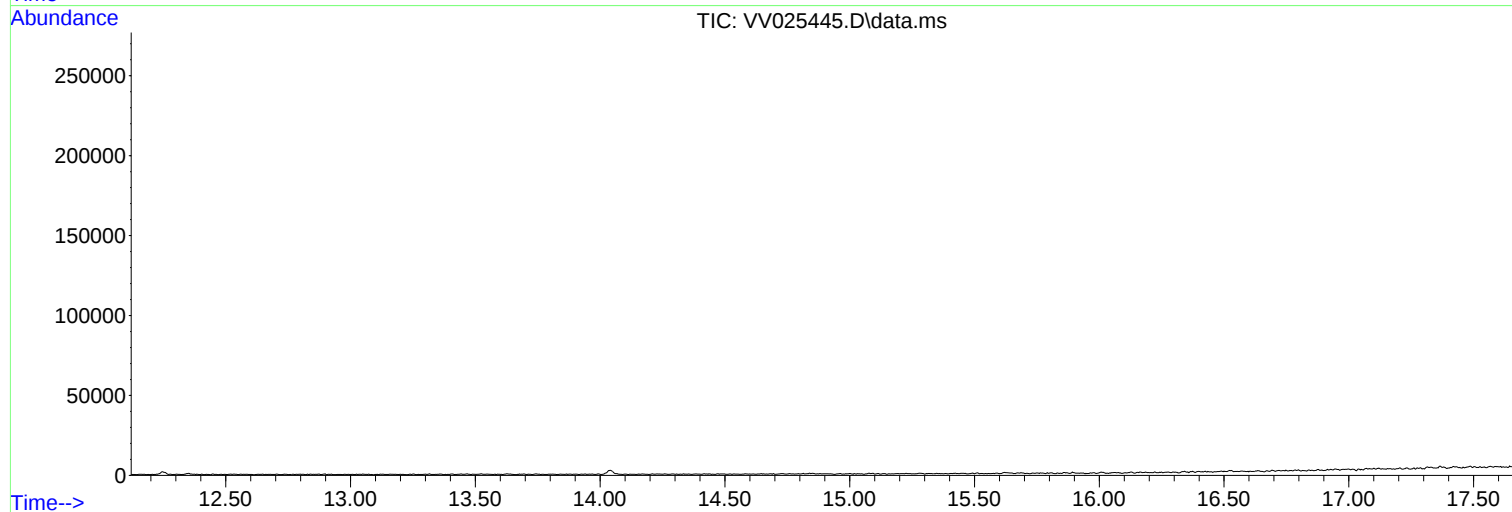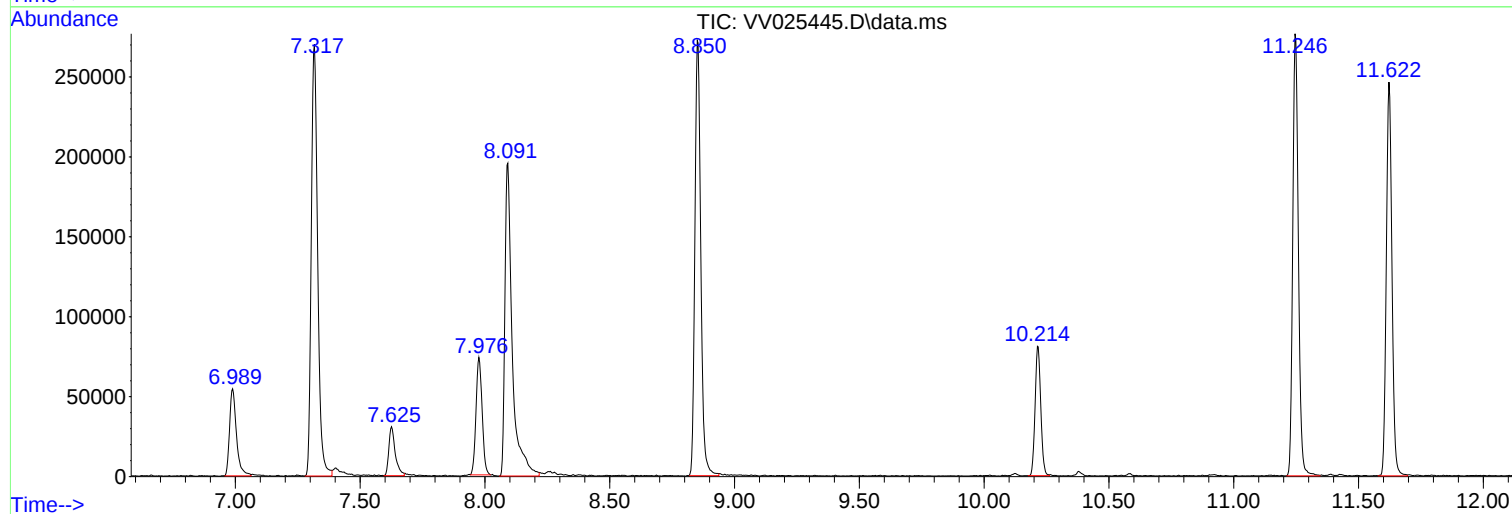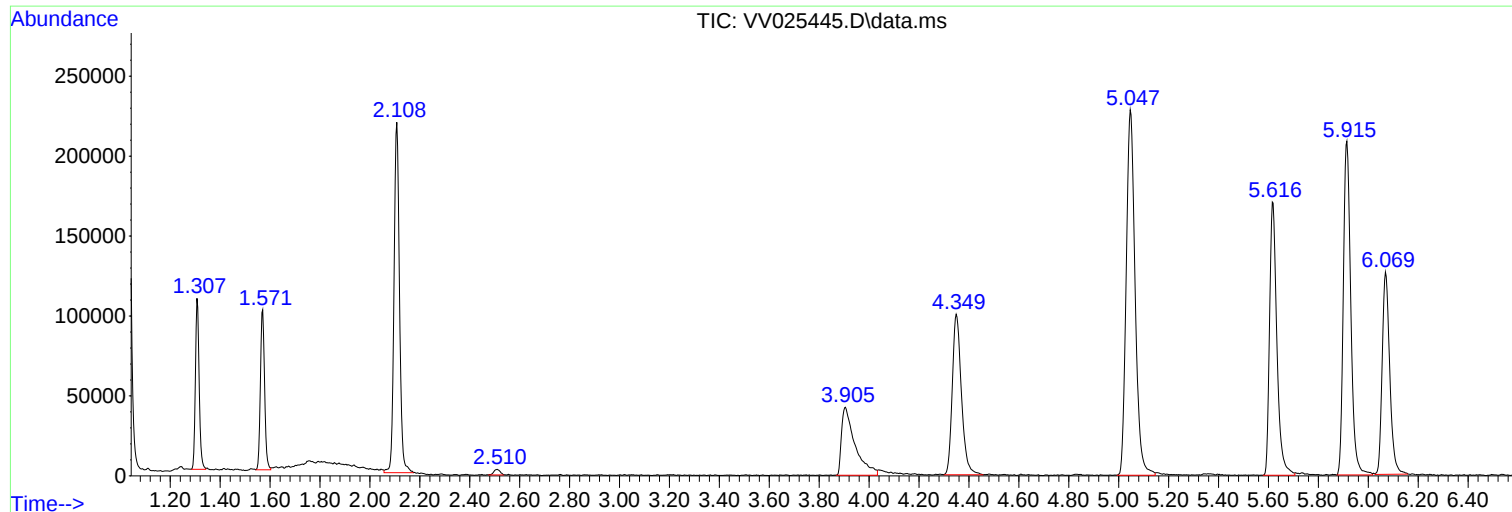

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041122\
Data File : VV025445.D
Acq On : 11 Apr 2022 13:15
Operator : SY/MD
Sample : N2319-06DL 10X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YB2H3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041122\
Data File : VV025445.D
Acq On : 11 Apr 2022 13:15
Operator : SY/MD
Sample : N2319-06DL 10X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YB2H3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc