

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041122\
 Data File : VV025446.D
 Acq On : 11 Apr 2022 13:39
 Operator : SY/MD
 Sample : N2319-11DL 10X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YB2H9DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV025446.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	101	rVB	95558	103619	20.73%	2.296%
2	1.571	156	165	174	rBV	91776	107178	21.44%	2.375%
3	2.105	321	331	346	rBV	179070	260421	52.09%	5.770%
4	2.507	449	456	467	rVB4	3471	5941	1.19%	0.132%
5	3.905	880	891	923	rBV	38903	140618	28.13%	3.116%
6	4.349	1012	1029	1052	rBV	88065	225814	45.17%	5.003%
7	5.047	1231	1246	1274	rBV2	200138	499898	100.00%	11.076%
8	5.616	1412	1423	1452	rBV	155536	321708	64.35%	7.128%
9	5.915	1501	1516	1536	rBV2	118050	241194	48.25%	5.344%
10	6.069	1552	1564	1590	rBV2	111756	232010	46.41%	5.140%
11	6.989	1840	1850	1867	rBV2	47537	89622	17.93%	1.986%
12	7.317	1941	1952	1970	rBV	233409	416103	83.24%	9.219%
13	7.625	2038	2048	2066	rBV2	25835	48067	9.62%	1.065%
14	7.976	2146	2157	2179	rVB2	120094	204273	40.86%	4.526%
15	8.092	2182	2193	2227	rBV	165349	351661	70.35%	7.791%
16	8.850	2419	2429	2451	rBV	253612	413849	82.79%	9.169%
17	10.217	2842	2854	2866	rBV	71898	113885	22.78%	2.523%
18	11.249	3164	3175	3193	rBV	256253	397906	79.60%	8.816%
19	11.622	3278	3291	3309	rBV	212250	339658	67.95%	7.526%




Sum of corrected areas: 4513425

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041122\
Data File : VV025446.D
Acq On : 11 Apr 2022 13:39
Operator : SY/MD
Sample : N2319-11DL 10X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YB2H9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

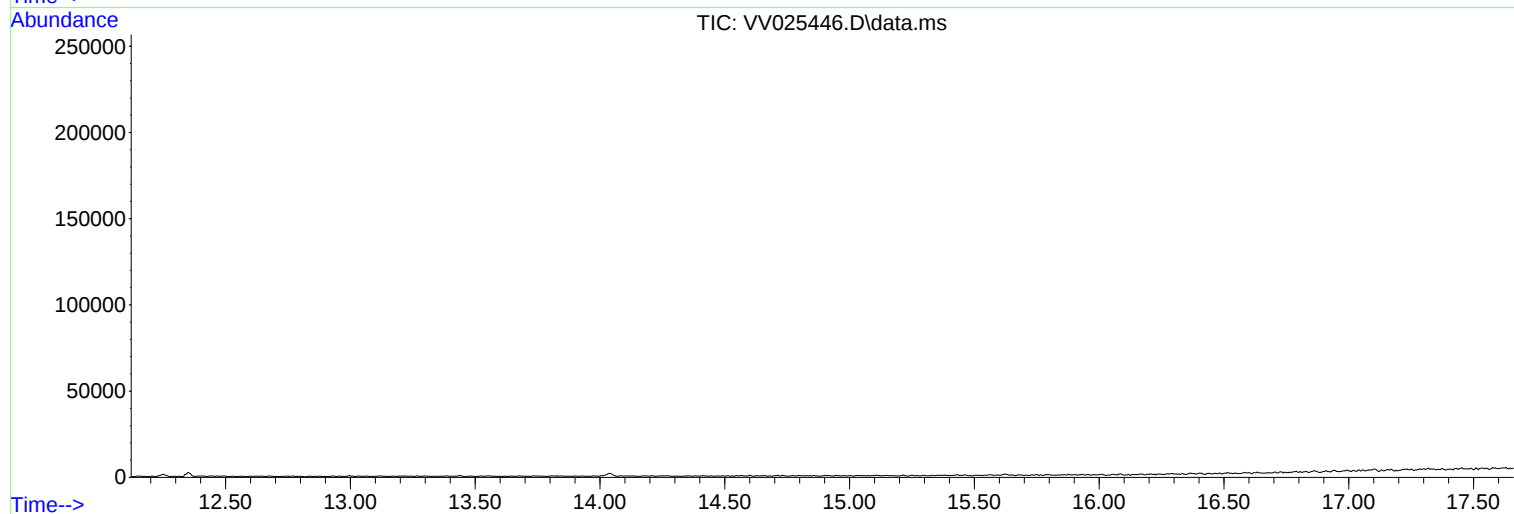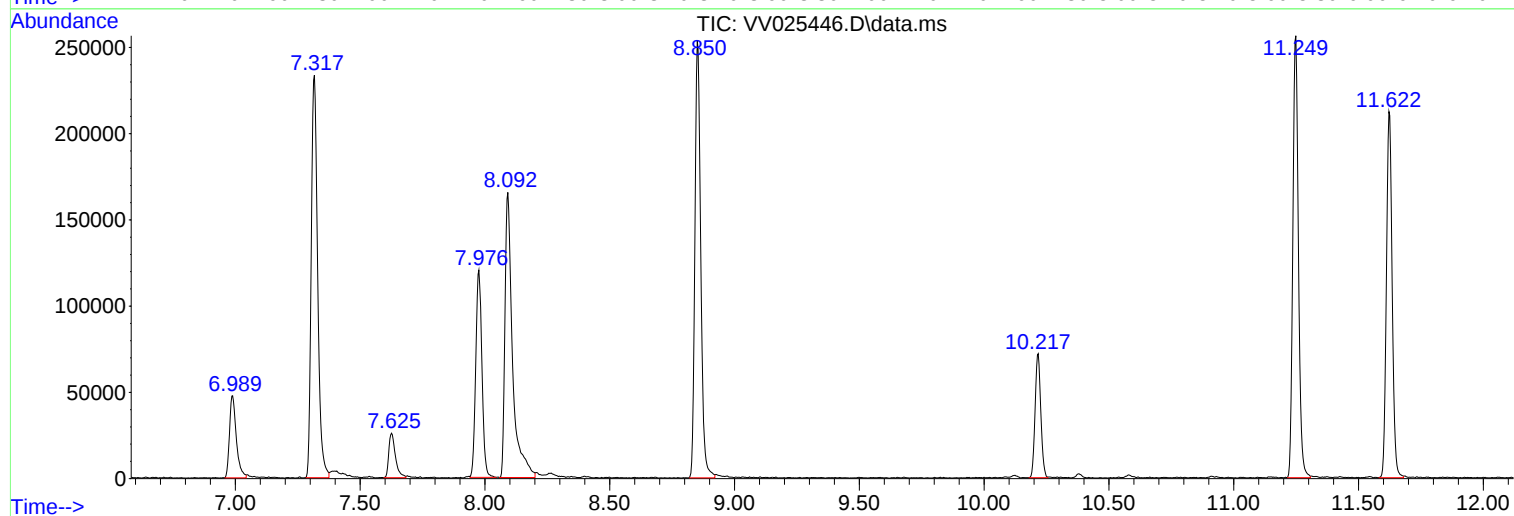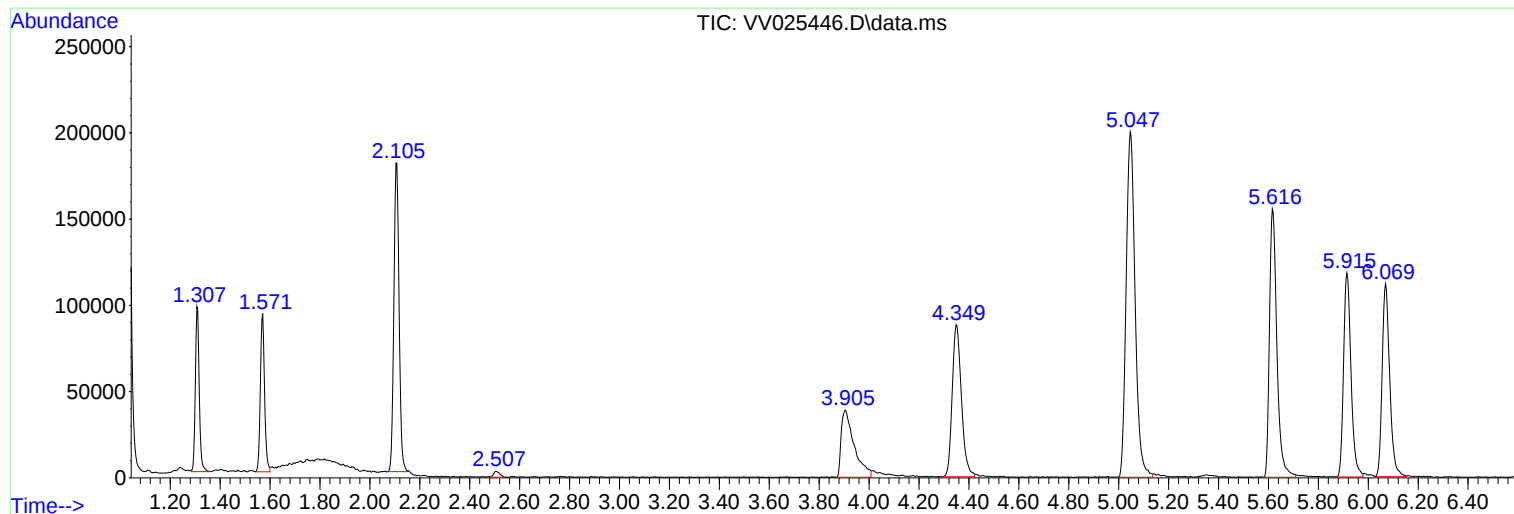

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041122\
Data File : VV025446.D
Acq On : 11 Apr 2022 13:39
Operator : SY/MD
Sample : N2319-11DL 10X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YB2H9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041122\
Data File : VV025446.D
Acq On : 11 Apr 2022 13:39
Operator : SY/MD
Sample : N2319-11DL 10X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YB2H9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc