

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041122\
 Data File : VV025447.D
 Acq On : 11 Apr 2022 14:02
 Operator : SY/MD
 Sample : N2319-08DL 5X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YB2H6DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV025447.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	104	rVB	96894	105425	21.01%	2.313%
2	1.571	157	165	177	rBV	84920	102406	20.41%	2.247%
3	1.754	215	222	232	rBV	13569	19851	3.96%	0.436%
4	2.105	321	331	355	rVB	211549	315269	62.84%	6.917%
5	2.510	445	457	470	rVB4	4525	8154	1.63%	0.179%
6	3.912	881	893	938	rBV2	33030	143794	28.66%	3.155%
7	4.349	1012	1029	1060	rBV	88248	230673	45.98%	5.061%
8	5.047	1231	1246	1274	rBV3	202069	501673	100.00%	11.007%
9	5.616	1412	1423	1458	rBV	156238	327806	65.34%	7.192%
10	5.915	1503	1516	1533	rBV	154987	308936	61.58%	6.778%
11	6.069	1552	1564	1589	rVB	111571	227686	45.39%	4.996%
12	6.989	1837	1850	1868	rBV2	48650	91417	18.22%	2.006%
13	7.317	1941	1952	1972	rBV	237903	419471	83.61%	9.203%
14	7.625	2037	2048	2064	rBV3	25636	48239	9.62%	1.058%
15	7.976	2146	2157	2172	rVB2	35754	62395	12.44%	1.369%
16	8.095	2181	2194	2226	rBV	155597	355978	70.96%	7.810%
17	8.850	2418	2429	2455	rBV	248562	414939	82.71%	9.104%
18	10.217	2841	2854	2870	rBV	72840	114969	22.92%	2.522%
19	11.249	3160	3175	3195	rBV	265380	410635	81.85%	9.010%
20	11.622	3279	3291	3307	rBV	217678	348079	69.38%	7.637%




Sum of corrected areas: 4557795

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041122\
Data File : VV025447.D
Acq On : 11 Apr 2022 14:02
Operator : SY/MD
Sample : N2319-08DL 5X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YB2H6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

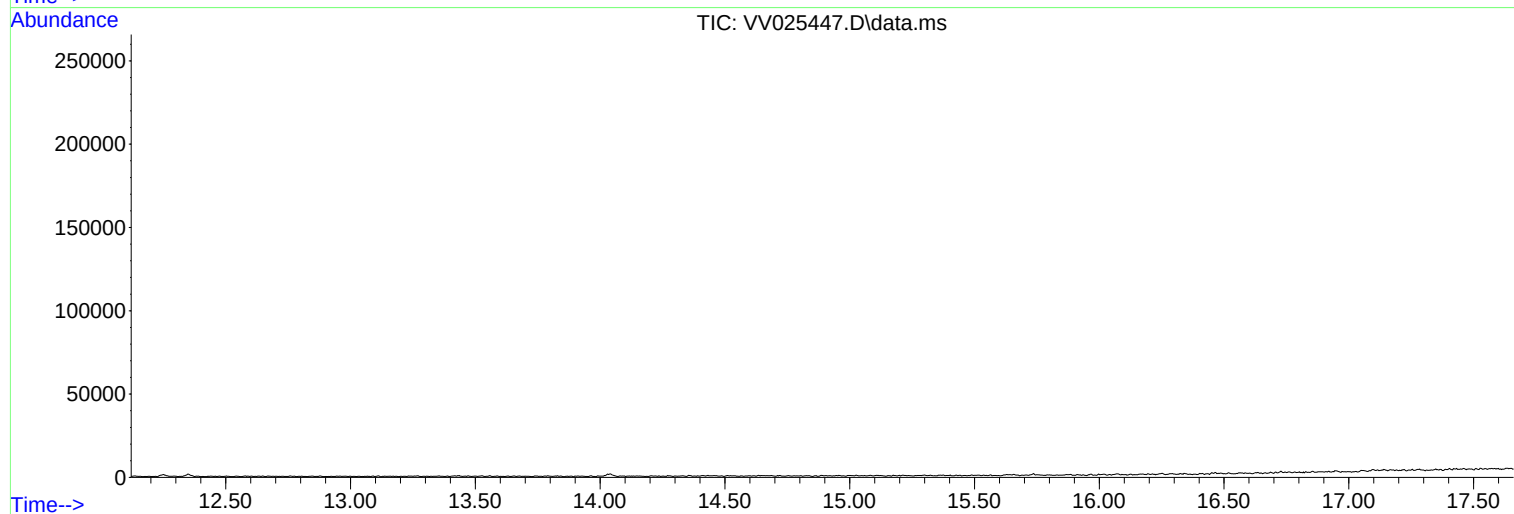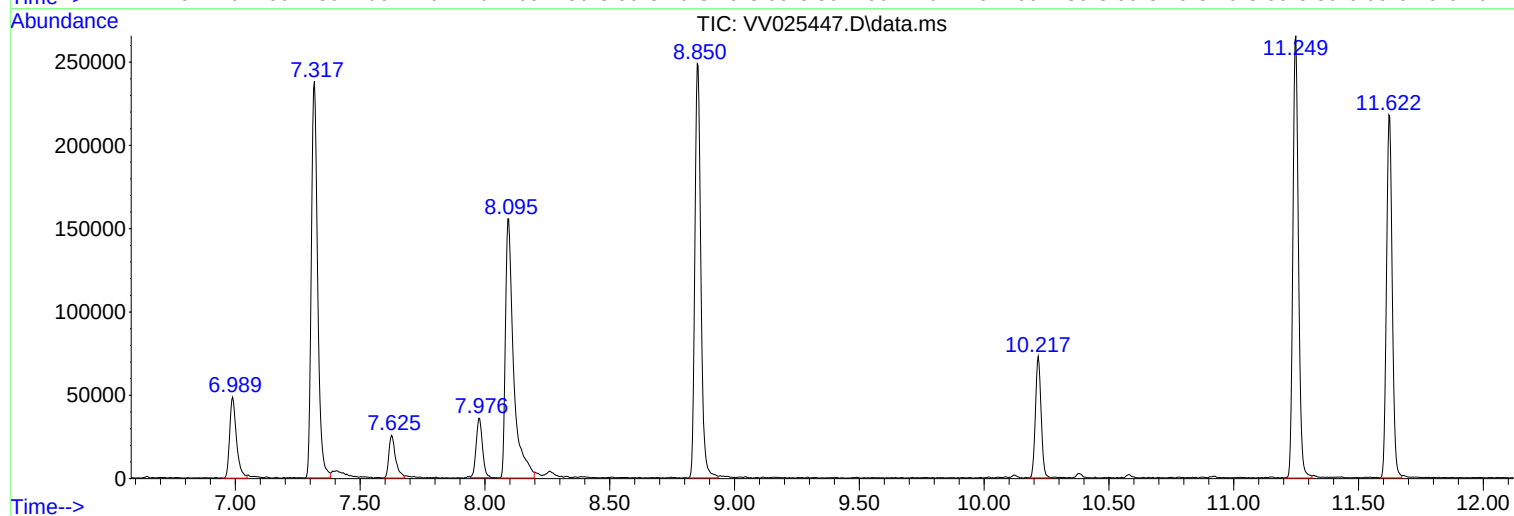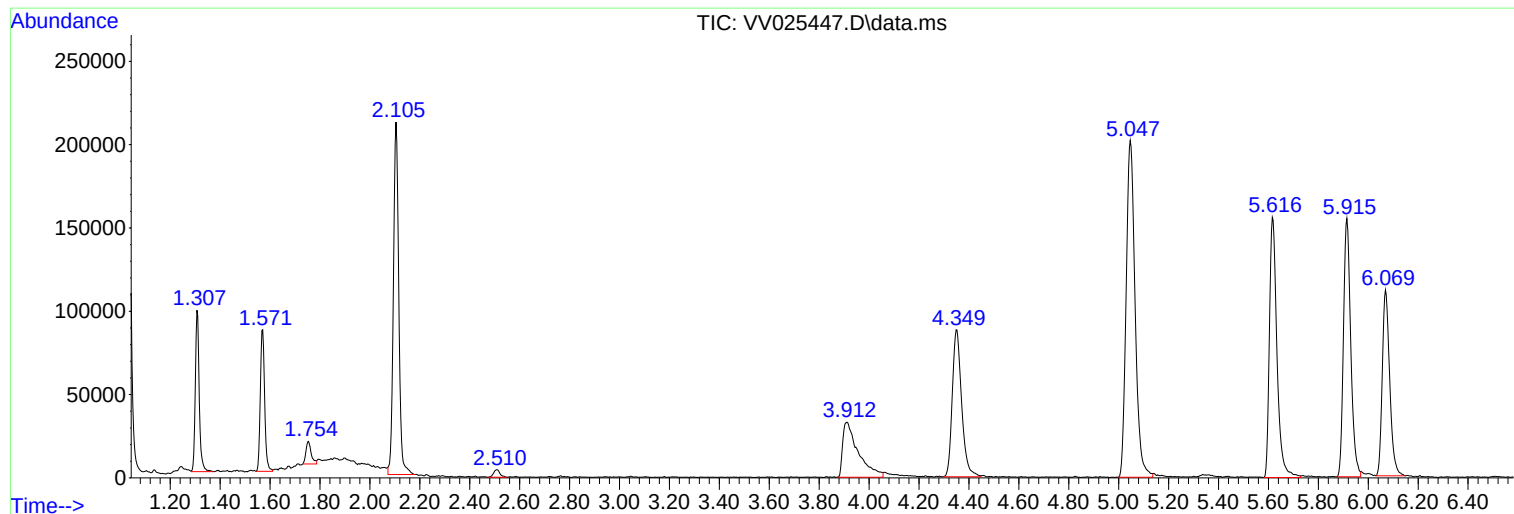

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041122\
Data File : VV025447.D
Acq On : 11 Apr 2022 14:02
Operator : SY/MD
Sample : N2319-08DL 5X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YB2H6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041122\
Data File : VV025447.D
Acq On : 11 Apr 2022 14:02
Operator : SY/MD
Sample : N2319-08DL 5X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YB2H6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc