

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041122\
 Data File : VV025448.D
 Acq On : 11 Apr 2022 14:25
 Operator : SY/MD
 Sample : N2319-05DL 5X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YB2H2DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV025448.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	98	rVB	99271	102246	17.03%	2.188%
2	1.571	157	165	175	rBV	92293	105054	17.49%	2.248%
3	1.754	217	222	231	rVB	5967	7491	1.25%	0.160%
4	2.111	320	333	345	rBV	176833	258977	43.12%	5.542%
5	3.902	878	890	922	rBV	39194	140025	23.32%	2.997%
6	4.352	1012	1030	1057	rBV	89675	229092	38.15%	4.903%
7	5.050	1231	1247	1275	rBV2	194590	488579	81.35%	10.456%
8	5.619	1409	1424	1445	rBV	153202	317705	52.90%	6.799%
9	5.915	1501	1516	1543	rBV	300334	600556	100.00%	12.852%
10	6.069	1551	1564	1589	rVB	109734	229758	38.26%	4.917%
11	6.989	1838	1850	1873	rBV2	46207	90492	15.07%	1.937%
12	7.317	1939	1952	1971	rBV	233868	410488	68.35%	8.785%
13	7.625	2039	2048	2063	rBV2	25380	45612	7.59%	0.976%
14	7.976	2148	2157	2172	rVB3	31241	53512	8.91%	1.145%
15	8.088	2179	2192	2226	rBV	164237	336802	56.08%	7.208%
16	8.850	2417	2429	2452	rBV	251079	410834	68.41%	8.792%
17	10.217	2843	2854	2865	rBV	69412	110787	18.45%	2.371%
18	11.249	3164	3175	3196	rBV	253880	393672	65.55%	8.425%
19	11.622	3278	3291	3309	rBV	208763	333323	55.50%	7.133%
20	12.345	3505	3516	3529	rVB6	4873	7711	1.28%	0.165%




Sum of corrected areas: 4672716

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041122\
Data File : VV025448.D
Acq On : 11 Apr 2022 14:25
Operator : SY/MD
Sample : N2319-05DL 5X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YB2H2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

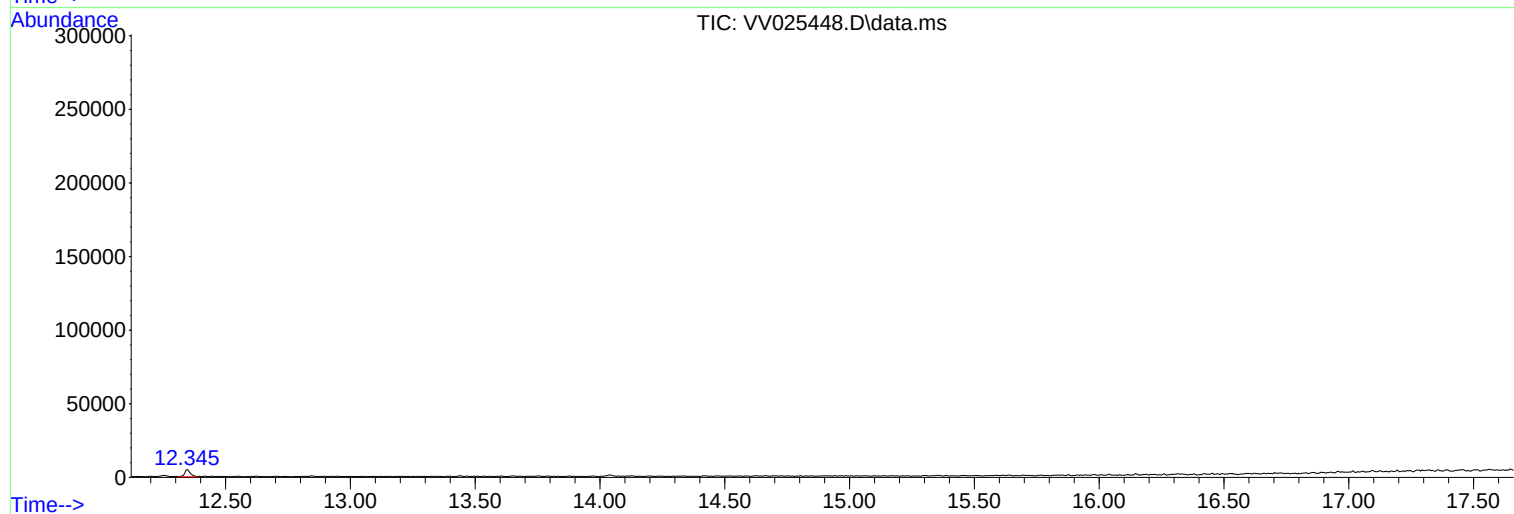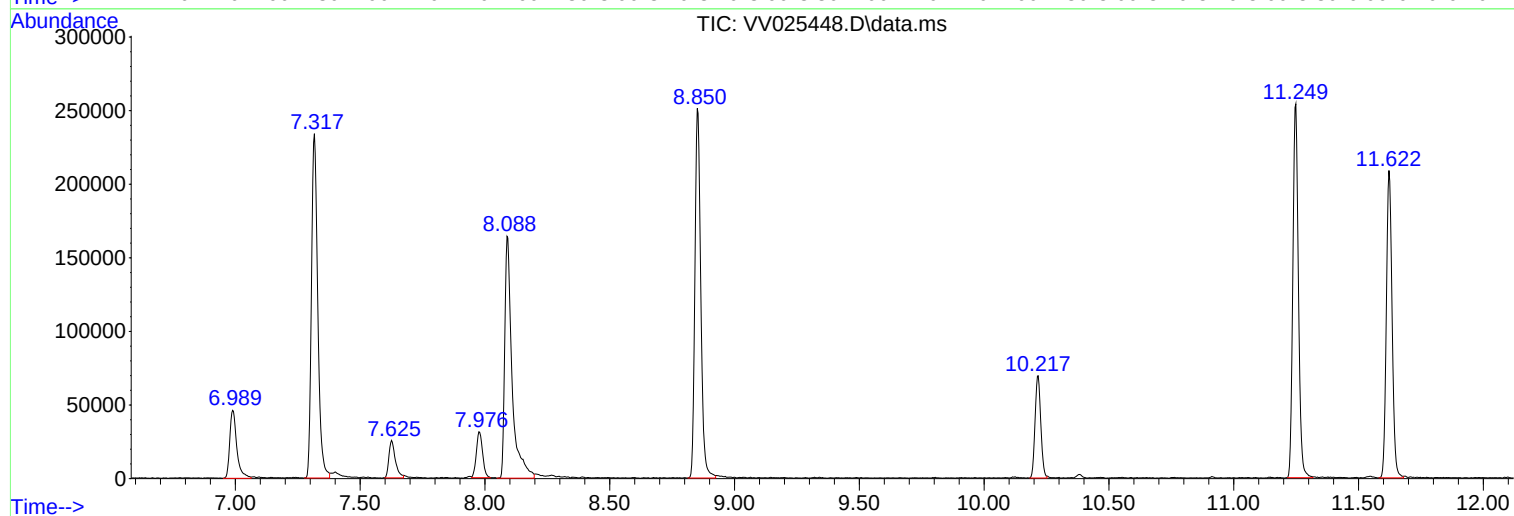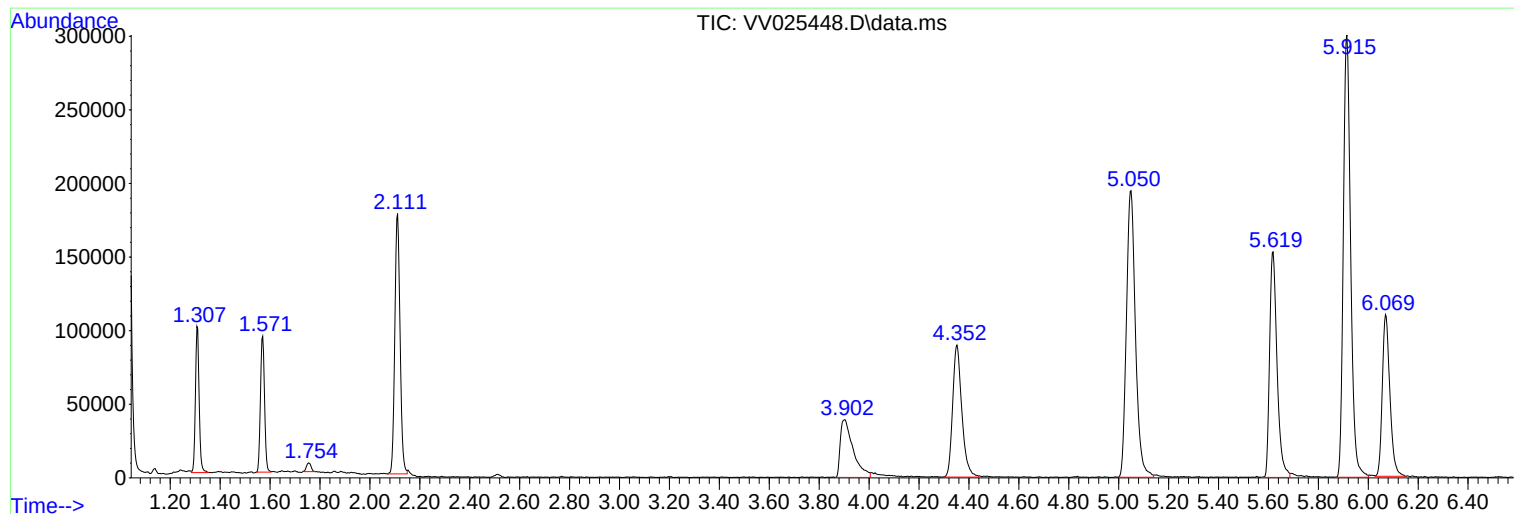

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041122\
Data File : VV025448.D
Acq On : 11 Apr 2022 14:25
Operator : SY/MD
Sample : N2319-05DL 5X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YB2H2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041122\
Data File : VV025448.D
Acq On : 11 Apr 2022 14:25
Operator : SY/MD
Sample : N2319-05DL 5X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YB2H2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc