

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041122\
 Data File : VV025450.D
 Acq On : 11 Apr 2022 15:12
 Operator : SY/MD
 Sample : N2319-07 100X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YB2H4

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV025450.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	96	rVB	99278	100948	20.97%	2.555%
2	1.568	156	164	173	rBV	88996	102444	21.28%	2.593%
3	2.108	321	332	350	rVB	175807	261023	54.22%	6.607%
4	2.510	447	457	466	rBV2	2935	4949	1.03%	0.125%
5	3.905	881	891	931	rBV	34529	134512	27.94%	3.405%
6	4.352	1012	1030	1052	rBV	85736	216636	45.00%	5.484%
7	5.050	1231	1247	1279	rBV3	192251	481457	100.00%	12.187%
8	5.619	1412	1424	1444	rBV	144230	295980	61.48%	7.492%
9	5.921	1505	1518	1529	rBV10	10845	26171	5.44%	0.662%
10	6.072	1552	1565	1591	rBV2	106320	223326	46.39%	5.653%
11	6.989	1840	1850	1873	rBV2	45437	85825	17.83%	2.172%
12	7.317	1941	1952	1974	rBV	224682	399176	82.91%	10.104%
13	7.625	2036	2048	2069	rBV2	24837	48993	10.18%	1.240%
14	7.976	2148	2157	2175	rVB2	22187	40528	8.42%	1.026%
15	8.092	2181	2193	2229	rBV	164614	341764	70.99%	8.651%
16	8.850	2416	2429	2456	rBV	233125	387309	80.45%	9.804%
17	10.217	2842	2854	2872	rBV	68232	108233	22.48%	2.740%
18	11.249	3163	3175	3193	rBV	234373	364876	75.79%	9.236%
19	11.622	3276	3291	3309	rBV	206011	326445	67.80%	8.263%




Sum of corrected areas: 3950595

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041122\
Data File : VV025450.D
Acq On : 11 Apr 2022 15:12
Operator : SY/MD
Sample : N2319-07 100X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YB2H4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

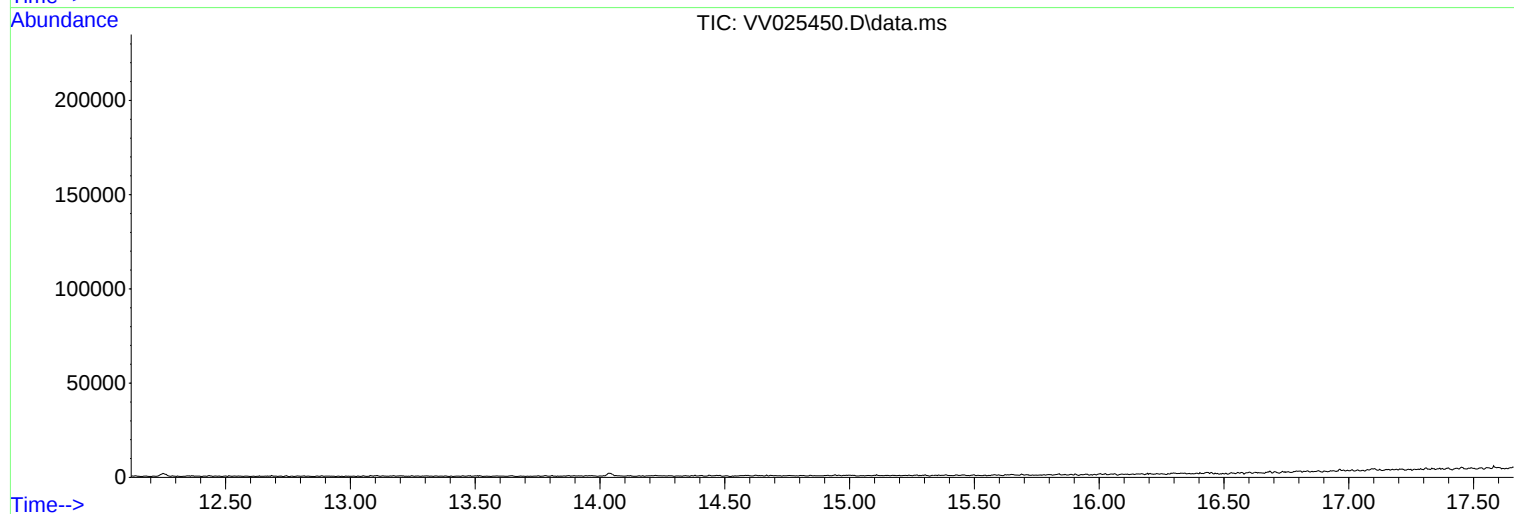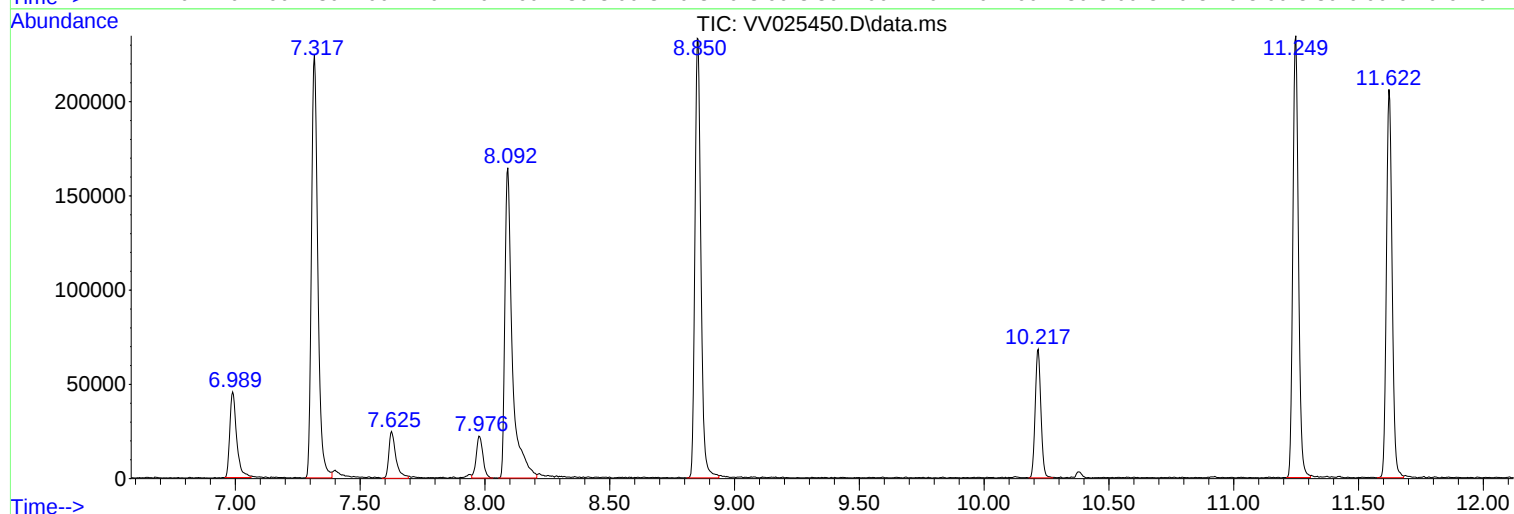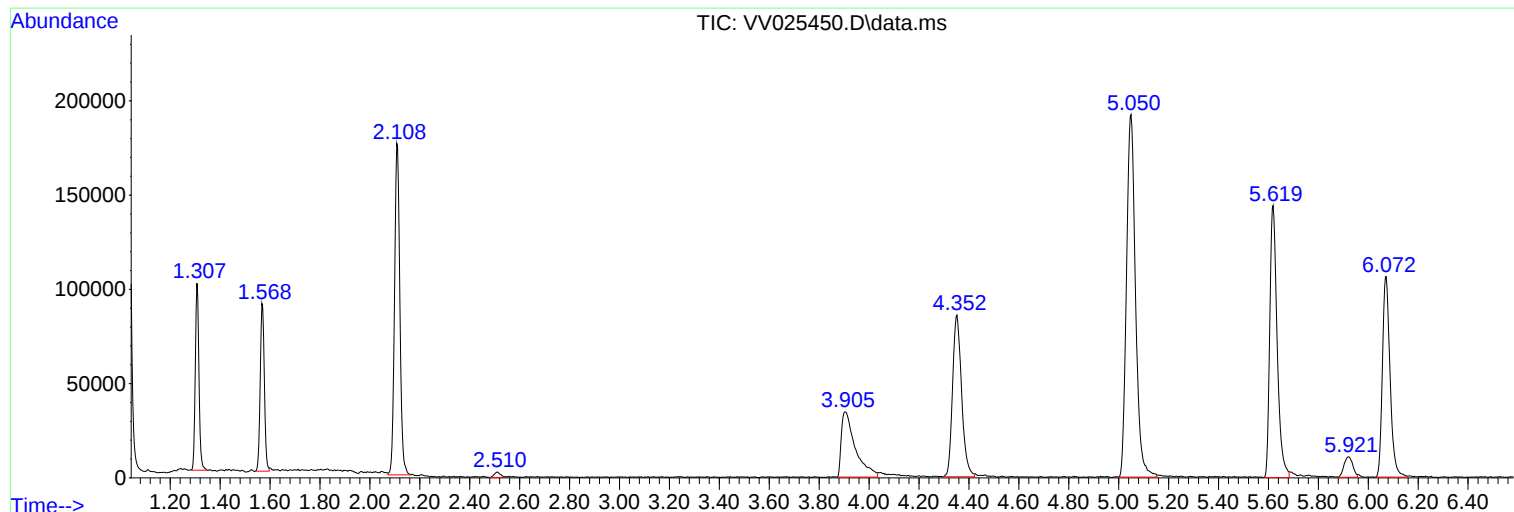

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041122\
Data File : VV025450.D
Acq On : 11 Apr 2022 15:12
Operator : SY/MD
Sample : N2319-07 100X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YB2H4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041122\
Data File : VV025450.D
Acq On : 11 Apr 2022 15:12
Operator : SY/MD
Sample : N2319-07 100X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YB2H4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc