

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041122\
 Data File : VV025458.D
 Acq On : 11 Apr 2022 18:19
 Operator : SY/MD
 Sample : N2357-02
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YAYW2

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV025458.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.310	77	84	95	rVB	94324	93278	20.37%	2.506%
2	1.571	157	165	177	rBV	82996	94898	20.73%	2.550%
3	2.111	323	333	354	rVB	161893	238985	52.20%	6.421%
4	3.905	881	891	927	rBV2	35240	133971	29.26%	3.600%
5	4.352	1015	1030	1056	rBV	80189	203521	44.46%	5.468%
6	5.050	1231	1247	1277	rBV2	181265	457810	100.00%	12.301%
7	5.619	1413	1424	1447	rBV	141177	286613	62.61%	7.701%
8	5.912	1507	1515	1527	rBV7	3825	7129	1.56%	0.192%
9	6.069	1551	1564	1587	rBV	102169	213170	46.56%	5.728%
10	6.989	1840	1850	1868	rBV	43942	81944	17.90%	2.202%
11	7.317	1941	1952	1972	rBV	214999	376286	82.19%	10.110%
12	7.625	2039	2048	2062	rBV3	23464	42420	9.27%	1.140%
13	7.940	2136	2146	2155	rBV2	3075	5779	1.26%	0.155%
14	8.091	2182	2193	2233	rBV	154378	322282	70.40%	8.659%
15	8.854	2419	2430	2452	rBV	227046	374921	81.89%	10.074%
16	10.217	2843	2854	2869	rBV2	64675	104725	22.88%	2.814%
17	10.381	2896	2905	2917	rBV3	6366	10299	2.25%	0.277%
18	11.249	3164	3175	3195	rBV	221686	350865	76.64%	9.427%
19	11.622	3280	3291	3307	rBV	195560	309118	67.52%	8.306%
20	12.345	3509	3516	3525	rBV6	3648	5560	1.21%	0.149%
21	15.403	4459	4467	4476	rVB7	5103	8213	1.79%	0.221%




Sum of corrected areas: 3721787

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041122\
Data File : VV025458.D
Acq On : 11 Apr 2022 18:19
Operator : SY/MD
Sample : N2357-02
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YAYW2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

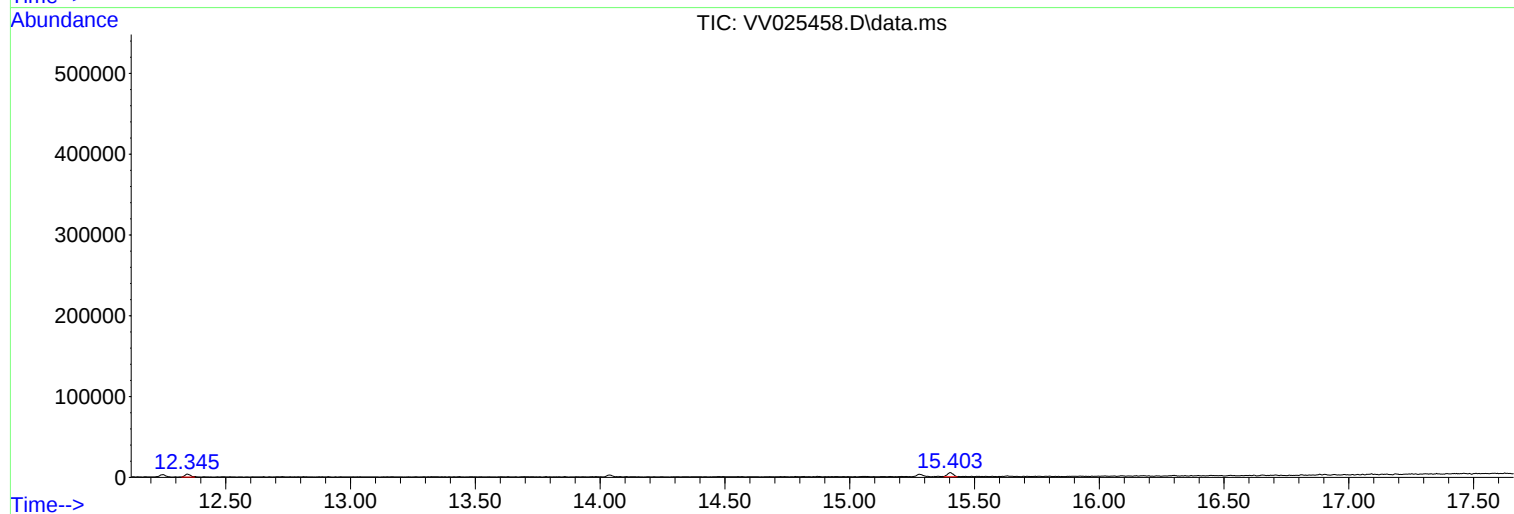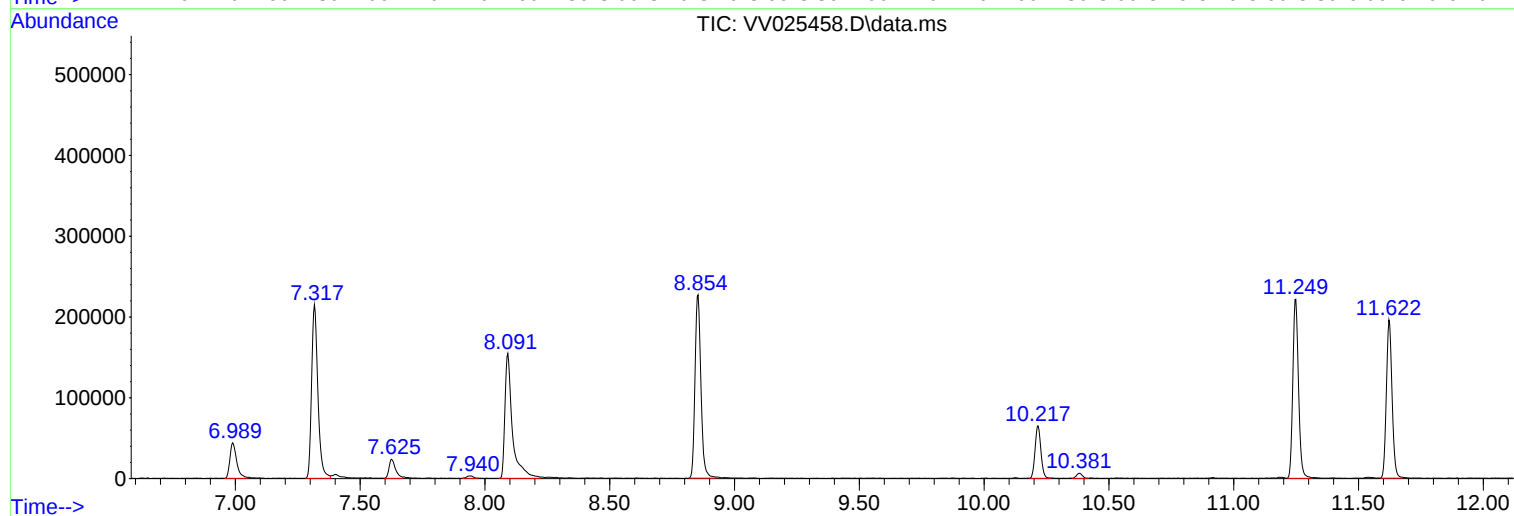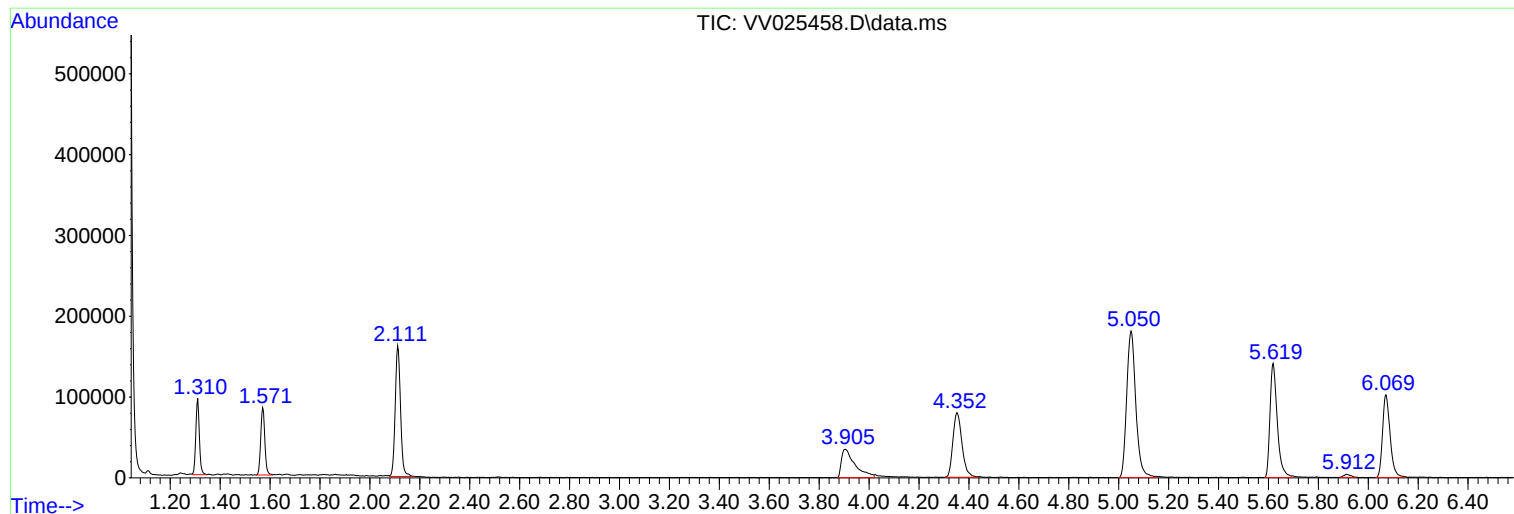

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041122\
Data File : VV025458.D
Acq On : 11 Apr 2022 18:19
Operator : SY/MD
Sample : N2357-02
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YAYW2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041122\
Data File : VV025458.D
Acq On : 11 Apr 2022 18:19
Operator : SY/MD
Sample : N2357-02
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YAYW2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc