


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041122\
 Data File : VV025437.D
 Acq On : 11 Apr 2022 09:02
 Operator : SY/MD
 Sample : BFB299
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB299

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Sat Apr 16 04:36:16 2022

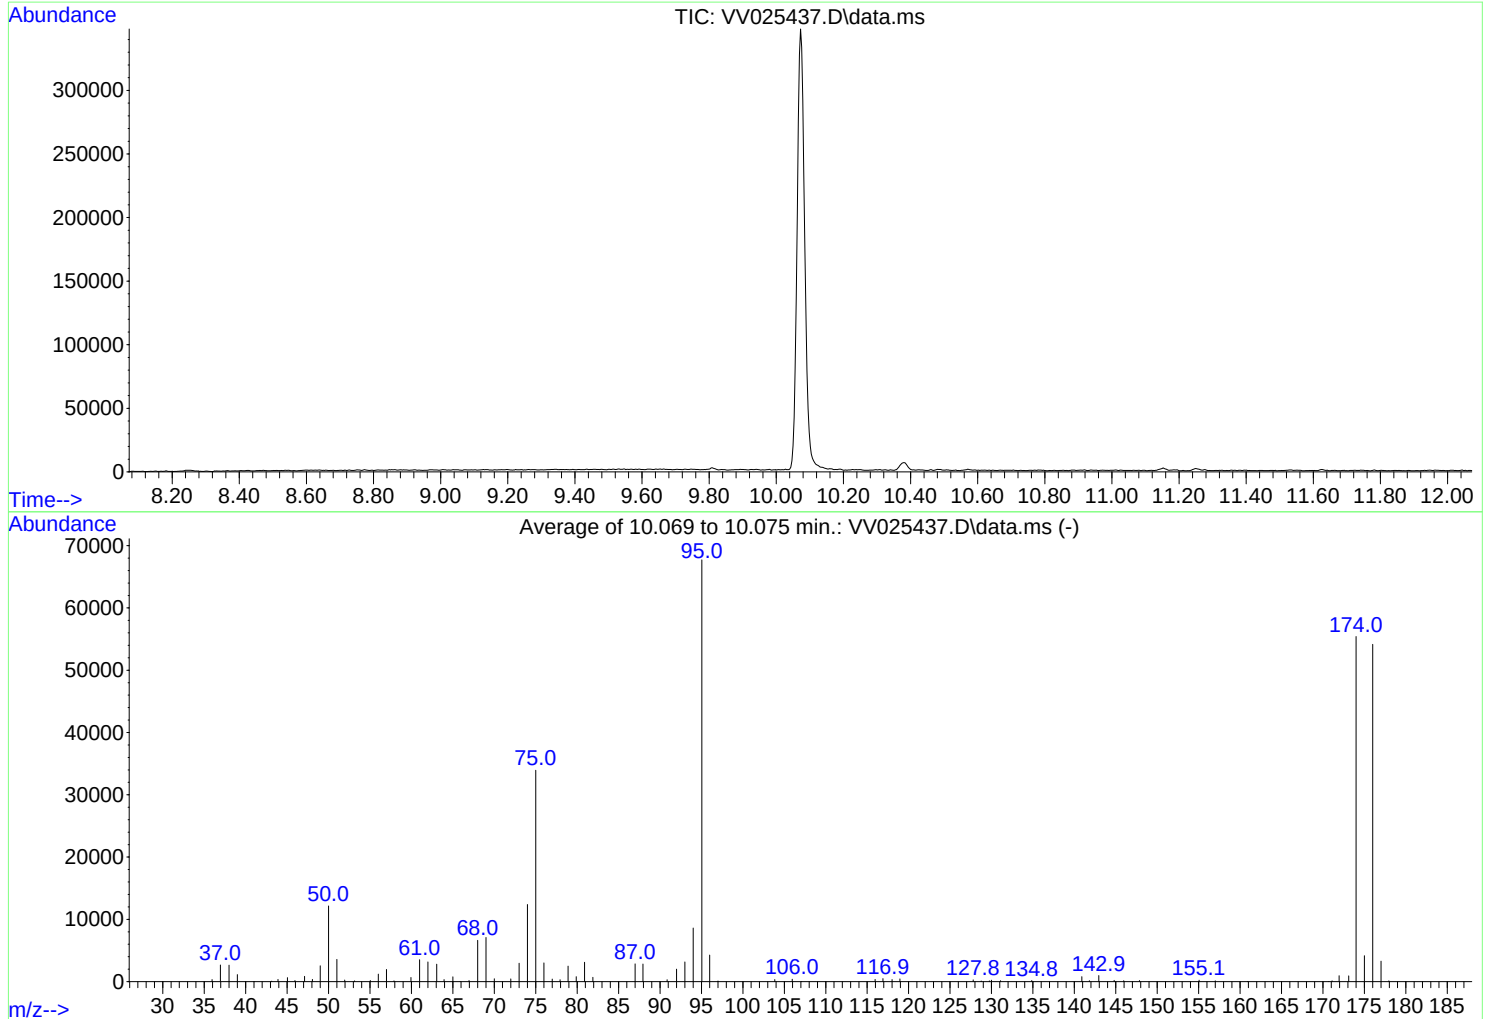

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.9	12143	PASS
75	95	30	80	50.1	33947	PASS
95	95	100	100	100.0	67725	PASS
96	95	5	9	6.3	4276	PASS
173	174	0.00	2	1.7	917	PASS
174	95	50	120	81.8	55416	PASS
175	174	5	9	7.5	4160	PASS
176	174	95	105	97.7	54163	PASS
177	176	5	10	6.1	3303	PASS

m/z	Abundance
36.00	853.0
36.90	146.0
37.90	323.0
40.10	148.0
42.10	115.0
43.90	205.0

Instrument :
MSVOA_V
ClientSampleId :
BFB299

m/z	Abundance
36.00	1225.0
37.00	2690.0
38.00	3031.0
39.00	1156.0
40.00	140.0
43.90	551.0
45.00	632.0
46.00	190.0
47.10	893.0
48.10	290.0
49.00	2485.0
50.00	12024.0
51.00	3615.0
52.00	263.0
53.10	138.0
55.00	193.0
56.00	1097.0
57.00	2015.0
57.90	147.0
60.00	656.0
61.00	3291.0
62.00	3201.0
63.10	2717.0
63.90	319.0
65.00	751.0
65.90	107.0
67.00	167.0
68.00	6705.0
69.00	7085.0
70.00	497.0
72.00	449.0
73.00	2944.0
74.00	12368.0
75.00	33232.0
76.00	2945.0
77.00	418.0
77.90	312.0
78.90	2454.0
79.90	731.0
80.90	3134.0
81.90	622.0
87.00	2850.0
87.90	2966.0
90.90	301.0
92.00	2088.0
93.00	2972.0
94.00	8387.0
95.00	66448.0
96.00	4256.0
97.00	102.0
103.80	336.0
106.00	391.0
115.90	330.0
116.90	485.0
118.00	327.0
119.00	447.0
127.80	291.0
128.70	123.0
129.70	202.0
130.10	195.0
131.10	146.0
134.80	159.0
140.90	845.0
141.80	107.0
142.90	928.0
144.80	201.0
145.90	137.0
147.90	158.0
155.00	247.0
157.00	125.0
160.90	104.0
170.70	109.0
171.10	126.0
171.90	975.0
173.10	842.0
174.00	52936.0
175.00	4014.0
176.00	51120.0
177.00	3349.0
177.90	137.0

Instrument :
MSVOA_V
ClientSampleId :
BFB299

m/z	Abundance
36.00	1212.0
37.00	2909.0
38.00	3065.0
39.00	1145.0
40.00	136.0
43.10	110.0
44.00	583.0
45.10	659.0
46.00	199.0
47.10	888.0
48.00	365.0
49.00	2651.0
50.00	12652.0
51.00	3670.0
51.90	285.0
53.10	137.0
55.10	175.0
56.00	1252.0
57.00	1995.0
57.90	139.0
59.90	665.0
61.00	3664.0
62.00	3290.0
63.10	2869.0
63.90	338.0
65.00	806.0
67.00	165.0
68.00	6807.0
69.00	7316.0
70.00	456.0
72.00	452.0
73.00	3036.0
74.00	12829.0
75.00	35184.0
76.00	3136.0
77.00	439.0
77.90	341.0
78.90	2600.0
79.90	831.0
80.90	3175.0
81.90	700.0
87.00	2893.0
88.00	2901.0
90.90	325.0
92.00	2074.0
93.00	3301.0
94.00	8859.0
95.00	70040.0
96.00	4362.0
97.00	104.0
103.90	341.0
106.00	385.0
107.10	103.0
115.90	378.0
116.90	524.0
118.00	342.0
119.00	454.0
127.80	303.0
128.80	100.0
129.80	219.0
130.00	220.0
131.10	160.0
134.90	184.0
140.90	861.0
141.80	180.0
143.00	1038.0
144.80	221.0
146.00	167.0
147.80	195.0
155.00	238.0
157.00	152.0
171.10	148.0
171.90	997.0
173.10	982.0
174.00	57048.0
175.00	4269.0
176.00	56320.0
177.00	3414.0
178.00	122.0

Instrument :
MSVOA_V
ClientSampleId :
BFB299

m/z	Abundance
35.90	1148.0
37.00	2883.0
38.10	2851.0
39.00	1126.0
39.90	150.0
41.00	101.0
43.20	120.0
44.00	601.0
45.00	621.0
45.90	166.0
47.10	776.0
48.00	409.0
49.00	2512.0
50.00	11753.0
51.00	3446.0
51.90	251.0
53.20	106.0
55.00	185.0
56.00	1289.0
57.00	1864.0
57.90	101.0
59.90	660.0
61.00	3596.0
62.00	3035.0
63.00	2792.0
64.00	317.0
65.00	772.0
66.90	176.0
68.00	6376.0
69.00	6846.0
70.00	408.0
72.00	404.0
73.00	2862.0
74.00	11929.0
75.00	33424.0
76.00	2947.0
77.00	414.0
78.00	312.0
78.90	2453.0
79.90	850.0
80.90	3031.0
81.90	729.0
87.00	2785.0
88.00	2648.0
90.80	329.0
92.00	1878.0
93.00	3212.0
94.00	8571.0
95.10	66688.0
96.00	4210.0
97.00	105.0
103.90	308.0
105.90	365.0
116.00	396.0
116.90	482.0
118.00	313.0
118.90	429.0
127.80	261.0
128.80	105.0
129.90	263.0
131.10	127.0
134.90	196.0
140.90	728.0
141.80	174.0
143.00	991.0
144.80	190.0
145.90	158.0
147.80	197.0
155.10	188.0
157.00	123.0
171.10	115.0
172.00	889.0
173.10	926.0
174.00	56264.0
175.00	4198.0
176.00	55048.0
177.00	3146.0
178.00	116.0

Instrument :
MSVOA_V
ClientSampleId :
BFB299