
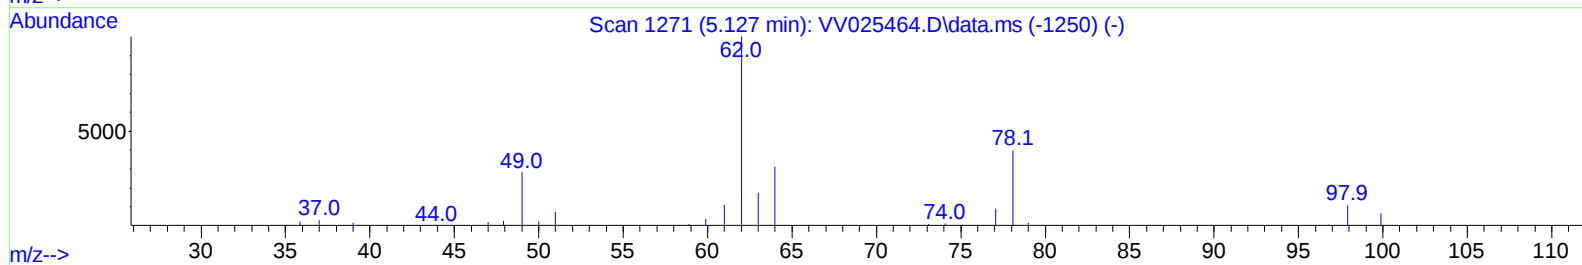
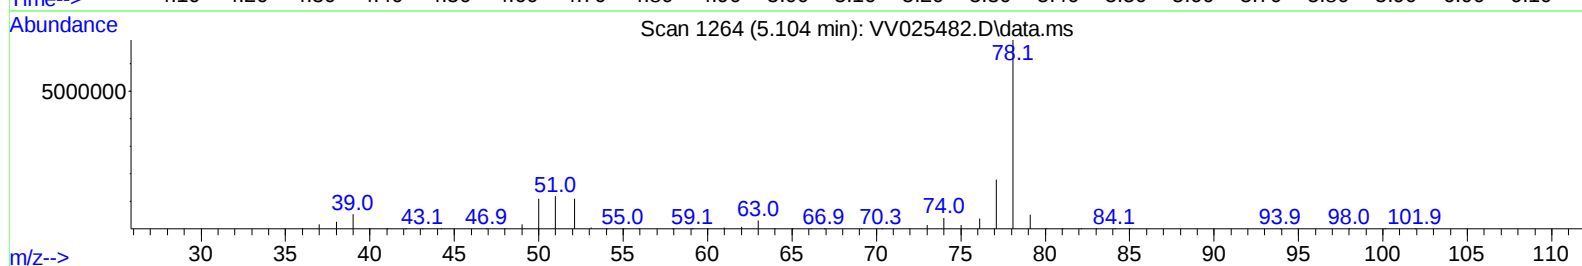


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041222\
 Data File : VV025482.D
 Acq On : 12 Apr 2022 18:16
 Operator : SY/MD
 Sample : N2356-08
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Quant Time: Apr 13 02:35:48 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Apr 13 02:31:13 2022
 Response via : Initial Calibration

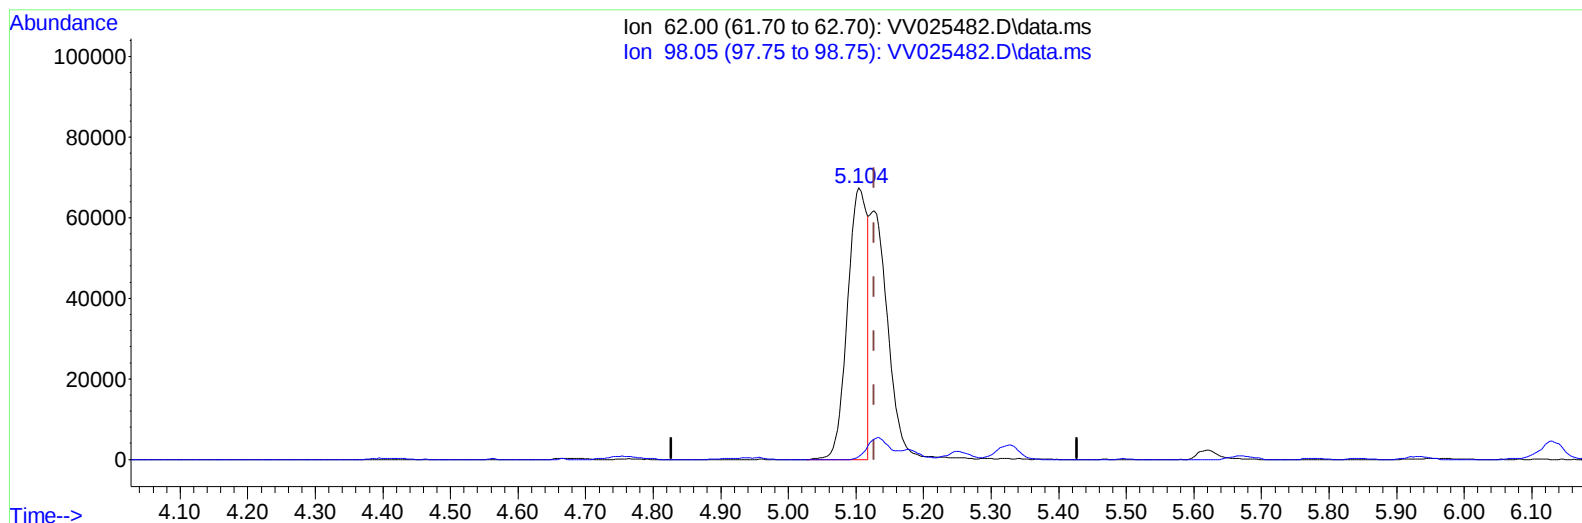

TIC: VV025482.D\data.ms

(27) 1,2-Dichloroethane (T)




5.104min (-0.023) 14.42 ug/L

response 134440

Ion	Exp%	Act%
62.00	100.00	100.00
98.05	11.00	1.10#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041222\
Data File : VV025482.D
Acq On : 12 Apr 2022 18:16
Operator : SY/MD
Sample : N2356-08
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Quant Time: Apr 13 02:35:48 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Apr 13 02:31:13 2022
Response via : Initial Calibration

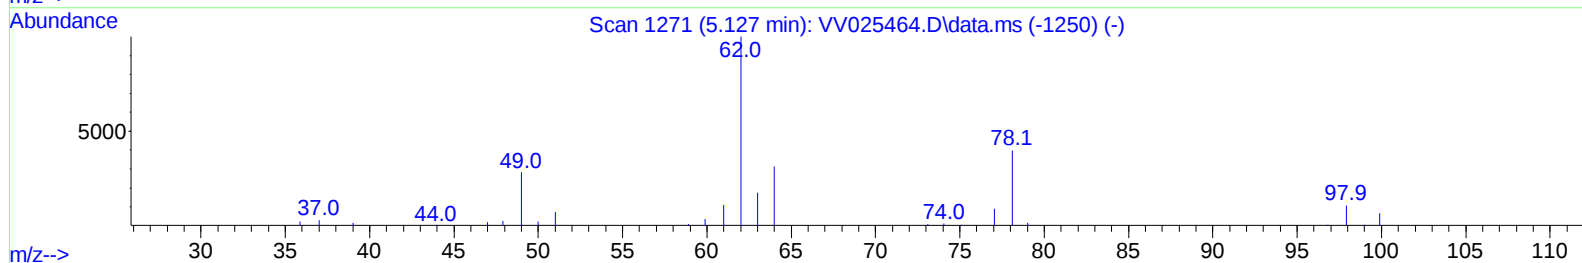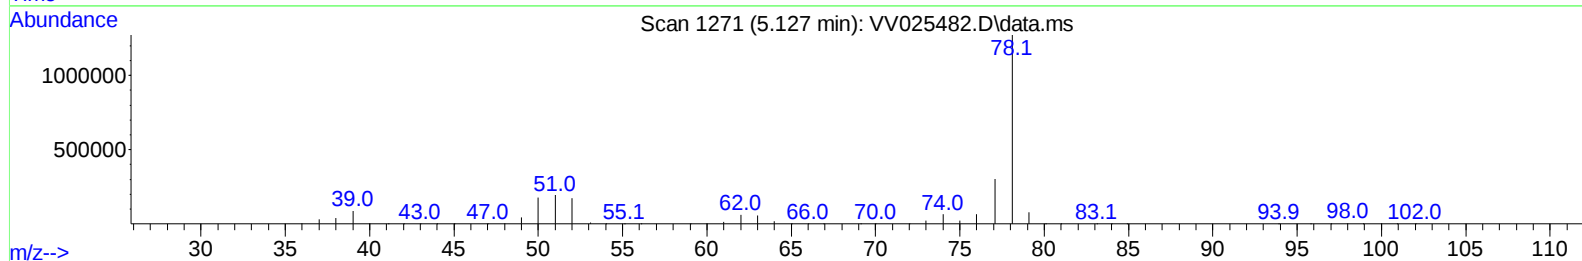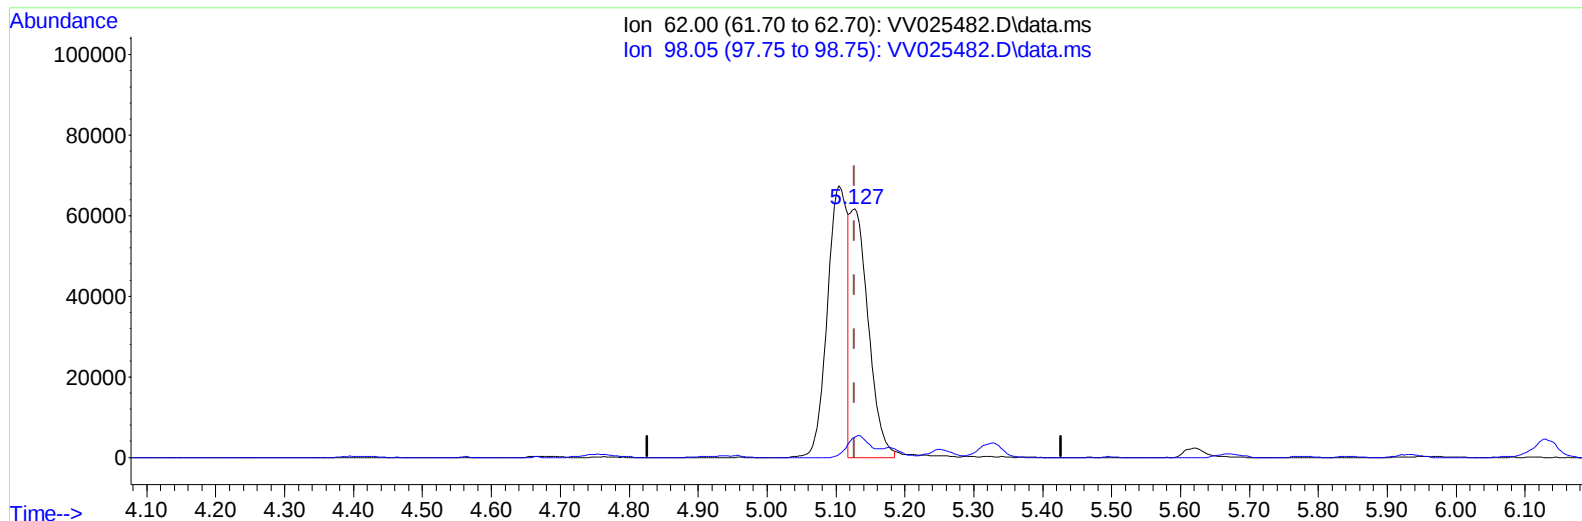

TIC: VV025482.D\data.ms

(27) 1,2-Dichloroethane (T)

5.127min (-0.000) 12.37 ug/L m

response 115366

Ion	Exp%	Act%
62.00	100.00	100.00
98.05	11.00	8.24#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041222\
 Data File : VV025482.D
 Acq On : 12 Apr 2022 18:16
 Operator : SY/MD
 Sample : N2356-08
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Quant Time: Apr 13 02:35:48 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Apr 13 02:31:13 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	135991	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	134394	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	68402	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	56018	4.431	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130	Recovery	=	88.600%	
7) Chloroethane-d5	1.571	69	49641	3.691	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130	Recovery	=	73.800%	
11) 1,1-Dichloroethene-d2	2.111	63	80787	3.190	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125	Recovery	=	63.800%	
20) 2-Butanone-d5	3.905	46	78940	51.329	ug/L	0.02
Spiked Amount 50.000	Range 40	- 130	Recovery	=	102.660%	
24) Chloroform-d	4.352	84	86426	4.524	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	90.400%	
26) 1,2-Dichloroethane-d4	5.037	65	40076	4.868	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	97.400%	
32) Benzene-d6	5.053	84	175719	4.519	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	90.400%	
36) 1,2-Dichloropropane-d6	6.069	67	54097	4.988	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140	Recovery	=	99.800%	
41) Toluene-d8	7.317	98	147446	4.086	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	81.800%	
43) trans-1,3-Dichloroprop...	7.625	79	13747	3.771	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130	Recovery	=	75.400%	
46) 2-Hexanone-d5	8.088	63	60064	46.951	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130	Recovery	=	93.900%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	33711	4.920	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120	Recovery	=	98.400%	
66) 1,2-Dichlorobenzene-d4	11.622	152	53554	4.670	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120	Recovery	=	93.400%	
Target Compounds						
					Qvalue	
8) Chloroethane	1.587	64	2713	0.233	ug/L	99
13) Acetone	2.204	43	4428	4.242	ug/L	90
22) cis-1,2-Dichloroethene	3.921	96	3193	0.307	ug/L	94
27) 1,2-Dichloroethane	5.127	62	114268m	12.256	ug/L	
30) Cyclohexane	4.680	56	190319	13.206	ug/L	98
33) Benzene	5.101	78	14813767	373.149	ug/L	100
35) Methylcyclohexane	6.127	83	22971	1.366	ug/L	94
42) Toluene	7.391	91	52189	1.209	ug/L	96
52) Ethylbenzene	9.014	91	20121	0.437	ug/L	99
53) m,p-Xylene	9.140	106	33060	1.888	ug/L	100
60) Isopropylbenzene	9.931	105	56590	1.337	ug/L	98
63) 1,2,4-Trimethylbenzene	10.914	105	8913	0.262	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041222\
Data File : VV025482.D
Acq On : 12 Apr 2022 18:16
Operator : SY/MD
Sample : N2356-08
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Quant Time: Apr 13 02:35:48 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Apr 13 02:31:13 2022
Response via : Initial Calibration

