




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041222\
 Data File : VV025484.D
 Acq On : 12 Apr 2022 19:03
 Operator : SY/MD
 Sample : N2356-10
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBDS8

Manual IntegrationsAPPROVED

Quant Time: Apr 13 02:36:27 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Apr 13 02:31:13 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 04/13/2022
 Supervised By :Mahesh Dadoda 04/13/2022

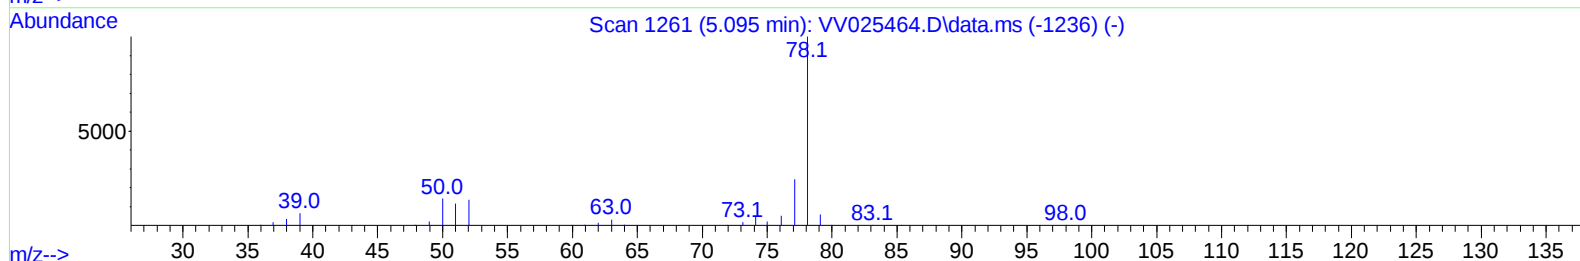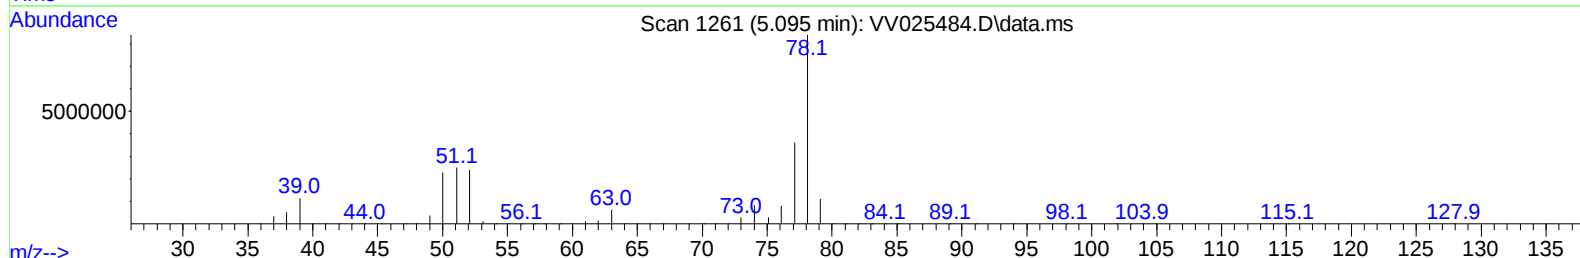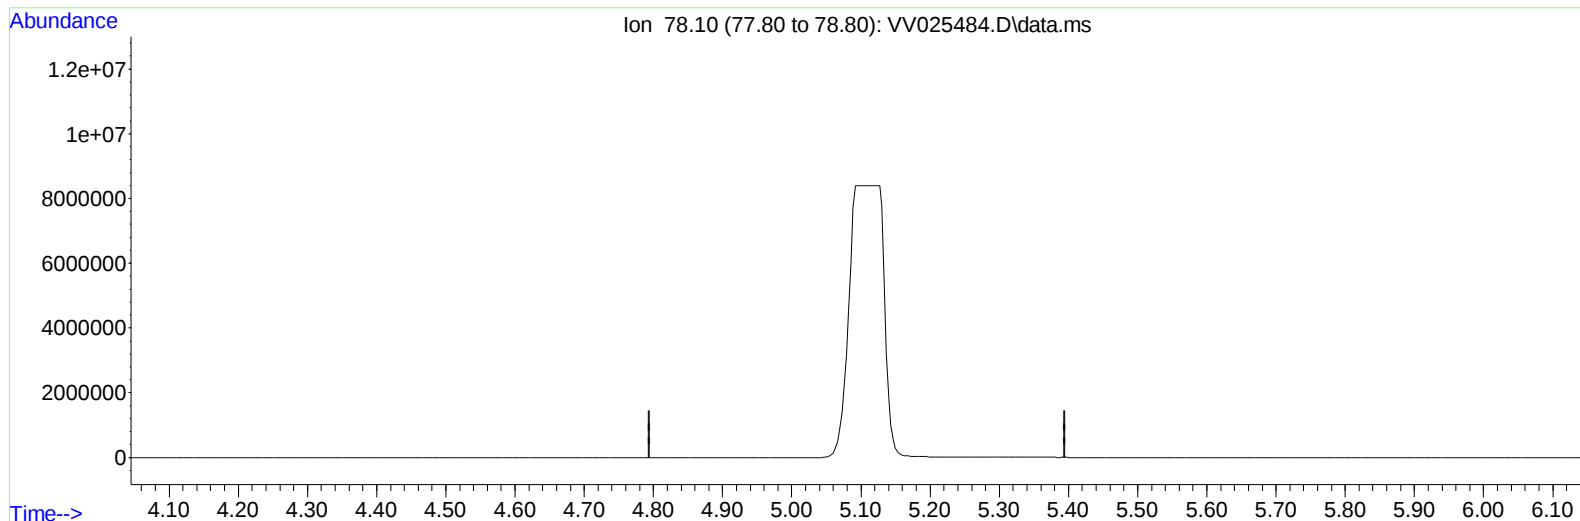

TIC: VV025484.D\data.ms

(33) Benzene (T)

5.095min (-5.095) 0.00 ug/L

response 0

Ion	Exp%	Act%
78.10	100.00	0.00
0.00	0.00	0.00
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041222\
 Data File : VV025484.D
 Acq On : 12 Apr 2022 19:03
 Operator : SY/MD
 Sample : N2356-10
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBDS8

Manual IntegrationsAPPROVED

Quant Time: Apr 13 02:36:27 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Apr 13 02:31:13 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 04/13/2022
 Supervised By :Mahesh Dadoda 04/13/2022

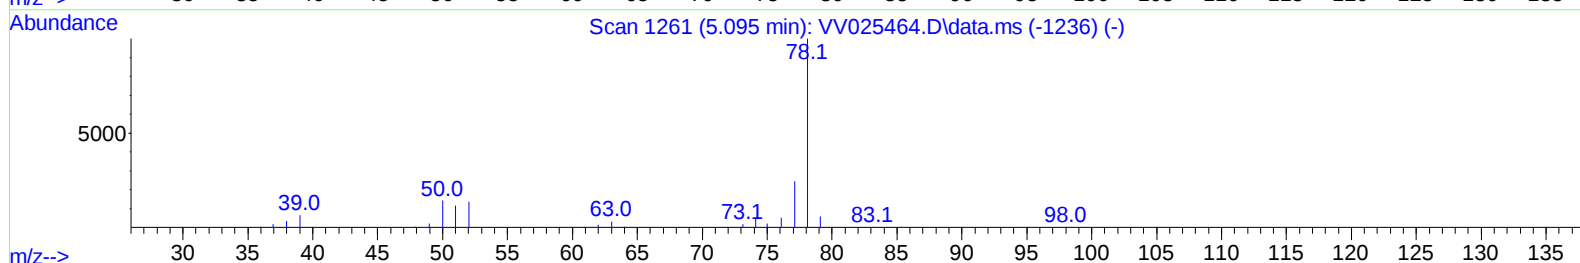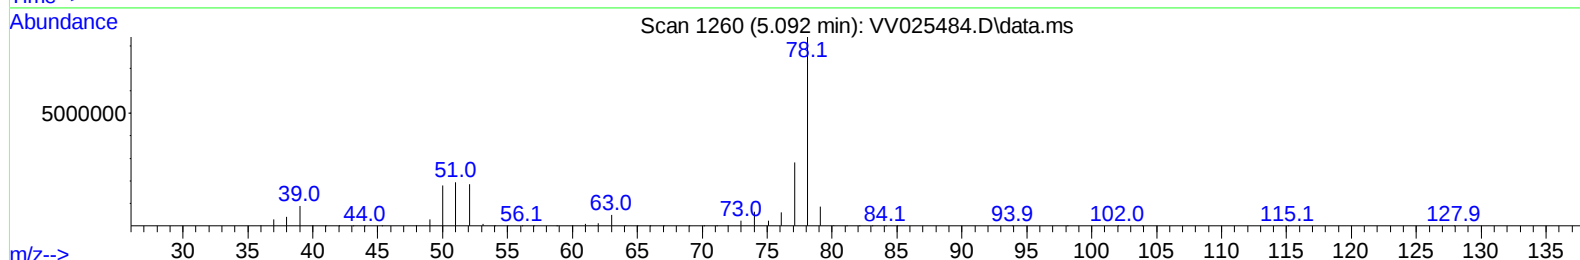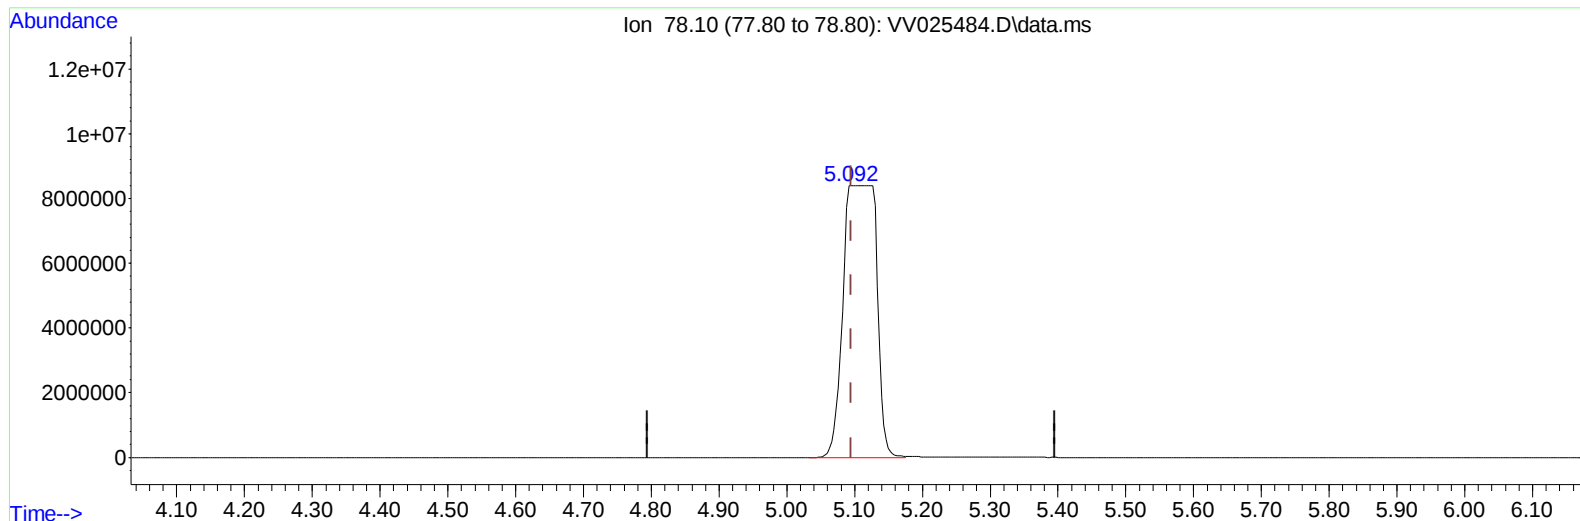

TIC: VV025484.D\data.ms

(33) Benzene (T)

5.092min (-0.003) 628.03 ug/L m

response 28551758

Ion	Exp%	Act%
78.10	100.00	100.00
0.00	0.00	0.00
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041222\
 Data File : VV025484.D
 Acq On : 12 Apr 2022 19:03
 Operator : SY/MD
 Sample : N2356-10
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBDS8

Manual IntegrationsAPPROVED

Quant Time: Apr 13 02:36:27 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Apr 13 02:31:13 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 04/13/2022
 Supervised By :Mahesh Dadoda 04/13/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	155977	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	153903	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	80411	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	76497	5.275	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130	Recovery	=	105.600%	
7) Chloroethane-d5	1.571	69	55332	3.587	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130	Recovery	=	71.800%	
11) 1,1-Dichloroethene-d2	2.111	63	89439	3.079	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125	Recovery	=	61.600%	
20) 2-Butanone-d5	3.905	46	91369	51.798	ug/L	0.02
Spiked Amount 50.000	Range 40	- 130	Recovery	=	103.600%	
24) Chloroform-d	4.352	84	95421	4.355	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	87.000%	
26) 1,2-Dichloroethane-d4	5.043	65	44440	4.707	ug/L	0.01
Spiked Amount 5.000	Range 70	- 130	Recovery	=	94.200%	
32) Benzene-d6	5.056	84	197491	4.435	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	88.800%	
36) 1,2-Dichloropropane-d6	6.072	67	57889	4.661	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140	Recovery	=	93.200%	
41) Toluene-d8	7.317	98	176159	4.263	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	85.200%	
43) trans-1,3-Dichloroprop...	7.625	79	16494	3.951	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130	Recovery	=	79.000%	
46) 2-Hexanone-d5	8.088	63	77626	52.987	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130	Recovery	=	105.980%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	39183	4.994	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120	Recovery	=	99.800%	
66) 1,2-Dichlorobenzene-d4	11.622	152	63165	4.685	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120	Recovery	=	93.800%	
Target Compounds						
					Qvalue	
5) vinyl chloride	1.310	62	39308	2.272	ug/L	98
8) Chloroethane	1.587	64	5916	0.443	ug/L	97
18) trans-1,2-Dichloroethene	2.767	96	5110	0.451	ug/L	92
22) cis-1,2-Dichloroethene	3.912	96	438840	36.770	ug/L #	93
25) Chloroform	4.407	83	17583	0.868	ug/L #	1
27) 1,2-Dichloroethane	5.114	62	752202	70.341	ug/L #	73
30) Cyclohexane	4.680	56	1169996	70.894	ug/L	96
33) Benzene	5.092	78	28551758m	628.033	ug/L	
34) Trichloroethene	5.918	95	11646	0.965	ug/L	95
35) Methylcyclohexane	6.130	83	237924	12.353	ug/L #	71
42) Toluene	7.387	91	305265	6.173	ug/L	98
52) Ethylbenzene	9.011	91	304979	5.782	ug/L	98
53) m,p-Xylene	9.136	106	295540	14.737	ug/L	95
54) o-Xylene	9.545	106	9613	0.494	ug/L	98
60) Isopropylbenzene	9.931	105	444764	8.936	ug/L	100
63) 1,2,4-Trimethylbenzene	10.915	105	16516	0.413	ug/L	98

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041222\
 Data File : VV025484.D
 Acq On : 12 Apr 2022 19:03
 Operator : SY/MD
 Sample : N2356-10
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBDS8

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 04/13/2022
 Supervised By :Mahesh Dadoda 04/13/2022

Quant Time: Apr 13 02:36:27 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Apr 13 02:31:13 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev	(Min)

(#) = qualifier out of range (m) = manual integration (+) = signals summed								

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041222\
Data File : VV025484.D
Acq On : 12 Apr 2022 19:03
Operator : SY/MD
Sample : N2356-10
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBDS8

Manual IntegrationsAPPROVED

Quant Time: Apr 13 02:36:27 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Apr 13 02:31:13 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 04/13/2022
Supervised By :Mahesh Dadoda 04/13/2022

